
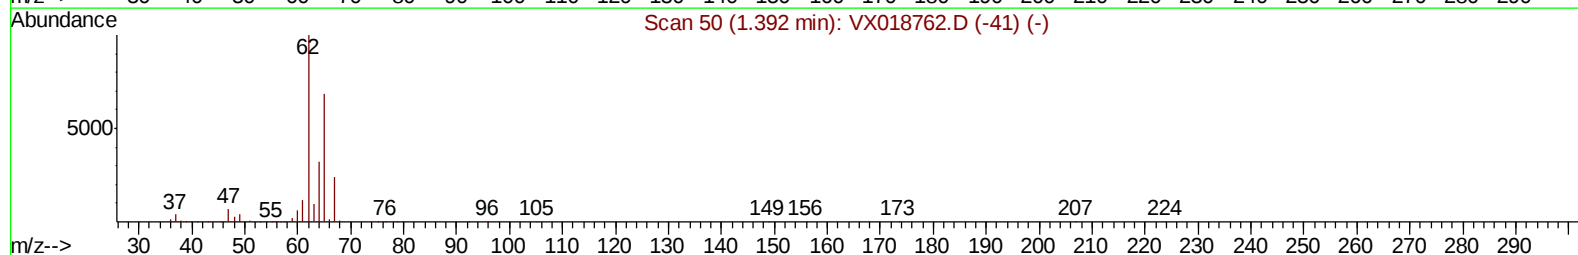
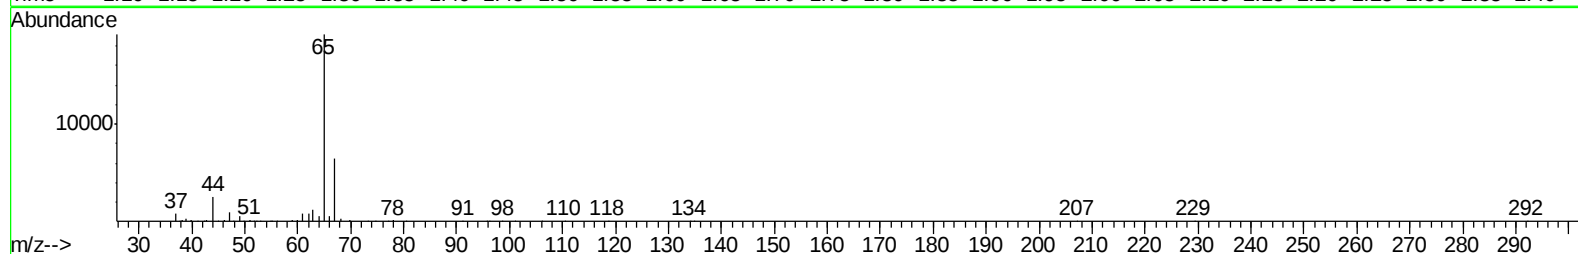


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100520\
 Data File : VX018770.D
 Acq On : 05 Oct 2020 17:03
 Operator : JC/SP
 Sample : L4239-05DL2 400X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 06 05:03:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 06 02:55:01 2020
 Response via : Initial Calibration

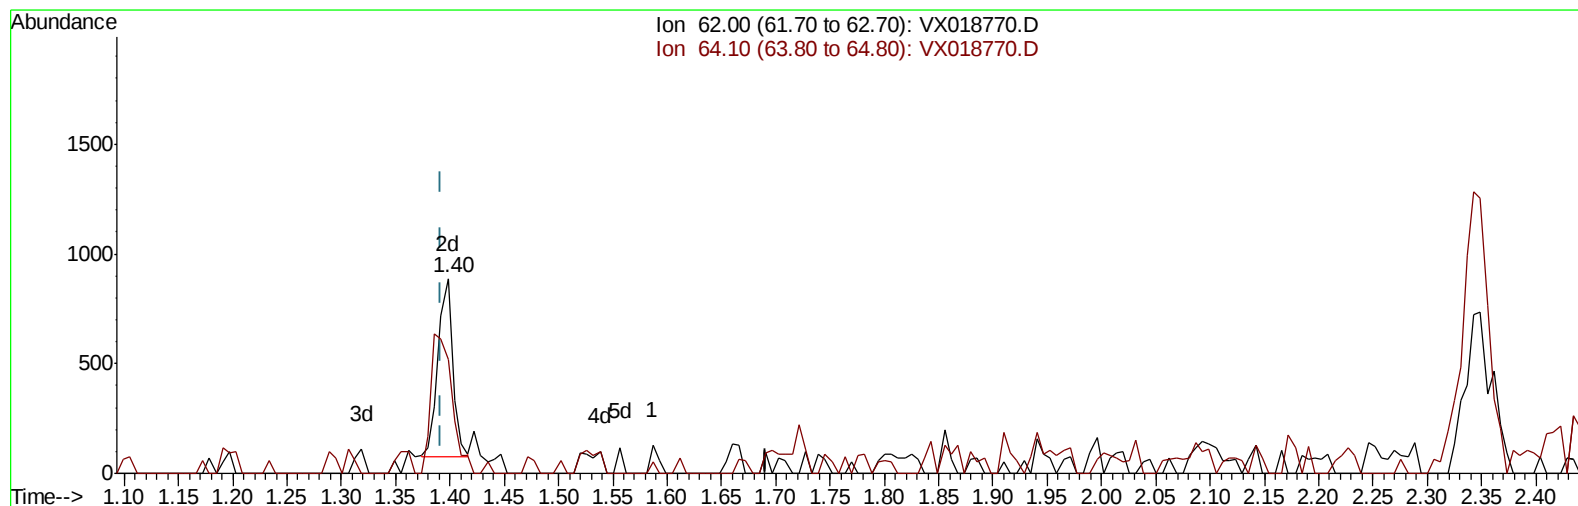

TIC: VX018770.D

(5) Vinyl chloride (T)

1.398min (+0.006) 0.10ug/L m

response 750

Ion	Exp%	Act%
62.00	100	100
64.10	34.70	58.74#
0.00	0.00	0.00
0.00	0.00	0.00