

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100520\
 Data File : VX018781.D
 Acq On : 05 Oct 2020 22:09
 Operator : JC/SP
 Sample : L4240-02 40X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3Q9

Quant Time: Oct 06 06:06:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 06 05:58:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	129393	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	123291	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	59317	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	39278	5.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.80%
7) Chloroethane-d5	1.70	69	34667	5.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.20%
11) 1,1-Dichloroethene-d2	2.34	63	66883	3.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.40%
20) 2-Butanone-d5	4.56	46	137550	69.38	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	138.76%#
24) Chloroform-d	5.14	84	99592	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.00%
26) 1,2-Dichloroethane-d4	6.03	65	57894	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	6.05	84	180416	5.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	117.80%
36) 1,2-Dichloropropane-d6	7.37	67	55659	6.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	125.60%
41) Toluene-d8	8.70	98	157611	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
45) trans-1,3-Dichloropropene-	8.99	79	23984	5.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.60%
48) 2-Hexanone-d5	9.43	63	108505	67.94	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	135.88%#
59) 1,1,2,2-Tetrachloroethane-	11.23	84	43583	6.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	121.00%#
65) 1,2-Dichlorobenzene-d4	12.36	152	63177	5.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.39	62	365	0.052	ug/L #	1
12) 1,1-Dichloroethene	2.34	96	931	0.144	ug/L #	1
15) Methyl Acetate	2.82	43	7050	2.650	ug/L #	48
16) Methylene chloride	2.84	84	3929	0.503	ug/L	87
22) cis-1,2-Dichloroethene	4.57	96	383	0.054	ug/L #	63
29) 1,1,1-Trichloroethane	5.46	97	1766	0.121	ug/L	90
30) Cyclohexane	5.54	56	9080	0.898	ug/L	96
35) Methylcyclohexane	7.37	83	14222	1.317	ug/L #	19
37) 1,2-Dichloropropane	7.37	63	6994	1.081	ug/L #	83
39) cis-1,3-Dichloropropene	8.37	75	1947	0.189	ug/L #	60
42) Toluene	8.76	91	52400	1.855	ug/L	99
43) 1,3,5-Trimethylbenzene	11.49	105	7887	0.295	ug/L	94
44) 1,2,4-Trimethylbenzene	11.79	105	25081	0.924	ug/L	100
50) 2-Hexanone	9.43	43	14637	5.378	ug/L #	71
54) Ethylbenzene	10.24	91	4741	0.150	ug/L	94
55) m,p-xylene	10.34	106	6420	0.520	ug/L	99
56) o-xylene	10.68	106	2387	0.209	ug/L	80


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100520\
Data File : VX018781.D
Acq On : 05 Oct 2020 22:09
Operator : JC/SP
Sample : L4240-02 40X
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG3Q9

Quant Time: Oct 06 06:06:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 06 05:58:52 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
63) 1,3-Dichlorobenzene	12.01	146	1205	0.084	ug/L	99
64) 1,4-Dichlorobenzene	12.09	146	4111	0.286	ug/L	95
66) 1,2-Dichlorobenzene	12.38	146	1363	0.101	ug/L	92
69) 1,2,4-trichlorobenzene	13.63	180	8678	0.942	ug/L	96
70) Naphthalene	13.82	128	1472	0.098	ug/L #	86
71) 1,2,3-Trichlorobenzene	14.00	180	3353	0.404	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

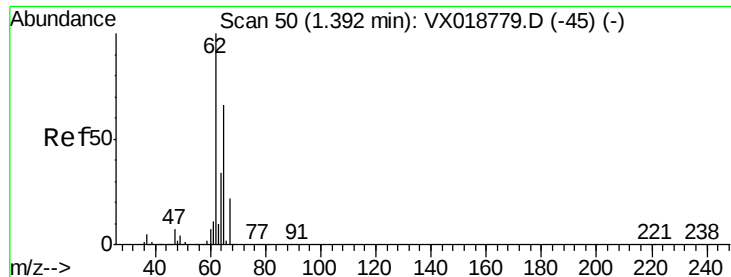

#5

Vinyl chloride

Concen: 0.052 ug/L

RT: 1.39 min Scan# 49

Delta R.T. -0.01 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09

Instrument :

MSVOA_X

ClientSampleId :





BG3Q9

Tot Ion: 62 Resp: 365

Ion Ratio Lower Upper

62 100

64 179.5 24.3 45.1#

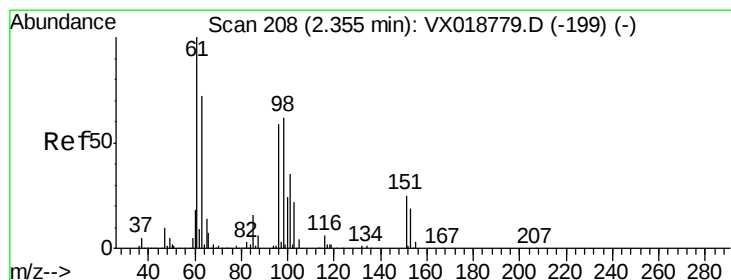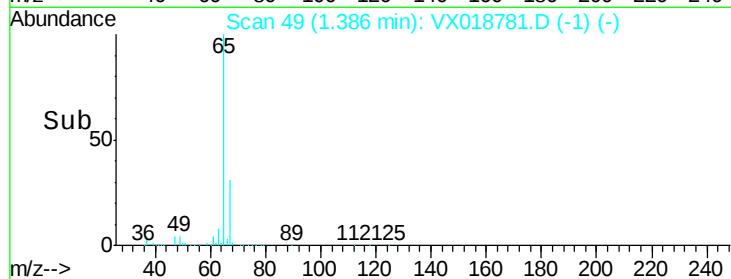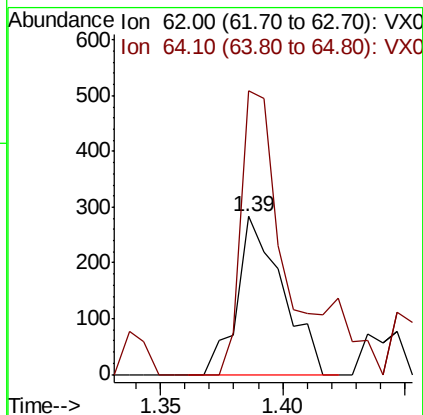

#12

1,1-Dichloroethene

Concen: 0.144 ug/L

RT: 2.34 min Scan# 205

Delta R.T. -0.02 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09




Tgt Ion: 96 Resp: 931


Ion Ratio Lower Upper

96 100

61 774.7 133.2 247.4#

63 5686.5 115.1 213.7#


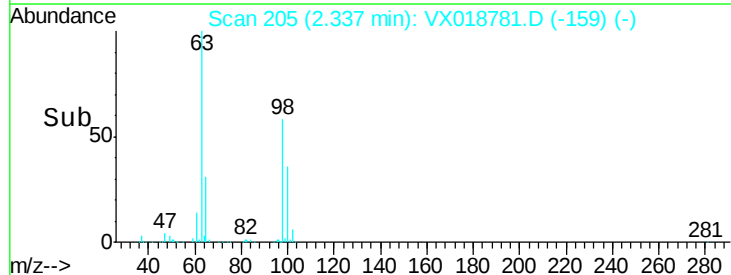
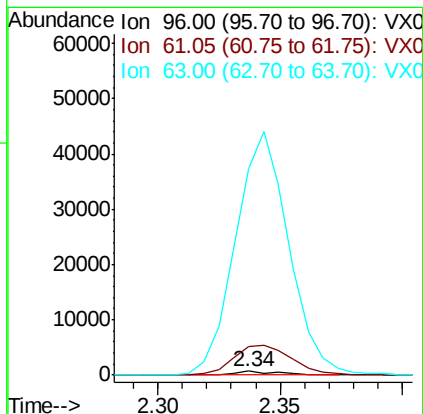





#15
Methyl Acetate
Concen: 2.650 ug/L
RT: 2.82 min Scan# 284
Delta R.T. 0.05 min
Lab File: VX018781.D
Acq: 05 Oct 2020 22:09




Instrument :
MSVOA_X
ClientSampled :
BG3Q9


Tot Ion: 43 Resp: 7050
Ion Ratio Lower Upper
43 100
74 0.3 21.9 32.9#

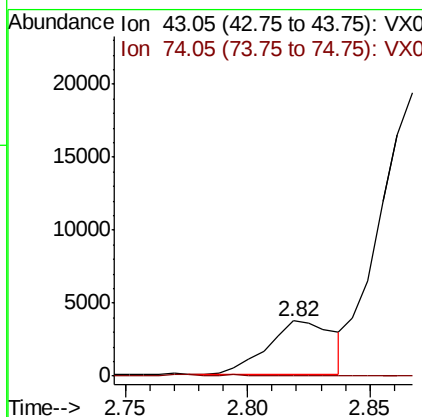

#16
Methylene chloride
Concen: 0.503 ug/L
RT: 2.84 min Scan# 287
Delta R.T. 0.01 min
Lab File: VX018781.D
Acq: 05 Oct 2020 22:09

Tgt Ion: 84 Resp: 3929
Ion Ratio Lower Upper
84 100
86 79.5 45.6 84.8
49 110.2 85.8 159.3

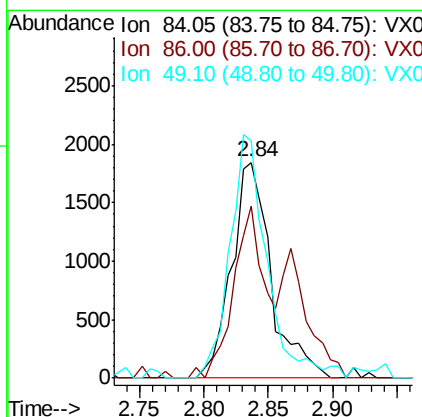




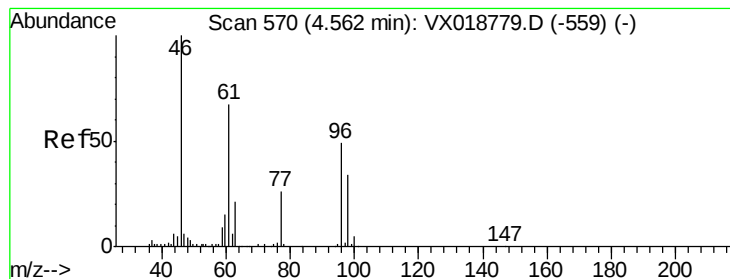


#22

cis-1,2-Dichloroethene
 Concen: 0.054 ug/L
 RT: 4.57 min Scan# 572
 Delta R.T. 0.01 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09

Instrument :
 MSVOA_X
 ClientSampled :
 BG3Q9




Tot Ion: 96 Resp: 383
 Ion Ratio Lower Upper
 96 100
 61 81.6 86.2 160.0#
 68 0.0 0.3 0.7#

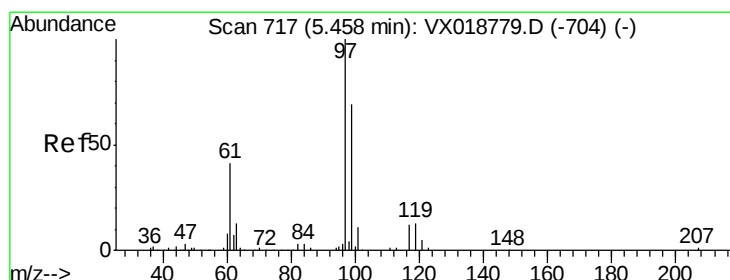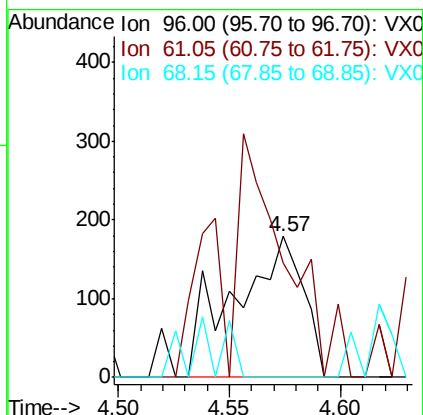


#29

1,1,1-Trichloroethane
 Concen: 0.121 ug/L
 RT: 5.46 min Scan# 718
 Delta R.T. 0.01 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09

Tgt Ion: 97 Resp: 1766
 Ion Ratio Lower Upper
 97 100
 99 55.7 51.3 76.9
 61 36.4 33.3 49.9



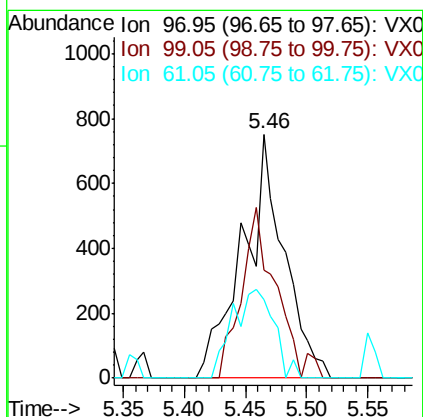



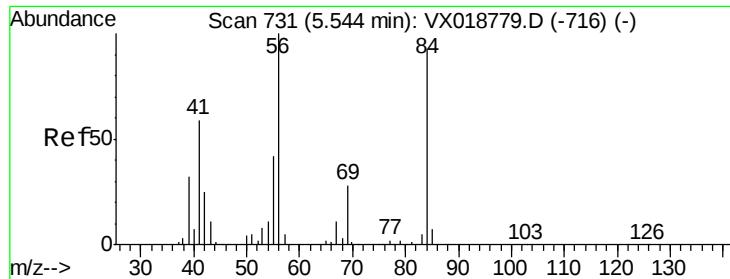

#30
Cyclohexane
Concen: 0.898 ug/L
RT: 5.54 min Scan# 731
Delta R.T. 0.00 min
Lab File: VX018781.D
Acq: 05 Oct 2020 22:09




Instrument :
MSVOA_X
ClientSampled :
BG3Q9


Tot Ion: 56 Resp: 9080
Ion Ratio Lower Upper
56 100
69 36.3 26.0 39.0
84 89.0 73.8 110.6

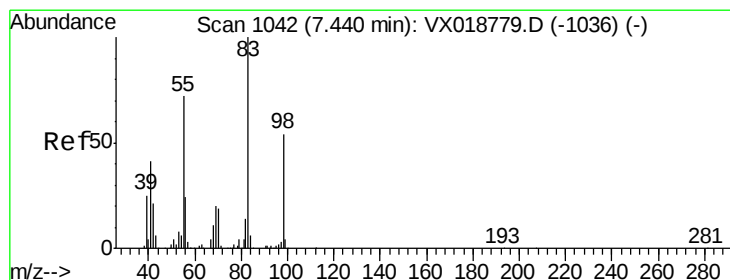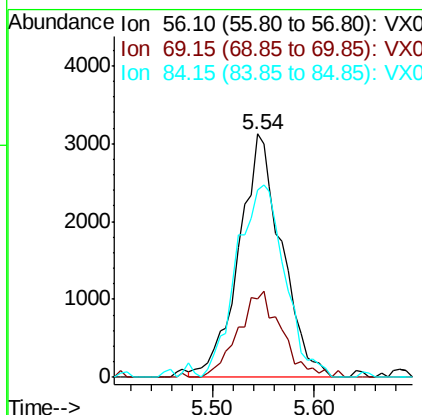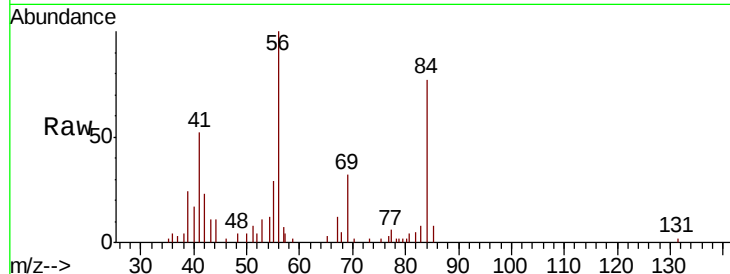

#35
Methylcyclohexane
Concen: 1.317 ug/L
RT: 7.37 min Scan# 1030
Delta R.T. -0.07 min
Lab File: VX018781.D
Acq: 05 Oct 2020 22:09

Tgt Ion: 83 Resp: 14222
Ion Ratio Lower Upper
83 100
55 0.2 60.3 90.5#
98 1.9 39.4 59.0#

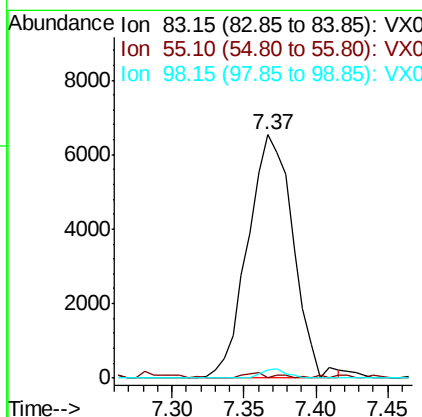

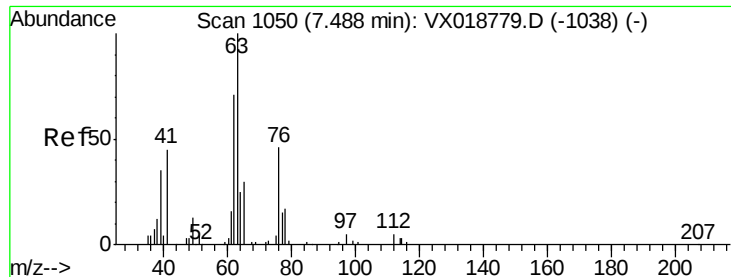

#37

1,2-Dichloropropane

Concen: 1.081 ug/L

RT: 7.37 min Scan# 1030

Delta R.T. -0.12 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09

Instrument :

MSVOA_X

ClientSampleId :





BG3Q9

Tot Ion: 63 Resp: 6994

Ion Ratio Lower Upper

63 100

112 0.3 4.7 7.1#

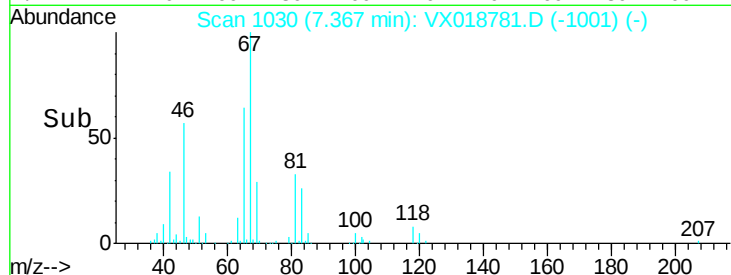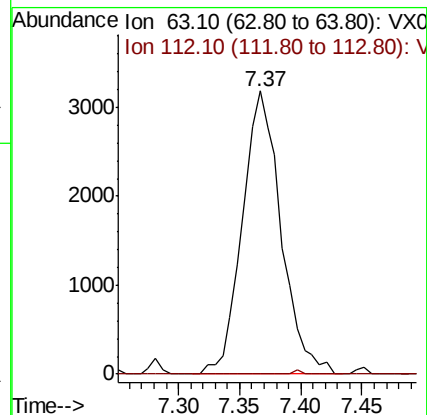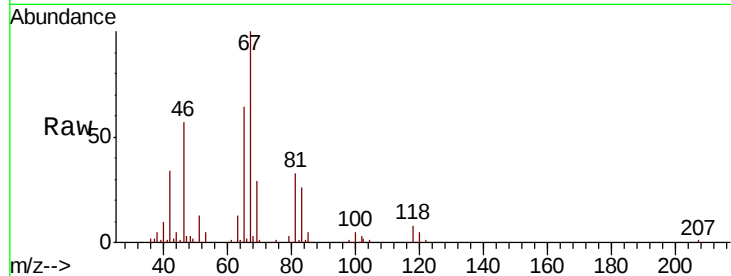

#39

cis-1,3-Dichloropropene

Concen: 0.189 ug/L

RT: 8.37 min Scan# 1194

Delta R.T. -0.05 min

Lab File: VX018781.D




Acq: 05 Oct 2020 22:09


Tgt Ion: 75 Resp: 1947

Ion Ratio Lower Upper

75 100

77 54.5 22.5 41.7#

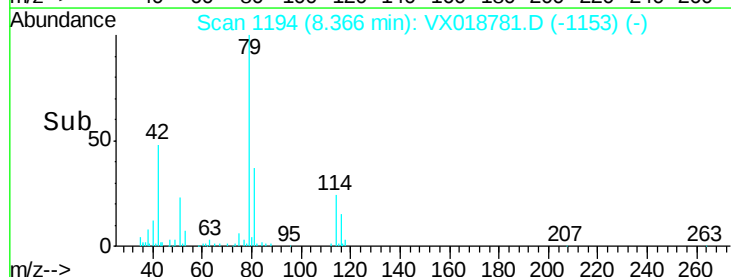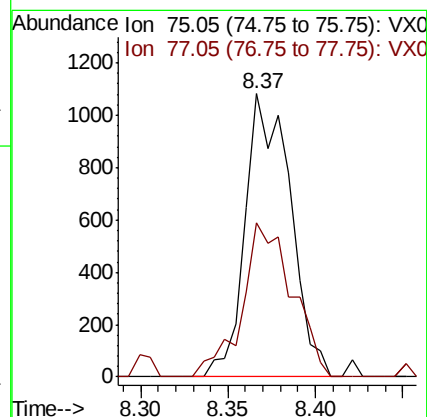

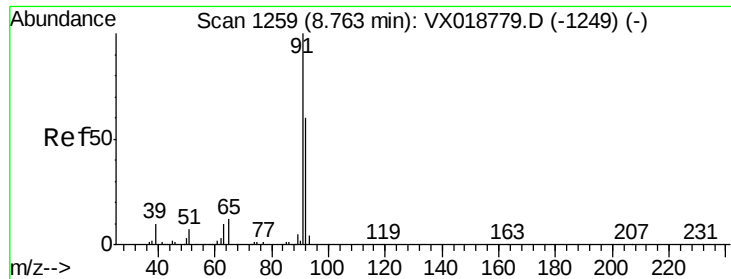

#42

Toluene

Concen: 1.855 ug/L

RT: 8.76 min Scan# 1259

Delta R.T. 0.00 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09

Instrument :

MSVOA_X

ClientSampleId :


BG3Q9

Tot Ion: 91 Resp: 52400

Ion Ratio Lower Upper




91 100

92 58.4 40.3 74.9

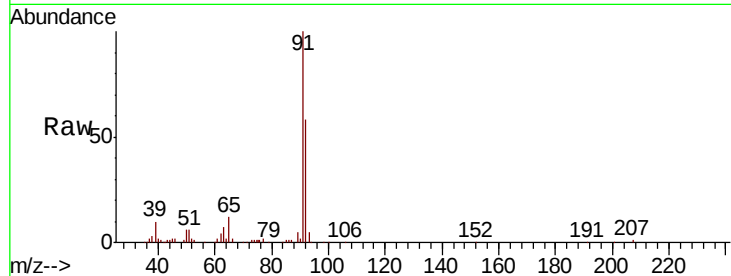

Abundance Ion 91.15 (90.85 to 91.85): VX0

Ion 92.15 (91.85 to 92.85): VX0

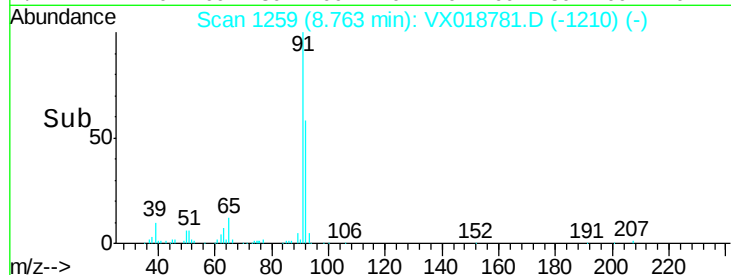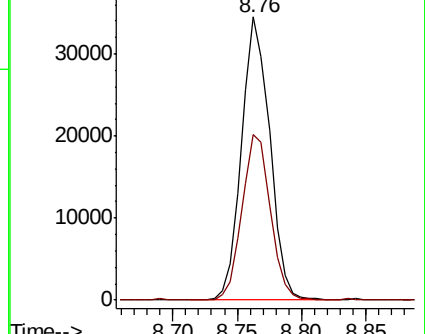

#43

1,3,5-Trimethylbenzene

Concen: 0.295 ug/L

RT: 11.49 min Scan# 1706

Delta R.T. -0.01 min

Lab File: VX018781.D


Acq: 05 Oct 2020 22:09

Tgt Ion:105 Resp: 7887

Ion Ratio Lower Upper



105 100


120 51.1 37.7 56.5



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V



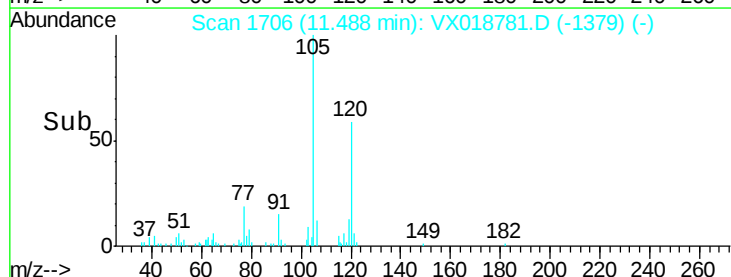
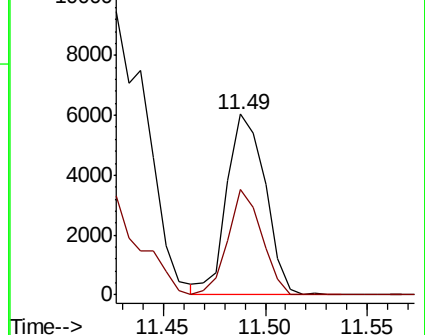




#44
 1,2,4-Trimethylbenzene
 Concen: 0.924 ug/L
 RT: 11.79 min Scan# 1756
 Delta R.T. 0.00 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09




Instrument :
 MSVOA_X
 ClientSampled :
 BG3Q9


Tot Ion:105 Resp: 25081
 Ion Ratio Lower Upper
 105 100
 120 44.1 35.1 52.7

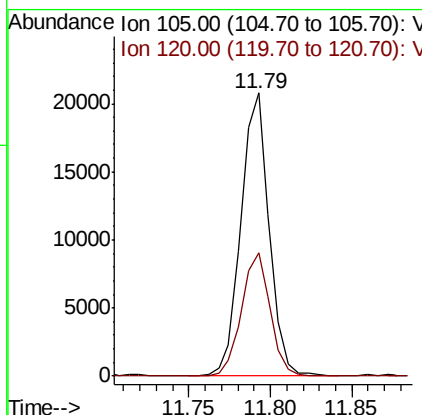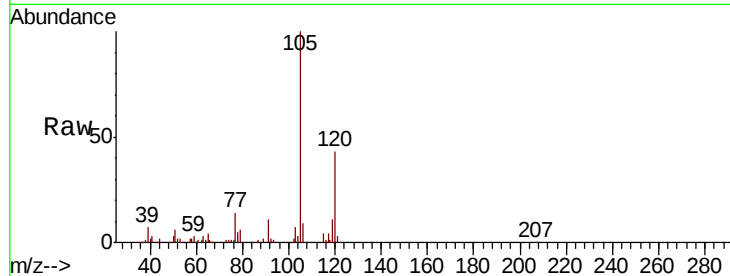

#50
 2-Hexanone
 Concen: 5.378 ug/L
 RT: 9.43 min Scan# 1368
 Delta R.T. -0.05 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09

Tgt Ion: 43 Resp: 14637
 Ion Ratio Lower Upper
 43 100
 58 27.0 41.0 61.4#
 57 27.3 15.9 23.9#
 100 1.0 10.1 15.1#

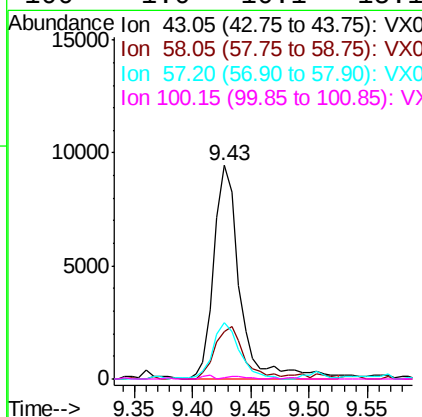

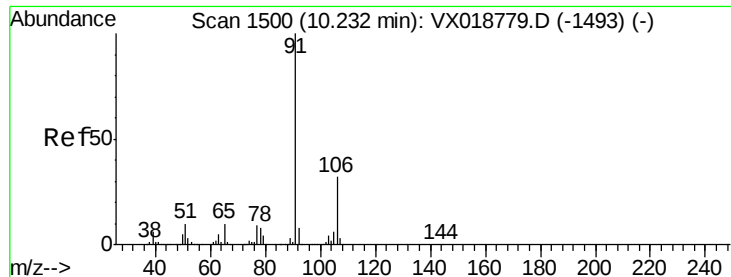

#54

Ethylbenzene

Concen: 0.150 ug/L

RT: 10.24 min Scan# 1501

Delta R.T. 0.01 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09

Instrument :

MSVOA_X

ClientSampleId :





BG3Q9

Tot Ion: 91 Resp: 4741

Ion Ratio Lower Upper

91 100

106 27.4 21.5 39.9

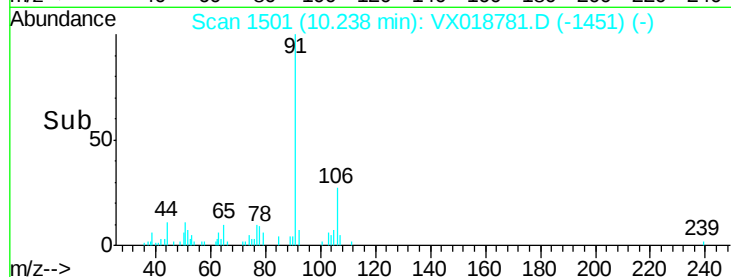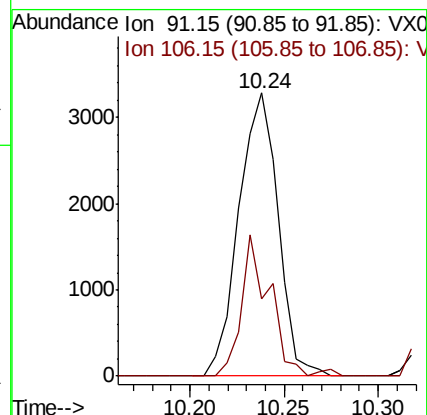

#55

m,p-xylene

Concen: 0.520 ug/L

RT: 10.34 min Scan# 1518

Delta R.T. 0.00 min

Lab File: VX018781.D




Acq: 05 Oct 2020 22:09


Tgt Ion: 106 Resp: 6420

Ion Ratio Lower Upper

106 100

91 205.8 143.4 266.2

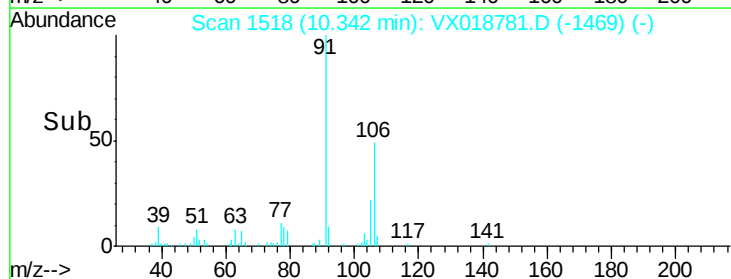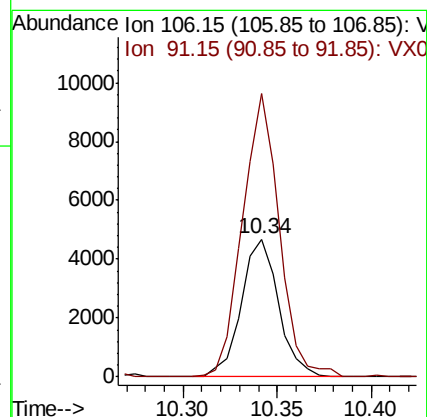


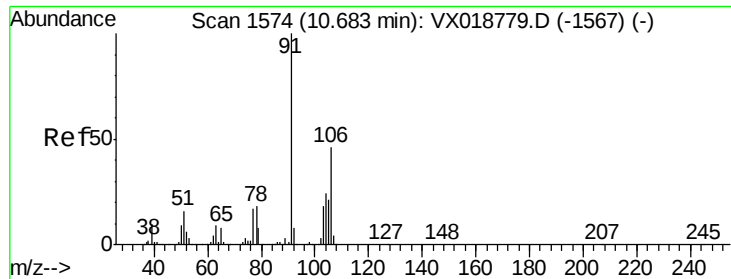




#56
o-xylene
Concen: 0.209 ug/L
RT: 10.68 min Scan# 1574
Delta R.T. 0.00 min
Lab File: VX018781.D
Acq: 05 Oct 2020 22:09

Instrument :
MSVOA_X
ClientSampleId :
BG3Q9

Tot Ion:106 Resp: 2387
Ion Ratio Lower Upper
106 100
91 187.1 153.4 284.8

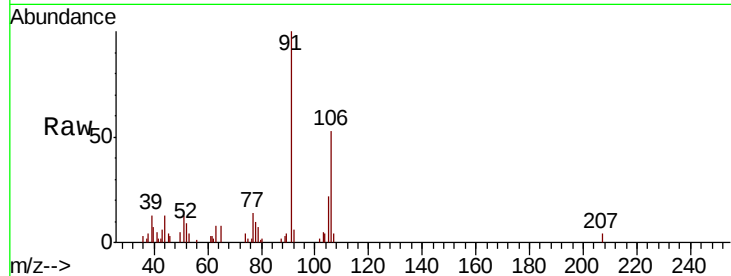


Abundance Ion 106.15 (105.85 to 106.85): V
Ion 91.15 (90.85 to 91.85): VX0

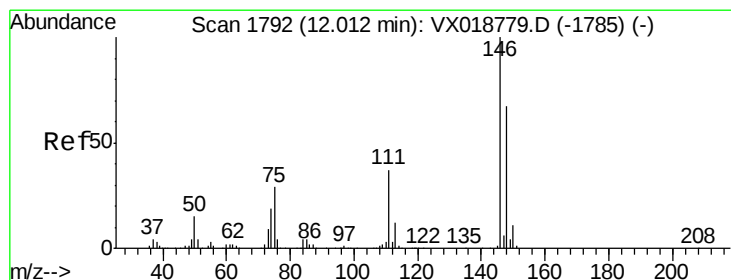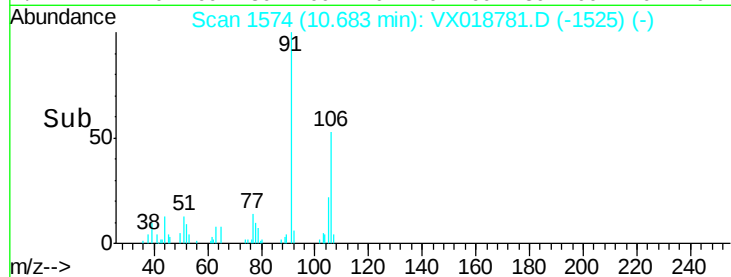
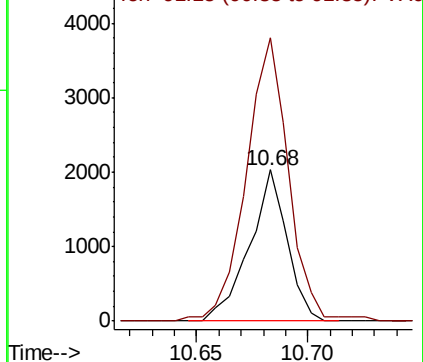



#63
1,3-Dichlorobenzene
Concen: 0.084 ug/L
RT: 12.01 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX018781.D
Acq: 05 Oct 2020 22:09

Tgt Ion:146 Resp: 1205
Ion Ratio Lower Upper
146 100
111 41.6 28.4 52.8
148 66.0 45.9 85.3



Abundance Ion 145.95 (145.65 to 146.65): V
Ion 111.00 (110.70 to 111.70): V
Ion 148.00 (147.70 to 148.70): V

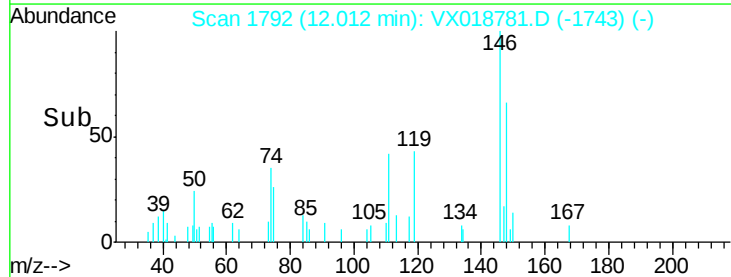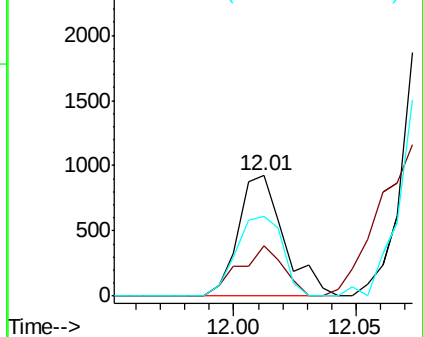



#64

1,4-Dichlorobenzene

Concen: 0.286 ug/L

RT: 12.09 min Scan# 1804

Delta R.T. 0.01 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09

Instrument :

MSVOA_X

ClientSampleId :

BG3Q9


Tot Ion:146 Resp: 4111

Ion Ratio Lower Upper

146 100

111 40.2 28.6 53.2




148 56.7 44.2 82.0



Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

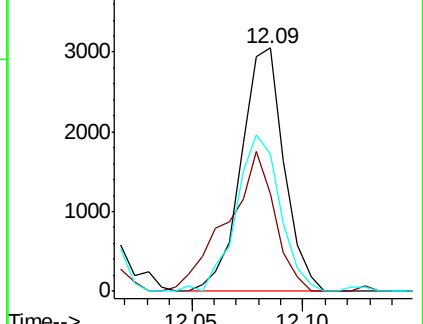

#66

1,2-Dichlorobenzene

Concen: 0.101 ug/L

RT: 12.38 min Scan# 1852

Delta R.T. 0.00 min

Lab File: VX018781.D

Acq: 05 Oct 2020 22:09


Tgt Ion:146 Resp: 1363

Ion Ratio Lower Upper

146 100

111 45.8 31.7 47.5



148 66.5 49.0 73.6




Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V




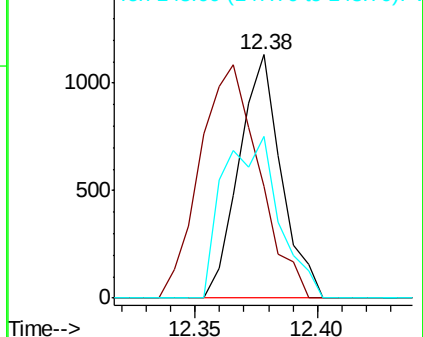




#69
 1,2,4-trichlorobenzene
 Concen: 0.942 ug/L
 RT: 13.63 min Scan# 2057
 Delta R.T. 0.00 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09




Instrument :
 MSVOA_X
 ClientSampled :
 BG3Q9


Tot Ion:180 Resp: 8678
 Ion Ratio Lower Upper
 180 100
 182 95.6 80.2 120.4
 145 33.2 25.2 37.8

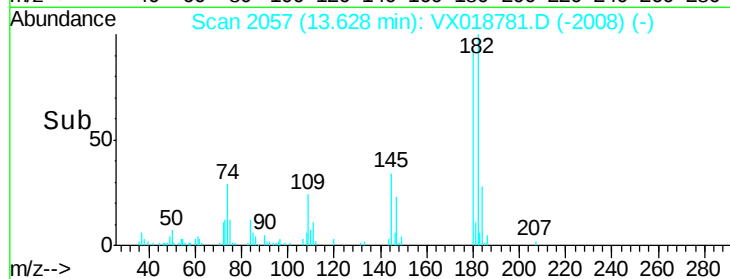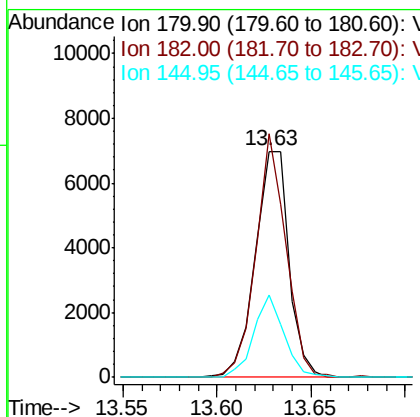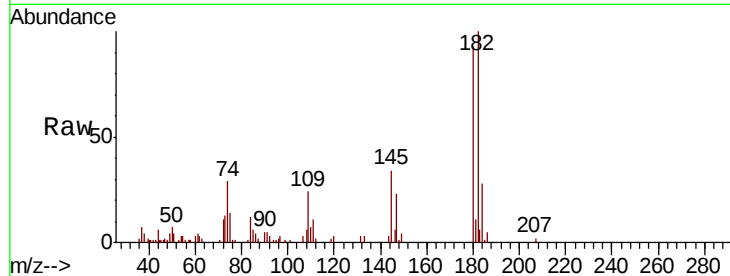

#70
 Naphthalene
 Concen: 0.098 ug/L
 RT: 13.82 min Scan# 2088
 Delta R.T. 0.00 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09

Tgt Ion:128 Resp: 1472
 Ion Ratio Lower Upper
 128 100
 129 5.9 9.0 13.4#
 127 18.9 10.5 15.7#

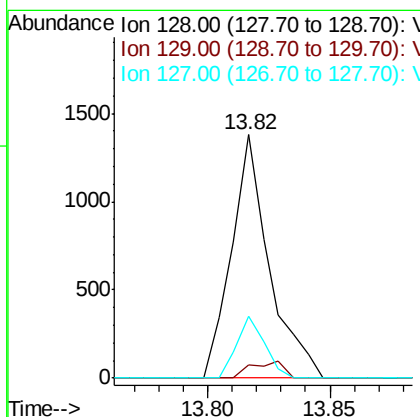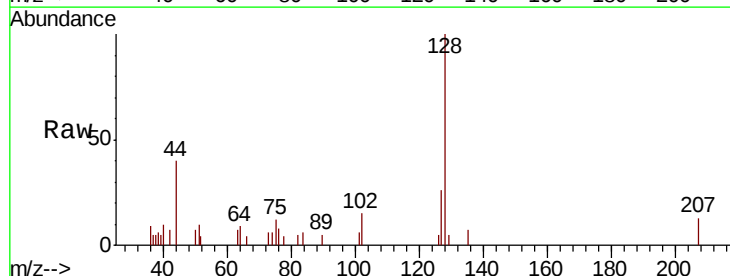


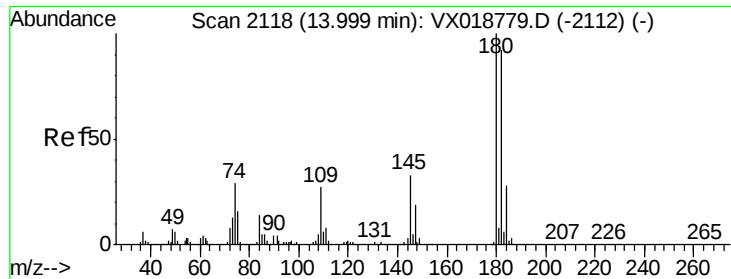

#71
 1,2,3-Trichlorobenzene
 Concen: 0.404 ug/L
 RT: 14.00 min Scan# 2118
 Delta R.T. 0.00 min
 Lab File: VX018781.D
 Acq: 05 Oct 2020 22:09

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3Q9

Tot Ion	Ratio	Lower	Upper
180	100		
182	93.6	73.6	110.4
145	30.6	26.6	40.0

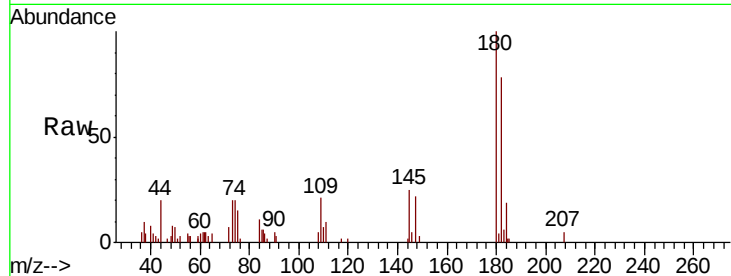

Abundance Ion 179.90 (179.60 to 180.60): V
 Ion 181.90 (181.60 to 182.60): V
 Ion 144.95 (144.65 to 145.65): V

