

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100520\
 Data File : VX018780.D
 Acq On : 05 Oct 2020 21:44
 Operator : JC/SP
 Sample : VX1005WBL02
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK79

Quant Time: Oct 06 06:20:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Oct 06 05:58:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	136209	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	126545	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	55891	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	36069	4.53	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.60%
7) Chloroethane-d5	1.70	69	32155	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.20%
11) 1,1-Dichloroethene-d2	2.34	63	62063	3.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.20%
20) 2-Butanone-d5	4.57	46	129205	61.91	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.82%
24) Chloroform-d	5.14	84	91147	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	6.03	65	53347	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%
32) Benzene-d6	6.05	84	166208	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
36) 1,2-Dichloropropane-d6	7.37	67	51796	5.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	114.00%
41) Toluene-d8	8.70	98	143501	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
45) trans-1,3-Dichloropropene-	8.99	79	22381	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
48) 2-Hexanone-d5	9.43	63	100801	61.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	122.98%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	42054	5.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	113.80%
65) 1,2-Dichlorobenzene-d4	12.36	152	57695	5.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.00%


Target Compounds					Ovalue
16) Methylene chloride	2.83	84	2859	0.348 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100520\
Data File : VX018780.D
Acq On : 05 Oct 2020 21:44
Operator : JC/SP
Sample : VX1005WBL02
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK79

Quant Time: Oct 06 06:20:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Oct 06 05:58:52 2020
Response via : Initial Calibration

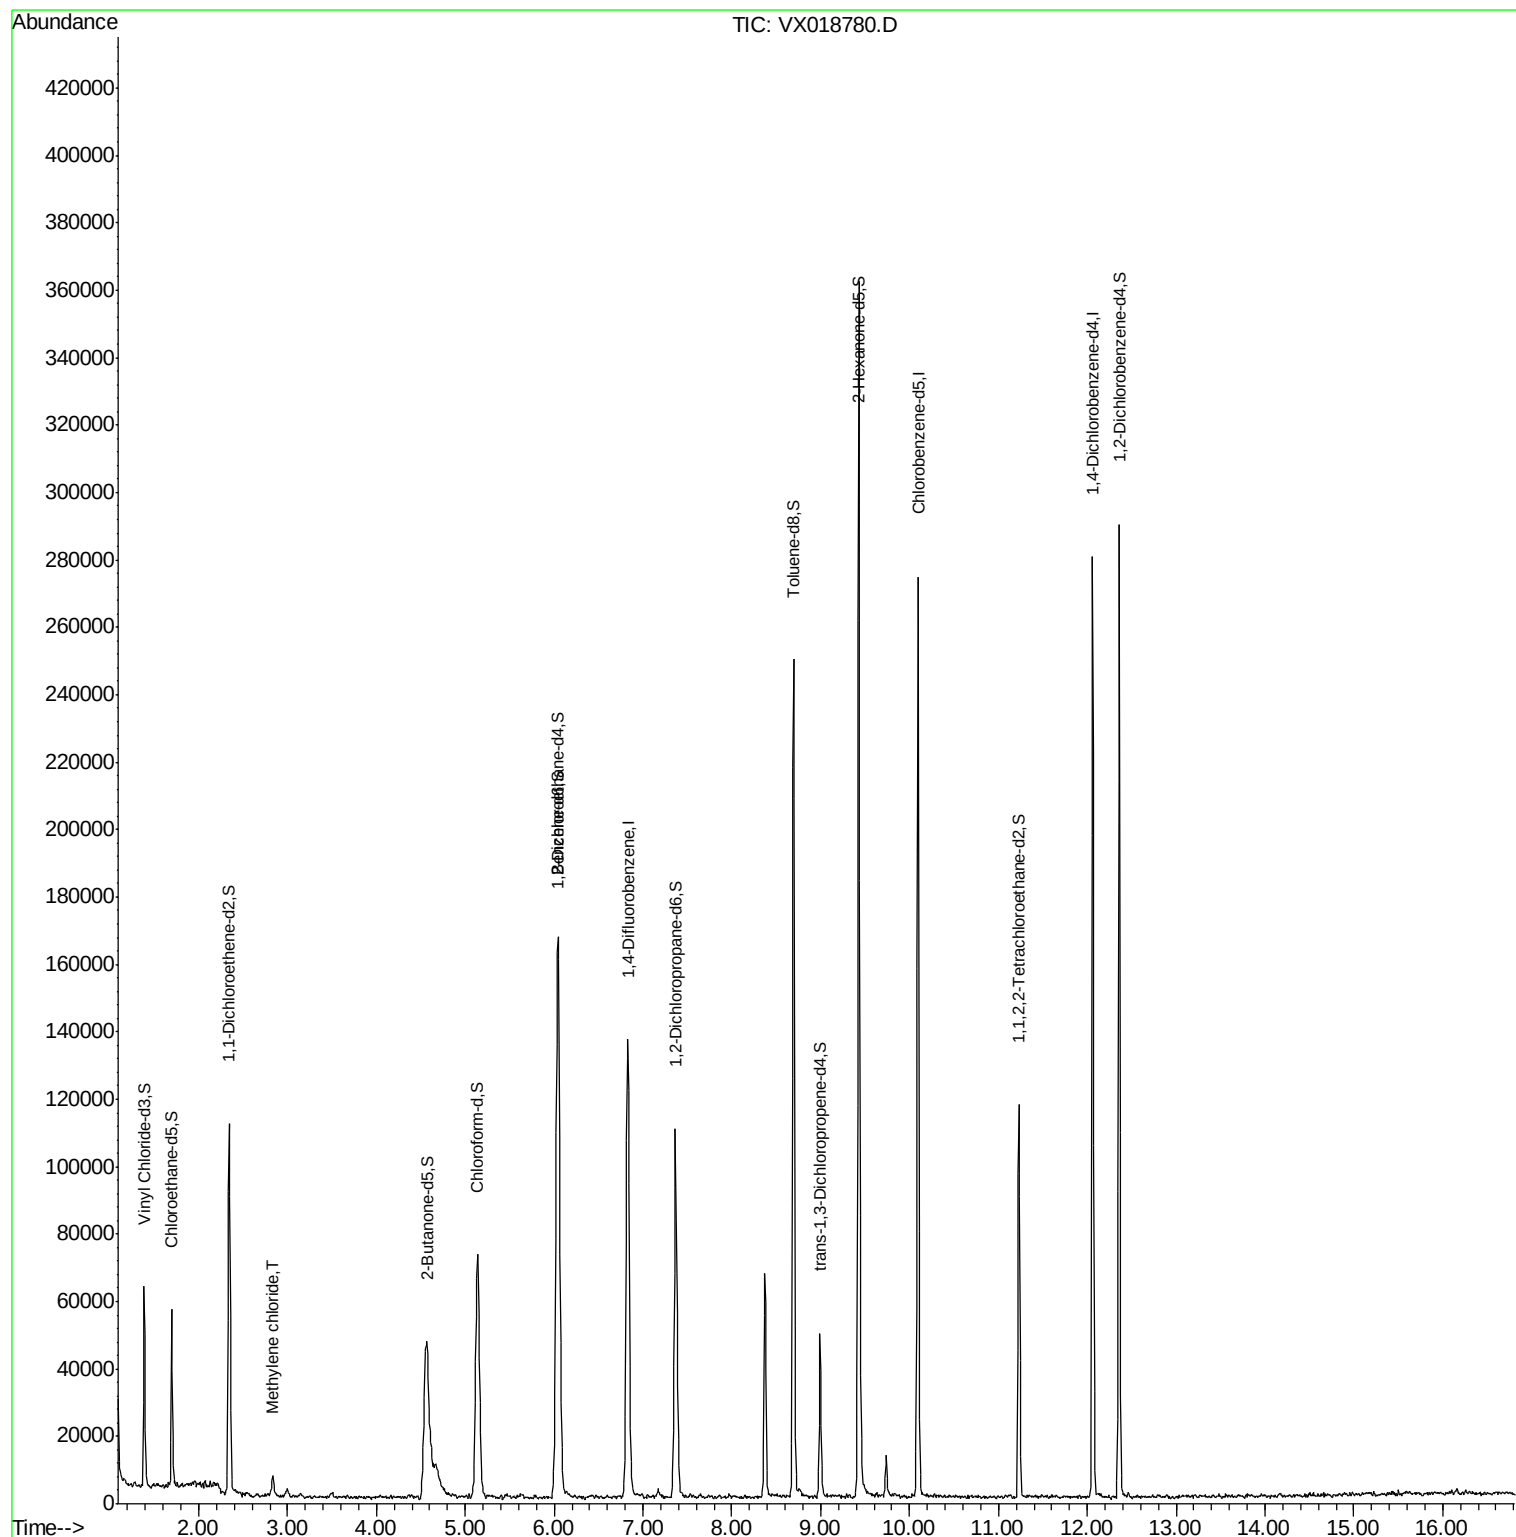

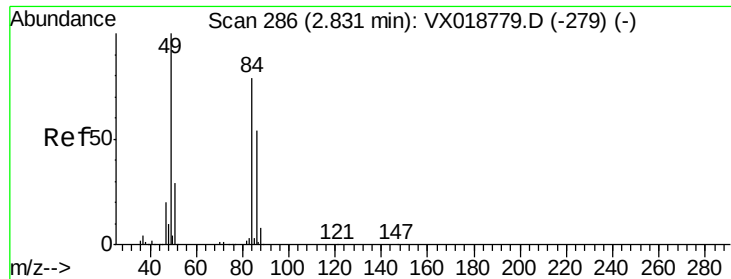

#16
 Methvlene chloride
 Concen: 0.348 ug/L
 RT: 2.83 min Scan# 286
 Delta R.T. -0.00 min
 Lab File: VX018780.D
 Acq: 05 Oct 2020 21:44

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK79

Tot Ion: 84 Resp: 2859
 Ion Ratio Lower Upper
 84 100
 86 57.0 45.6 84.8
 49 131.3 85.8 159.3

