


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100520\
 Data File : VX018761.D
 Acq On : 05 Oct 2020 09:30
 Operator : JC/SP
 Sample : BFB77
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB77

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Oct 06 05:58:52 2020

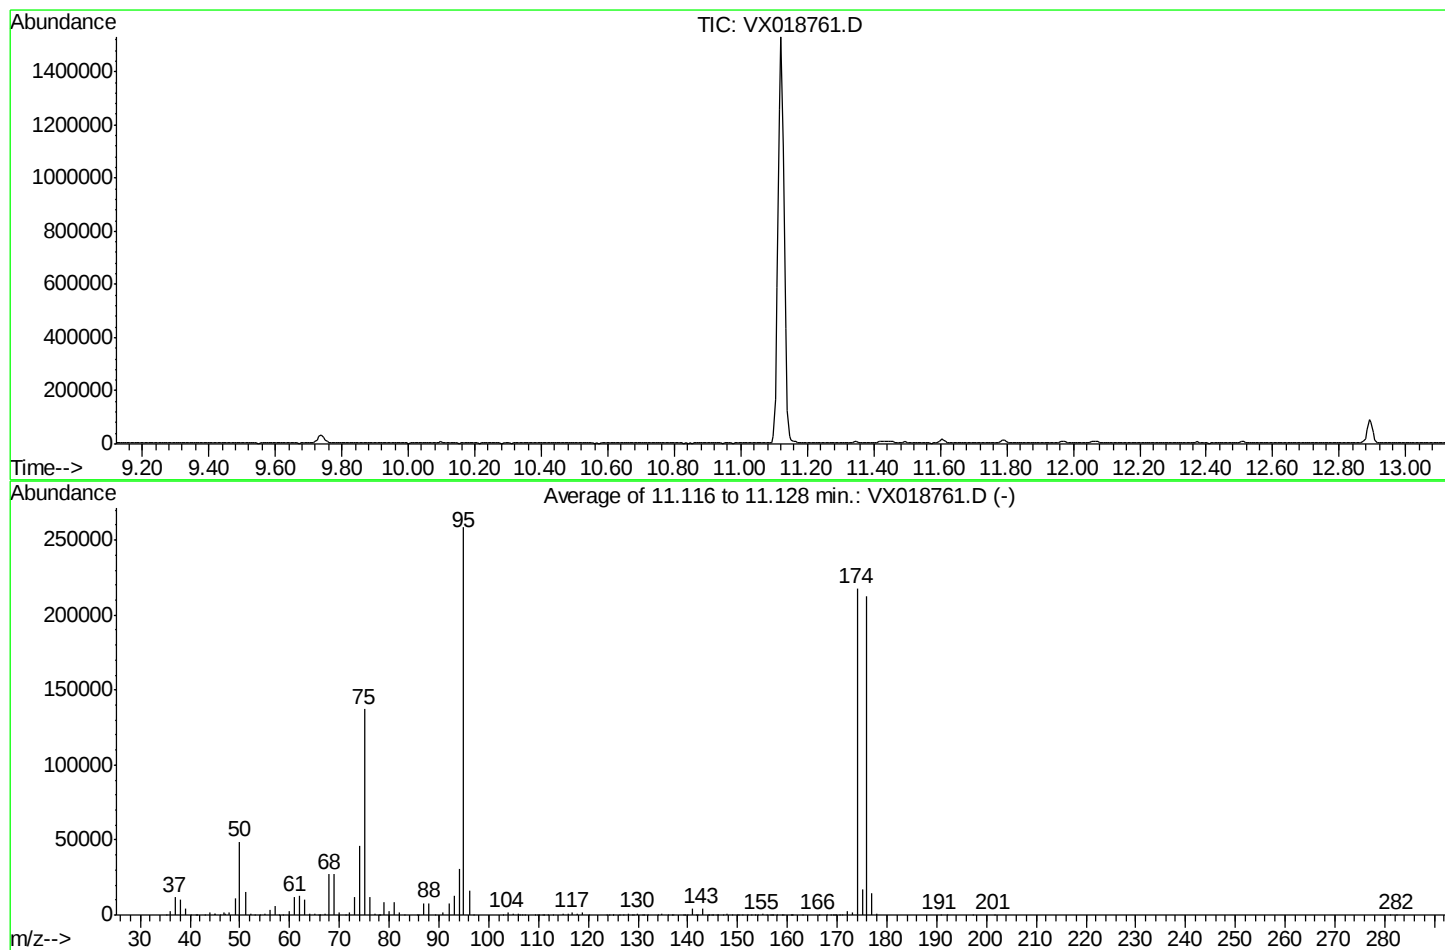

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	49101	PASS
75	95	30	80	53.0	137109	PASS
95	95	100	100	100.0	258560	PASS
96	95	5	9	6.3	16311	PASS
173	174	0.00	2	0.7	1599	PASS
174	95	50	120	84.2	217600	PASS
175	174	5	9	7.9	17164	PASS
176	174	95	101	97.6	212288	PASS
177	176	5	9	6.8	14488	PASS

m/z	Abundance
36.00	2383.0
37.00	13549.0
38.00	11736.0
39.00	4750.0
40.10	321.0
40.70	96.0
41.20	114.0
43.00	197.0
44.00	1479.0
44.90	2184.0
46.10	368.0
46.90	1875.0
48.00	1715.0
49.00	12556.0
50.00	52128.0
51.00	17248.0
52.20	549.0
53.00	167.0
55.00	771.0
56.10	4051.0
57.10	6943.0
57.90	398.0
58.70	256.0
60.00	3390.0
61.00	12488.0
62.00	14564.0
63.00	10971.0
64.10	1712.0
65.00	1603.0
67.10	916.0
68.00	28040.0
69.00	30528.0
70.00	2379.0
71.10	110.0
71.90	1293.0
73.00	12806.0
74.00	48616.0
75.00	141376.0
76.00	13184.0
77.10	1435.0
77.90	1329.0
78.90	8871.0
79.90	2527.0
80.90	8494.0
81.90	1908.0
83.10	396.0
86.00	311.0
87.00	8238.0
88.00	7762.0
89.20	152.0
90.90	1561.0
92.00	7641.0
93.00	12865.0
94.00	30344.0
95.00	264000.0
96.00	16120.0
97.00	428.0
102.70	118.0
103.80	1653.0
105.10	335.0
105.90	1594.0
106.70	189.0
107.20	91.0
109.80	55.0
110.10	65.0
110.90	352.0
112.00	261.0
113.00	211.0
114.90	452.0
115.90	1099.0
116.90	1550.0
117.80	852.0
118.90	1687.0
120.00	106.0
123.80	72.0
124.40	66.0
124.90	102.0
126.10	125.0
127.10	306.0
127.90	1335.0
128.80	447.0
130.00	1157.0
134.80	407.0
136.10	71.0
136.90	530.0
139.10	156.0
139.50	77.0
140.00	314.0
140.90	3470.0
141.80	498.0
142.90	3486.0
144.20	416.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77

145.10	654.0
145.90	541.0
147.10	158.0
147.90	740.0
149.00	155.0
150.00	309.0
151.00	82.0
152.00	145.0
152.90	180.0
153.70	195.0
155.10	880.0
155.90	76.0
157.00	613.0
158.00	73.0
158.90	384.0
160.90	314.0
166.30	55.0
168.00	56.0
168.60	107.0
169.50	248.0
170.50	324.0
172.00	1971.0
174.00	178176.0
175.00	14905.0
176.00	180480.0
177.00	14164.0
178.10	426.0
192.00	98.0
201.60	79.0
207.10	87.0
281.10	116.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77

m/z	Abundance
36.00	2768.0
37.00	14193.0
38.10	11879.0
39.00	5209.0
40.00	592.0
41.40	203.0
42.80	206.0
44.10	2083.0
45.10	2330.0
46.90	2559.0
48.00	1687.0
49.00	13783.0
50.00	59216.0
51.10	17888.0
52.00	756.0
53.00	360.0
55.00	1142.0
56.10	4263.0
57.00	7147.0
58.00	324.0
58.60	125.0
60.00	2898.0
61.00	14692.0
62.00	15533.0
63.00	11458.0
64.00	1148.0
65.10	1202.0
66.20	297.0
66.90	797.0
68.00	33336.0
69.00	32856.0
70.10	2175.0
71.00	75.0
72.00	2126.0
73.00	14331.0
74.00	55040.0
75.00	164160.0
76.00	14726.0
77.00	1316.0
78.90	9932.0
80.00	2566.0
80.90	11126.0
81.90	2417.0
83.20	209.0
85.90	232.0
87.10	8728.0
88.00	9250.0
89.30	82.0
90.80	1433.0
92.00	9641.0
93.00	15117.0
94.00	36264.0
95.00	299648.0
96.00	20040.0
97.00	416.0
103.90	1654.0
104.90	481.0
105.90	1627.0
106.80	209.0
110.20	120.0
111.10	395.0
111.90	226.0
112.80	418.0
114.90	363.0
116.00	1090.0
116.80	2365.0
117.80	1254.0
118.90	2151.0
120.10	81.0
123.70	100.0
125.10	174.0
126.20	223.0
128.00	1215.0
129.00	628.0
130.00	1379.0
130.80	513.0
133.90	202.0
134.80	1027.0
136.10	97.0
137.10	583.0
139.90	624.0
140.90	4838.0
142.00	511.0
142.90	5102.0
144.20	281.0
144.80	753.0
145.90	641.0
147.00	162.0
147.70	798.0
148.00	764.0
148.80	284.0
149.80	405.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77

150.30	215.0
151.90	61.0
152.80	278.0
154.00	327.0
154.90	941.0
155.90	165.0
156.70	332.0
157.20	386.0
159.10	313.0
160.60	316.0
161.10	401.0
163.10	71.0
166.40	121.0
169.10	147.0
169.80	290.0
170.50	363.0
170.90	457.0
172.00	2295.0
173.10	4799.0
174.00	259456.0
175.00	20328.0
176.00	243136.0
177.00	16792.0
178.00	517.0
190.70	54.0
197.20	55.0
207.10	184.0
281.30	212.0
282.40	100.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77

m/z	Abundance
35.20	188.0
36.00	1830.0
37.10	8093.0
38.00	7850.0
39.00	3277.0
40.00	436.0
42.60	141.0
43.20	164.0
44.00	1734.0
45.10	1378.0
46.00	282.0
47.10	1495.0
47.80	975.0
49.00	7741.0
50.00	36232.0
51.00	11327.0
52.10	419.0
53.00	210.0
53.90	72.0
55.10	425.0
56.00	3002.0
57.10	4915.0
58.00	325.0
60.10	1938.0
61.00	8988.0
62.10	9520.0
63.00	8504.0
63.90	667.0
64.90	865.0
65.80	153.0
67.10	585.0
68.00	20104.0
69.00	19864.0
70.10	1617.0
71.20	106.0
71.90	1583.0
73.00	9864.0
74.00	35408.0
75.10	105792.0
76.00	8969.0
77.00	931.0
78.10	619.0
78.90	6163.0
80.00	1898.0
80.90	6995.0
81.90	1870.0
85.70	233.0
86.90	5924.0
88.00	6128.0
90.90	1169.0
92.00	7066.0
93.00	10276.0
94.00	26168.0
95.00	212032.0
96.10	12774.0
97.00	386.0
102.80	104.0
103.80	923.0
104.80	655.0
106.10	870.0
106.80	126.0
107.20	196.0
109.30	100.0
109.90	125.0
110.70	156.0
111.00	147.0
111.90	351.0
112.80	570.0
114.80	627.0
115.90	972.0
117.00	1327.0
117.80	1090.0
119.00	1142.0
123.80	170.0
124.20	143.0
125.00	228.0
126.20	117.0
127.00	109.0
127.90	697.0
129.00	574.0
129.80	1004.0
131.10	402.0
132.00	161.0
134.00	115.0
134.80	496.0
136.00	188.0
136.90	665.0
138.90	99.0
139.90	268.0
140.90	3573.0
142.10	548.0
142.90	3375.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77

143.90	364.0
144.90	394.0
146.10	355.0
146.90	223.0
147.90	982.0
148.90	346.0
149.90	361.0
151.90	112.0
152.90	350.0
153.50	127.0
154.00	289.0
155.00	537.0
155.90	142.0
156.90	482.0
157.80	159.0
159.00	518.0
161.00	337.0
169.10	238.0
169.70	231.0
170.90	220.0
171.90	1267.0
172.10	1255.0
174.00	215168.0
175.00	16259.0
176.00	213248.0
177.00	12510.0
178.00	650.0
190.70	67.0
197.20	56.0
207.20	338.0
281.10	212.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77

m/z	Abundance
35.20	57.0
36.30	112.0
37.80	60.0
38.30	92.0
40.10	135.0
40.90	187.0
42.00	97.0
42.70	79.0
43.10	60.0
44.20	327.0
44.90	73.0
45.50	104.0
46.90	70.0
49.80	91.0
54.50	64.0
58.30	69.0
73.00	120.0
78.20	120.0
85.60	62.0
94.10	74.0
103.40	60.0
116.80	57.0
207.20	221.0
269.70	92.0
281.00	95.0
281.30	81.0

Instrument :
MSVOA_X
ClientSampleId :
BFB77