

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
 Data File : VX024576.D
 Acq On : 05 Oct 2021 17:13
 Operator : JC/MD
 Sample : M4080-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-03-(SA)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	36	rBV	17028	27611	3.45%	0.668%
2	2.544	233	239	251	rVB	15291	27381	3.42%	0.663%
3	5.397	691	707	721	rBV	92217	261936	32.74%	6.341%
4	5.562	722	734	745	rBV	140031	390759	48.84%	9.460%
5	5.964	790	800	812	rBV	100275	261886	32.73%	6.340%
6	6.769	922	932	945	rBV	244754	580139	72.51%	14.045%
7	8.653	1234	1241	1249	rBV	521853	800049	100.00%	19.369%
8	8.726	1249	1253	1258	rVB	5439	8780	1.10%	0.213%
9	10.055	1464	1471	1481	rBV	510773	676455	84.55%	16.377%
10	11.085	1634	1640	1654	rVB	406251	515836	64.48%	12.488%
11	12.024	1789	1794	1804	rVB	482295	579748	72.46%	14.036%




Sum of corrected areas: 4130580

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024576.D
Acq On : 05 Oct 2021 17:13
Operator : JC/MD
Sample : M4080-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

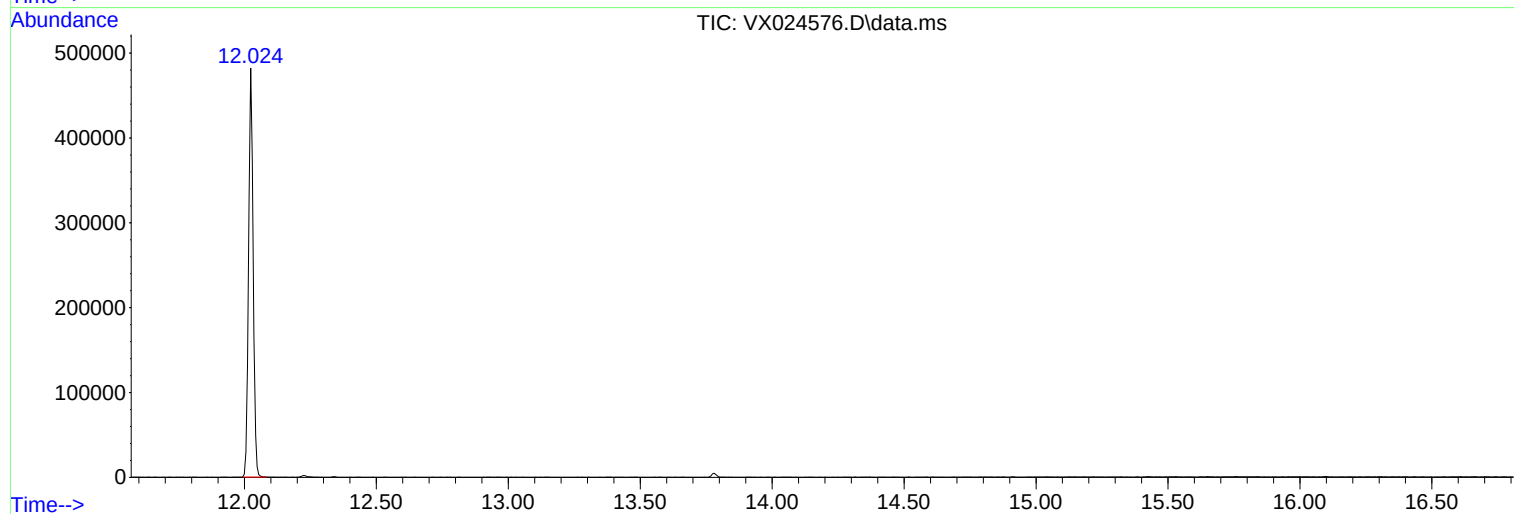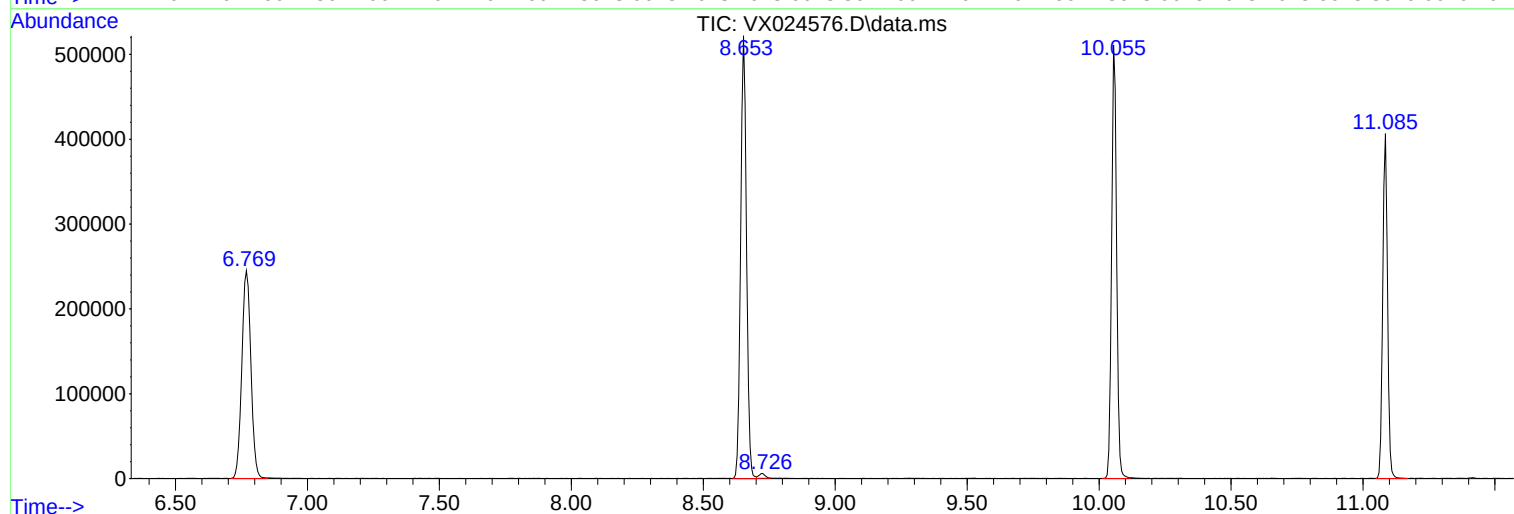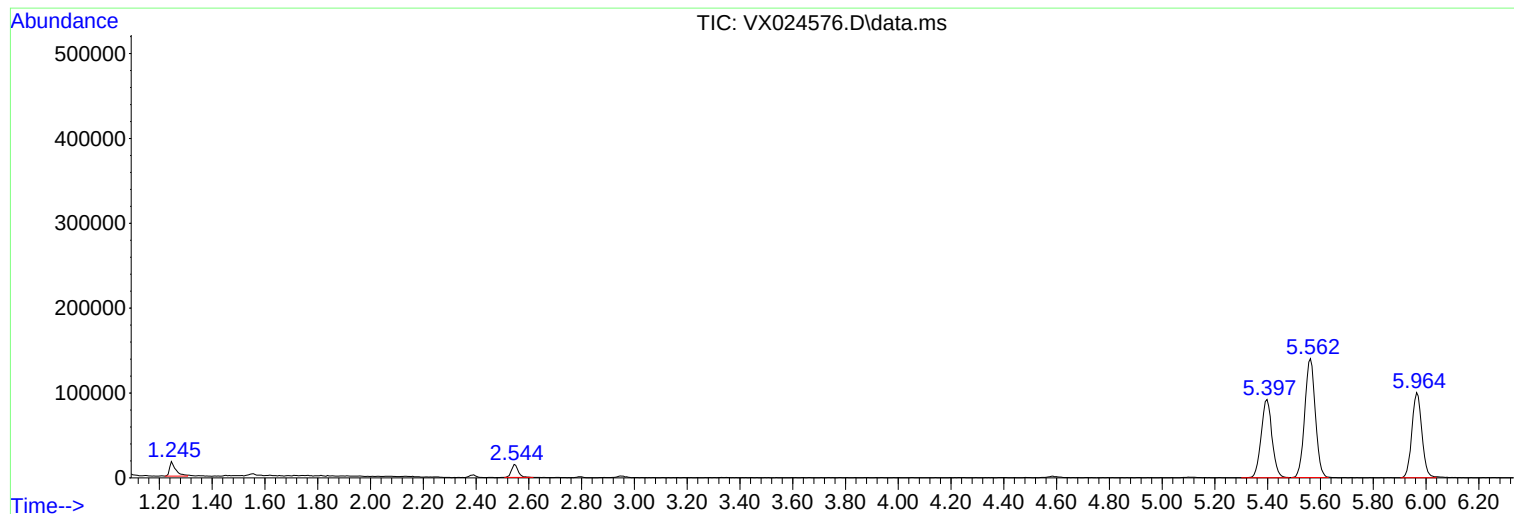

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024576.D
Acq On : 05 Oct 2021 17:13
Operator : JC/MD
Sample : M4080-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024576.D
Acq On : 05 Oct 2021 17:13
Operator : JC/MD
Sample : M4080-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-03-(SA)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------