

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
 Data File : VX024577.D
 Acq On : 05 Oct 2021 17:36
 Operator : JC/MD
 Sample : M4080-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SW-RR-01-(2.0)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	17668	25897	3.17%	0.623%
2	2.544	232	239	251	rBV	15458	29399	3.60%	0.707%
3	2.953	296	306	314	rVB	4428	10345	1.27%	0.249%
4	4.587	564	574	585	rBV2	3194	10847	1.33%	0.261%
5	5.397	694	707	722	rBV	97440	282888	34.61%	6.801%
6	5.556	722	733	752	rVB	150861	429687	52.57%	10.330%
7	5.964	789	800	818	rBV2	104063	275238	33.68%	6.617%
8	6.769	921	932	945	rBV	250238	583584	71.40%	14.029%
9	8.653	1234	1241	1253	rBV	534658	817291	100.00%	19.648%
10	10.055	1465	1471	1486	rBV	450364	629104	76.97%	15.124%
11	11.085	1634	1640	1654	rBV	410153	505461	61.85%	12.151%
12	12.024	1789	1794	1802	rBV	462153	559971	68.52%	13.462%




Sum of corrected areas: 4159712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024577.D
Acq On : 05 Oct 2021 17:36
Operator : JC/MD
Sample : M4080-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-01-(2.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

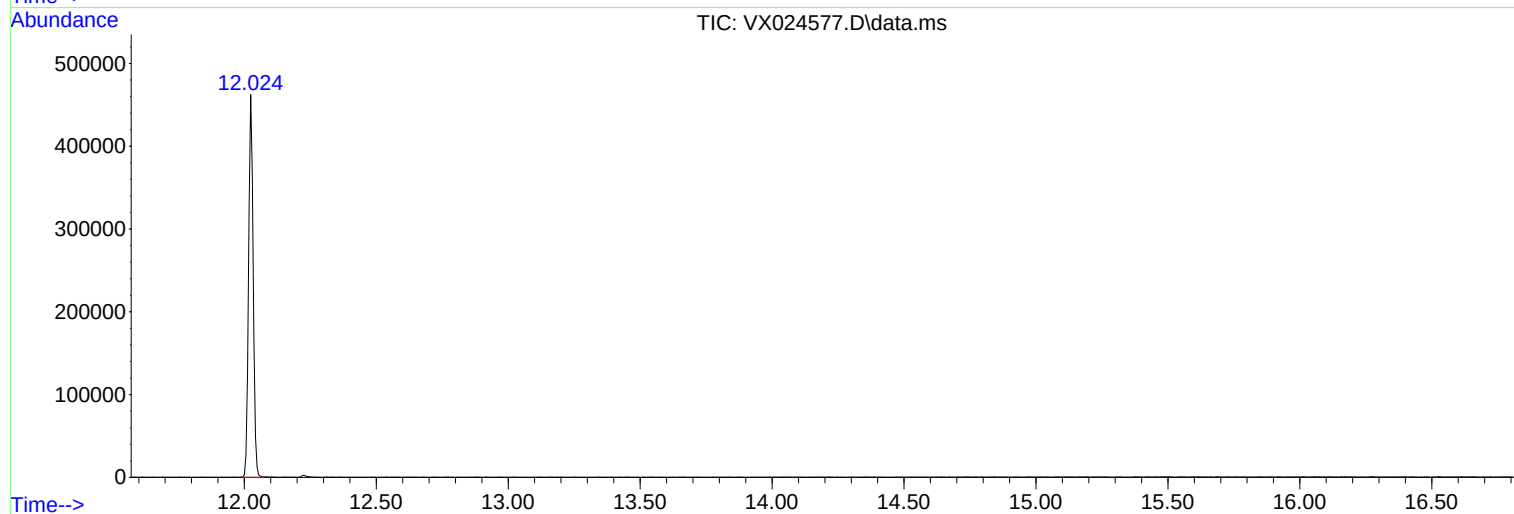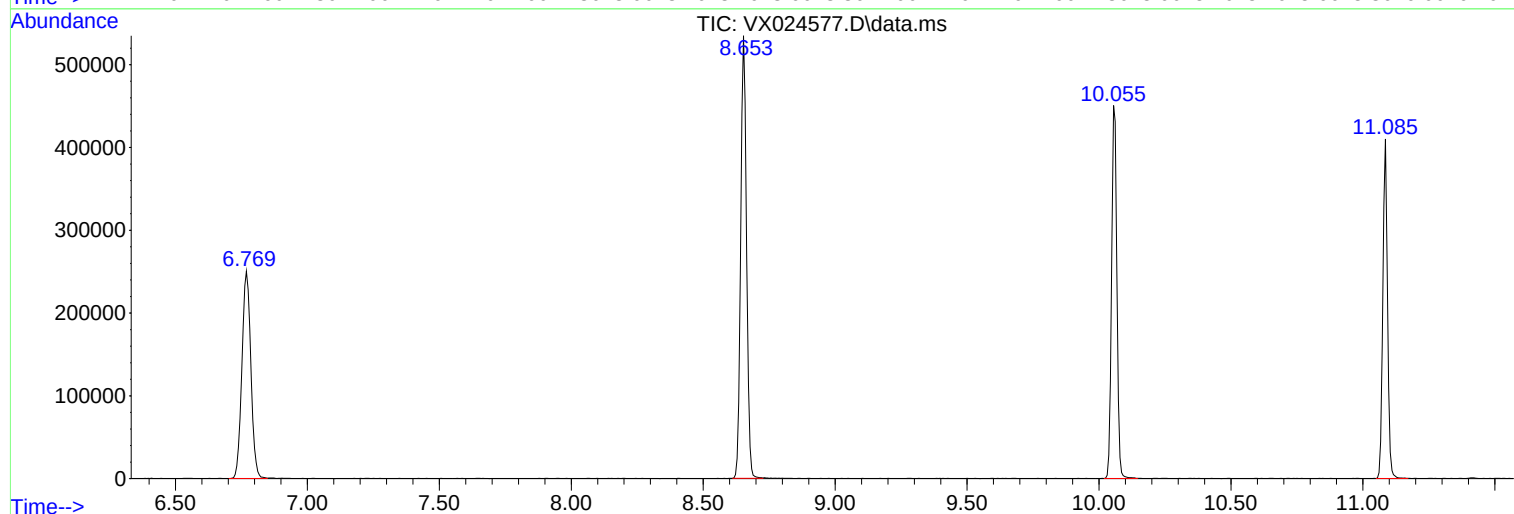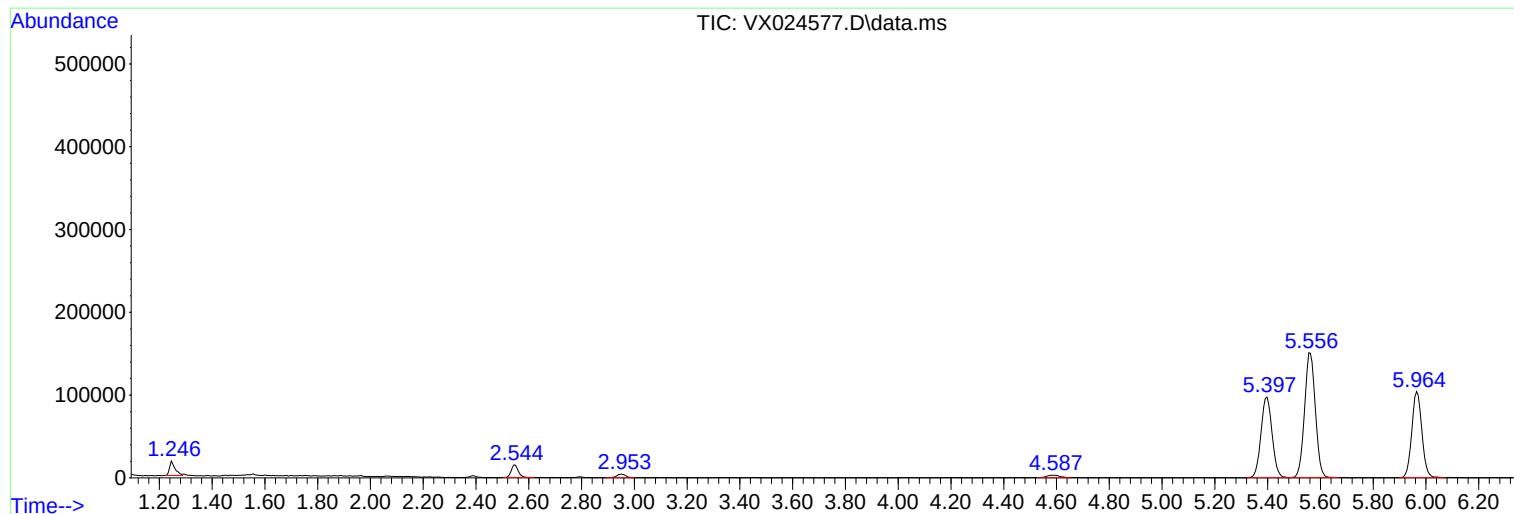

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024577.D
Acq On : 05 Oct 2021 17:36
Operator : JC/MD
Sample : M4080-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-01-(2.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024577.D
Acq On : 05 Oct 2021 17:36
Operator : JC/MD
Sample : M4080-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SW-RR-01-(2.0)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
