

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
 Data File : VX024582.D
 Acq On : 05 Oct 2021 19:34
 Operator : JC/MD
 Sample : M4059-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SH-SUMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024582.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	37	rBV2	4976	10647	1.29%	0.250%
2	2.544	233	239	246	rBV	6196	11019	1.33%	0.259%
3	2.947	299	305	315	rVB3	3796	8982	1.08%	0.211%
4	4.581	565	573	583	rBV2	2732	8448	1.02%	0.198%
5	5.398	694	707	721	rBV3	98877	285835	34.51%	6.714%
6	5.562	722	734	751	rVB	153073	432630	52.23%	10.162%
7	5.964	788	800	814	rBV	100989	267020	32.24%	6.272%
8	6.769	920	932	944	rBV	250534	592623	71.55%	13.920%
9	8.653	1234	1241	1250	rBV	553853	828299	100.00%	19.456%
10	10.055	1465	1471	1487	rBV	533061	719591	86.88%	16.903%
11	11.086	1634	1640	1653	rBV	390599	512311	61.85%	12.034%
12	12.024	1789	1794	1804	rBV	469334	579799	70.00%	13.619%




Sum of corrected areas: 4257204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024582.D
Acq On : 05 Oct 2021 19:34
Operator : JC/MD
Sample : M4059-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SH-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

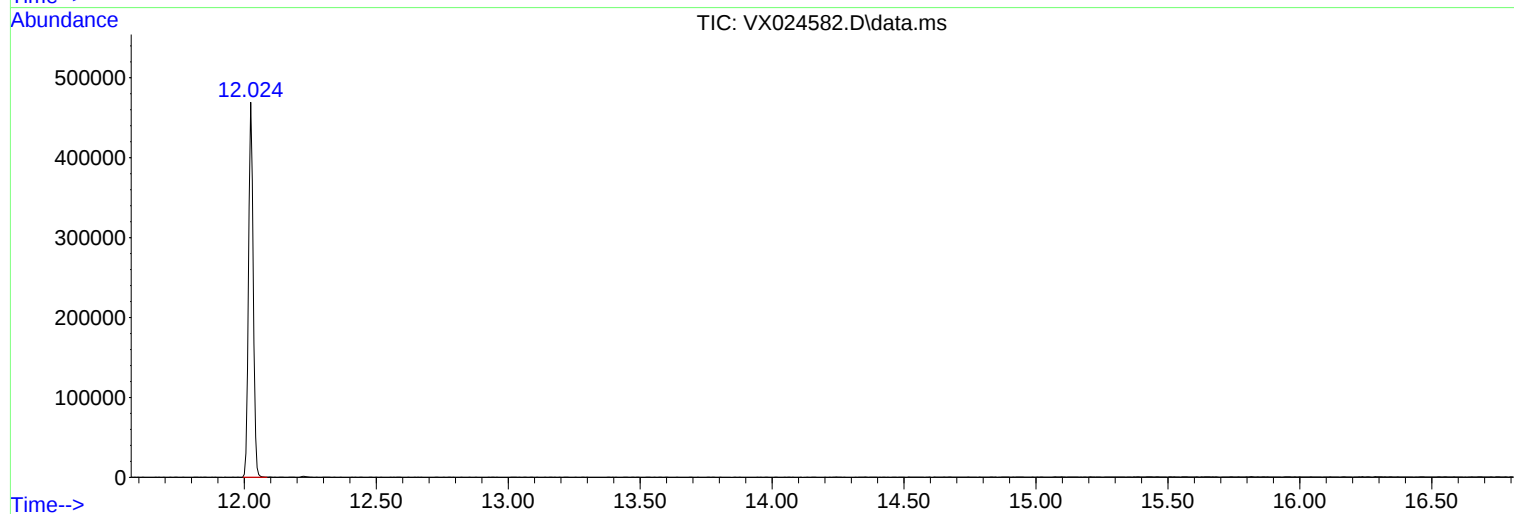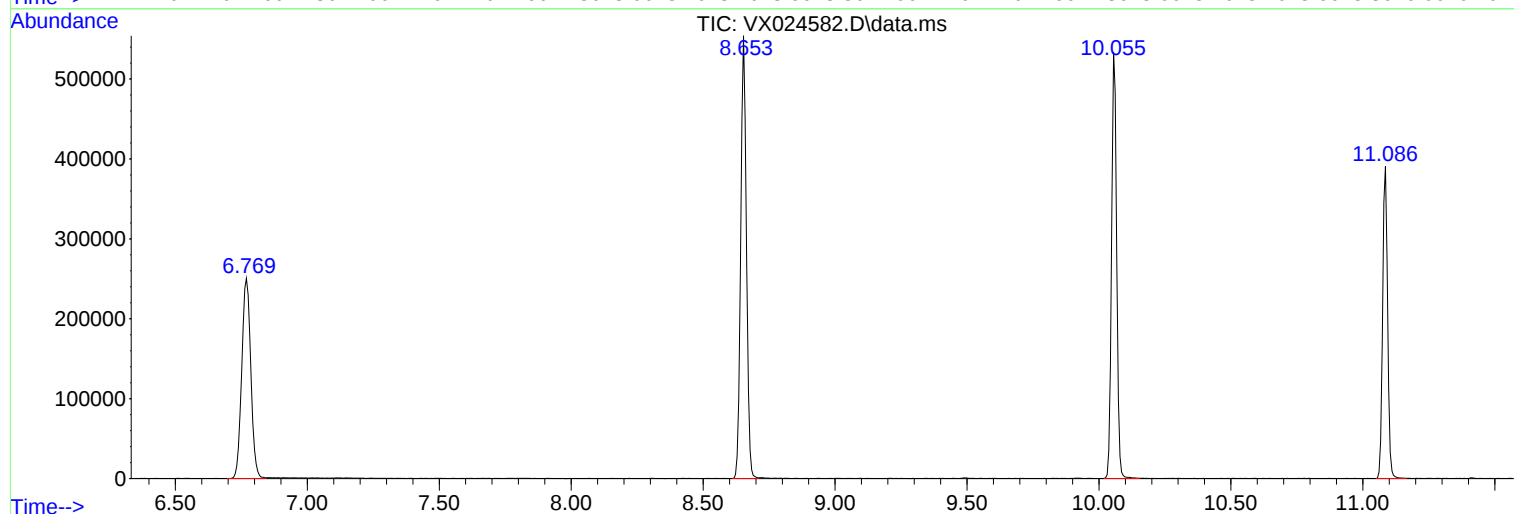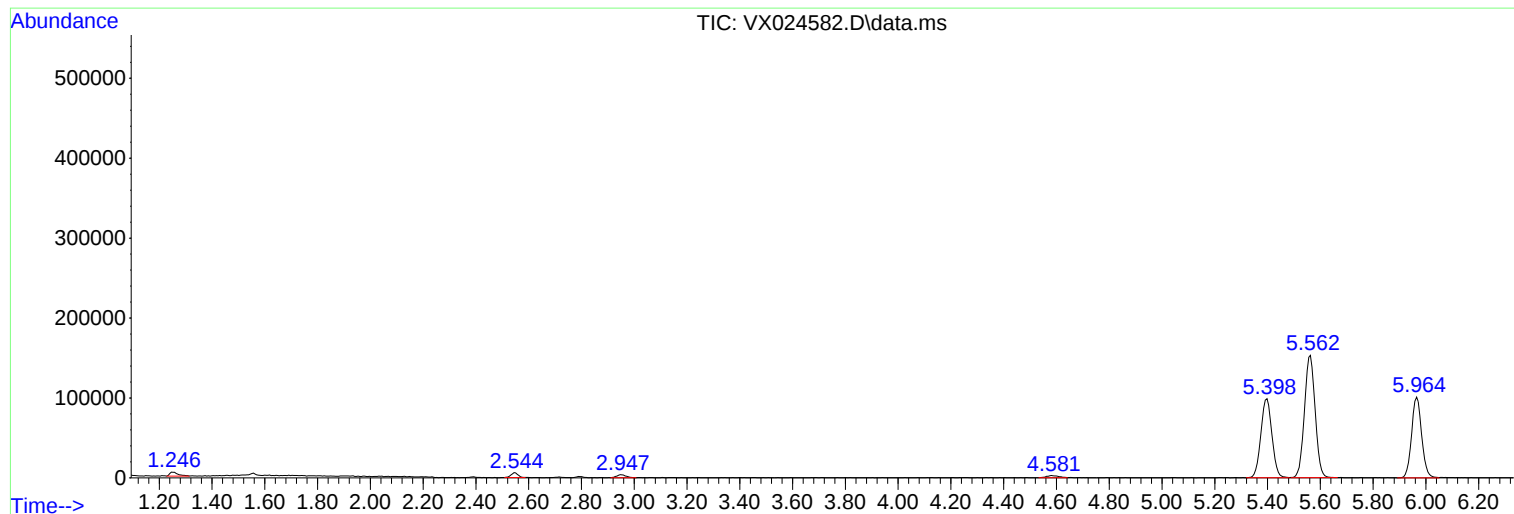

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024582.D
Acq On : 05 Oct 2021 19:34
Operator : JC/MD
Sample : M4059-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SH-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024582.D
Acq On : 05 Oct 2021 19:34
Operator : JC/MD
Sample : M4059-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SH-SUMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
