

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
 Data File : VX024596.D
 Acq On : 06 Oct 2021 02:11
 Operator : JC/MD
 Sample : M4028-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024596.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	23	27	42	rVB3	20428	34610	4.66%	0.843%
2	2.544	231	239	250	rVB	10202	19727	2.65%	0.481%
3	2.947	299	305	315	rVB	3403	7775	1.05%	0.189%
4	5.397	694	707	720	rBV2	89449	268917	36.18%	6.552%
5	5.562	723	734	748	rVB	147092	414079	55.71%	10.089%
6	5.964	789	800	814	rBV	104798	272419	36.65%	6.637%
7	6.769	921	932	946	rBV	240920	567143	76.31%	13.818%
8	8.653	1234	1241	1254	rBV	479168	743253	100.00%	18.109%
9	10.055	1465	1471	1481	rBV	508186	689801	92.81%	16.806%
10	11.085	1634	1640	1653	rBV	409926	515292	69.33%	12.555%
11	12.024	1789	1794	1802	rBV	473406	571366	76.87%	13.921%




Sum of corrected areas: 4104382

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024596.D
Acq On : 06 Oct 2021 02:11
Operator : JC/MD
Sample : M4028-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

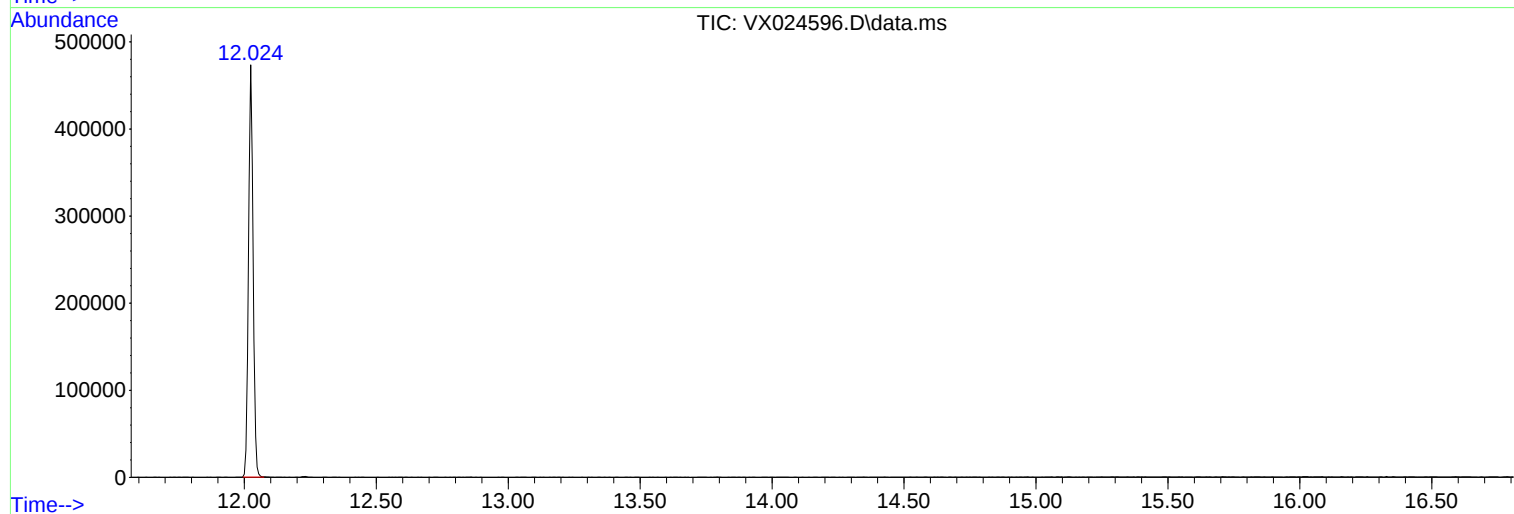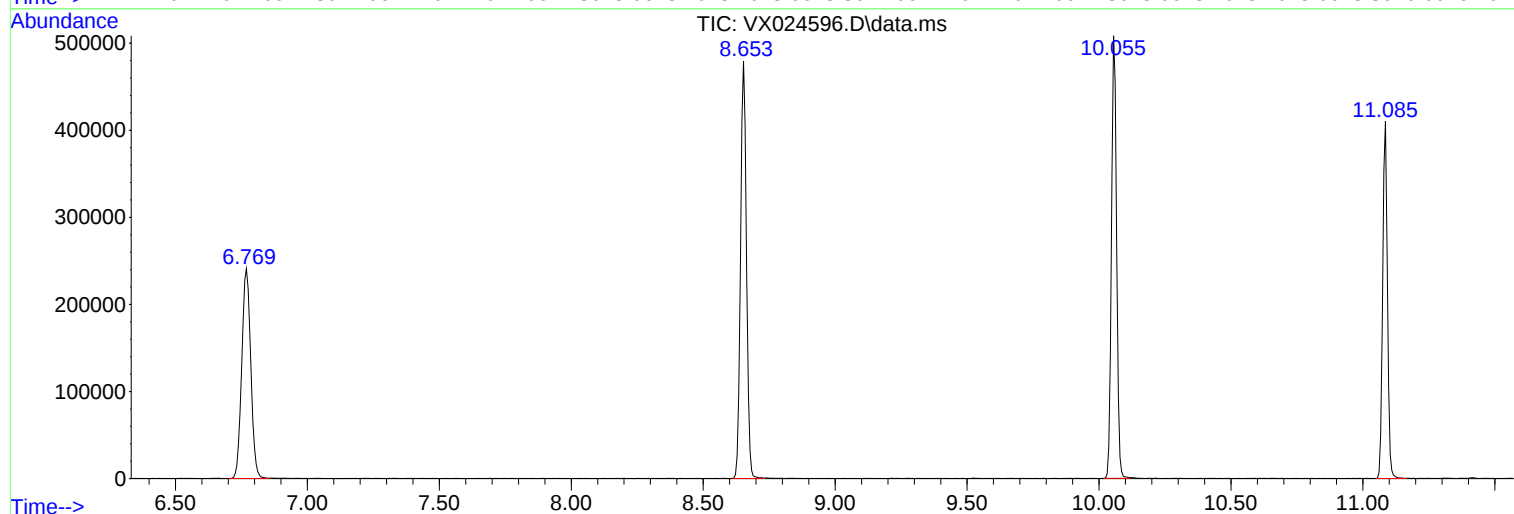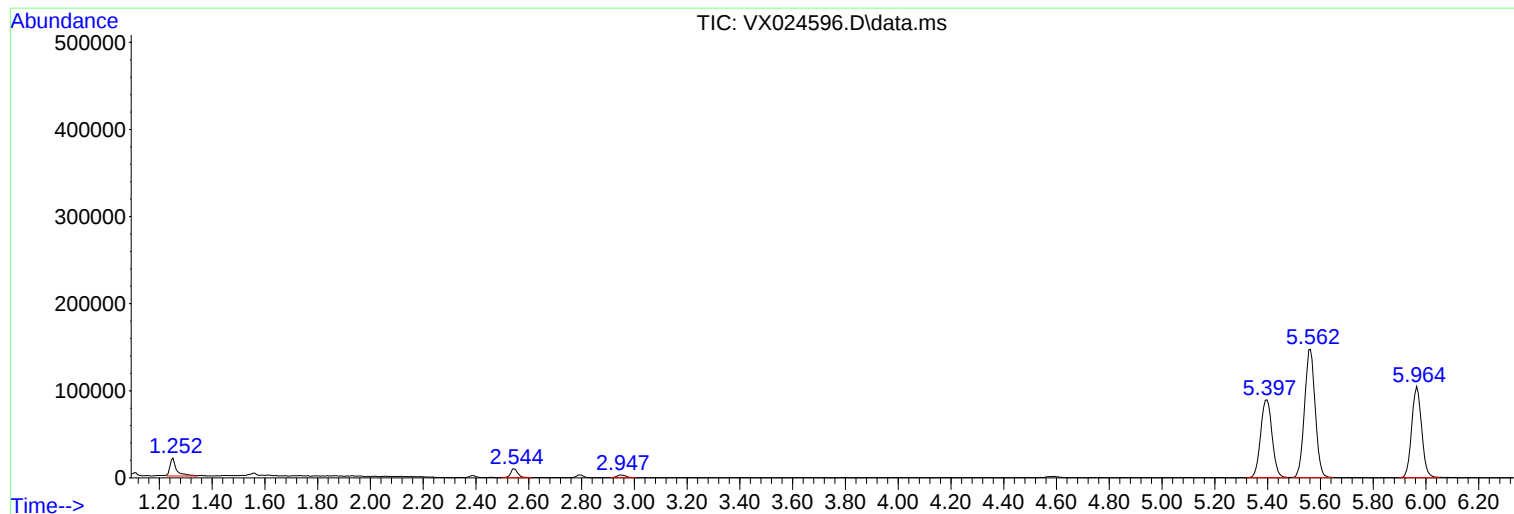

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024596.D
Acq On : 06 Oct 2021 02:11
Operator : JC/MD
Sample : M4028-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024596.D
Acq On : 06 Oct 2021 02:11
Operator : JC/MD
Sample : M4028-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
