

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
 Data File : VX024597.D
 Acq On : 06 Oct 2021 02:35
 Operator : JC/MD
 Sample : M4055-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20210927

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	22	27	34	rBV2	24251	34913	4.72%	0.816%
2	2.544	229	239	249	rBV	18483	35082	4.74%	0.819%
3	2.794	275	280	286	rVB3	4343	7710	1.04%	0.180%
4	2.947	298	305	315	rBV	3707	8415	1.14%	0.197%
5	5.397	696	707	721	rBV2	101975	295246	39.93%	6.896%
6	5.562	721	734	746	rBV2	156973	445597	60.26%	10.408%
7	5.964	789	800	818	rBV	109690	286878	38.79%	6.701%
8	6.769	922	932	947	rBV	253543	604658	81.77%	14.124%
9	8.653	1234	1241	1256	rBV	483458	739472	100.00%	17.273%
10	10.055	1465	1471	1487	rBV	547879	732519	99.06%	17.110%
11	11.085	1634	1640	1653	rVB	387626	491368	66.45%	11.478%
12	12.024	1789	1794	1804	rBV	494862	599265	81.04%	13.998%




Sum of corrected areas: 4281123

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024597.D
Acq On : 06 Oct 2021 02:35
Operator : JC/MD
Sample : M4055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20210927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

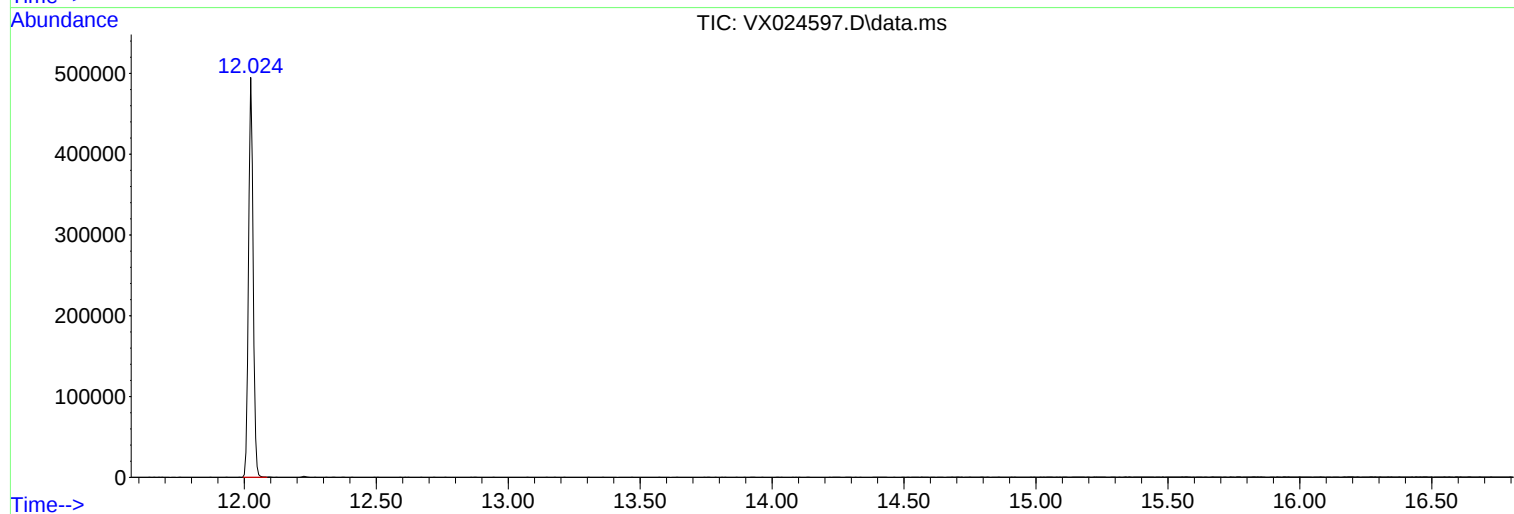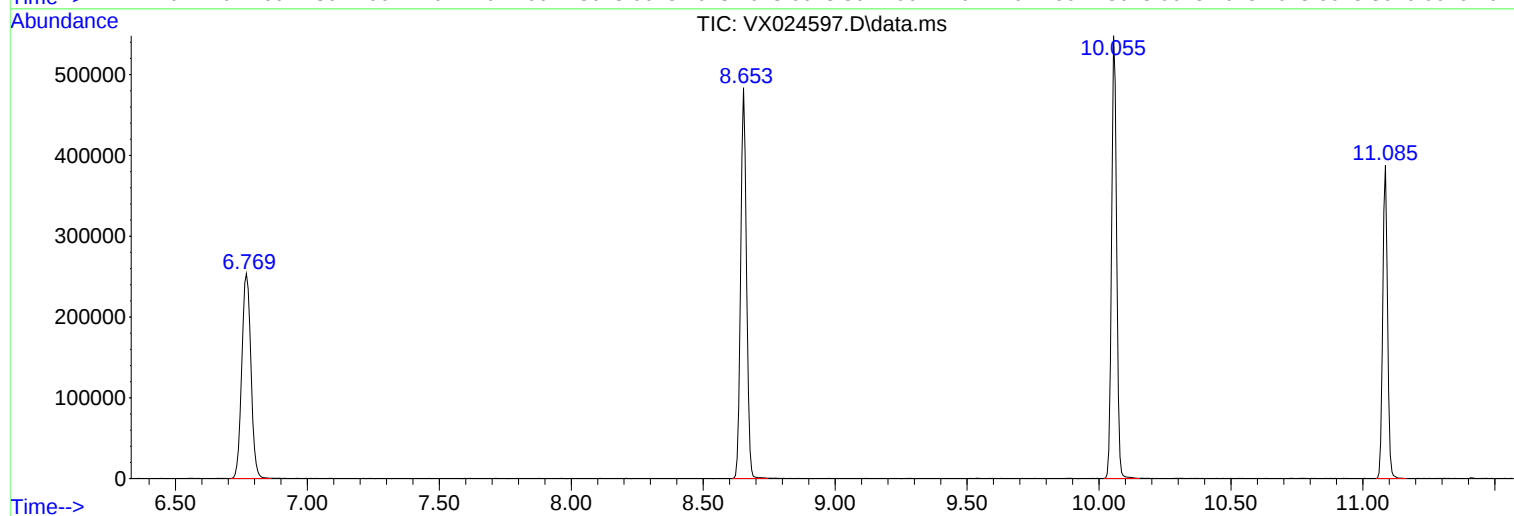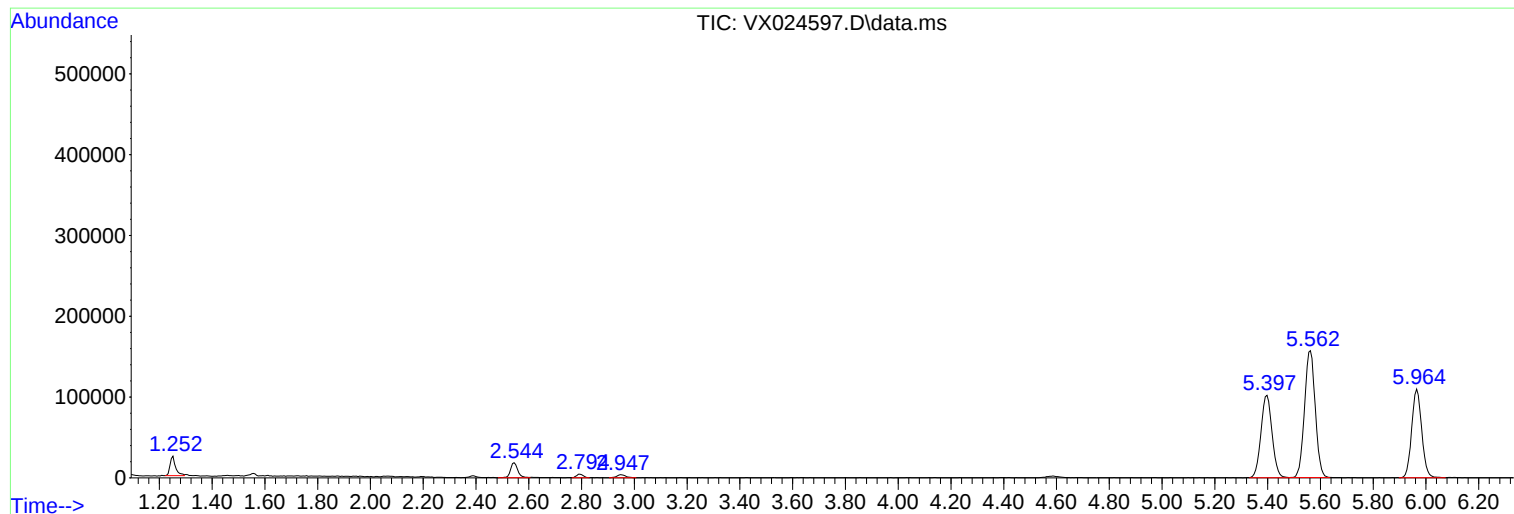

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024597.D
Acq On : 06 Oct 2021 02:35
Operator : JC/MD
Sample : M4055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20210927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100521\
Data File : VX024597.D
Acq On : 06 Oct 2021 02:35
Operator : JC/MD
Sample : M4055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20210927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
