


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100522\  
Data File : VX031881.D  
Acq On : 05 Oct 2022 09:19  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100522W.M  
Title : SW846 8260  
Last Update : Wed Oct 05 12:20:53 2022

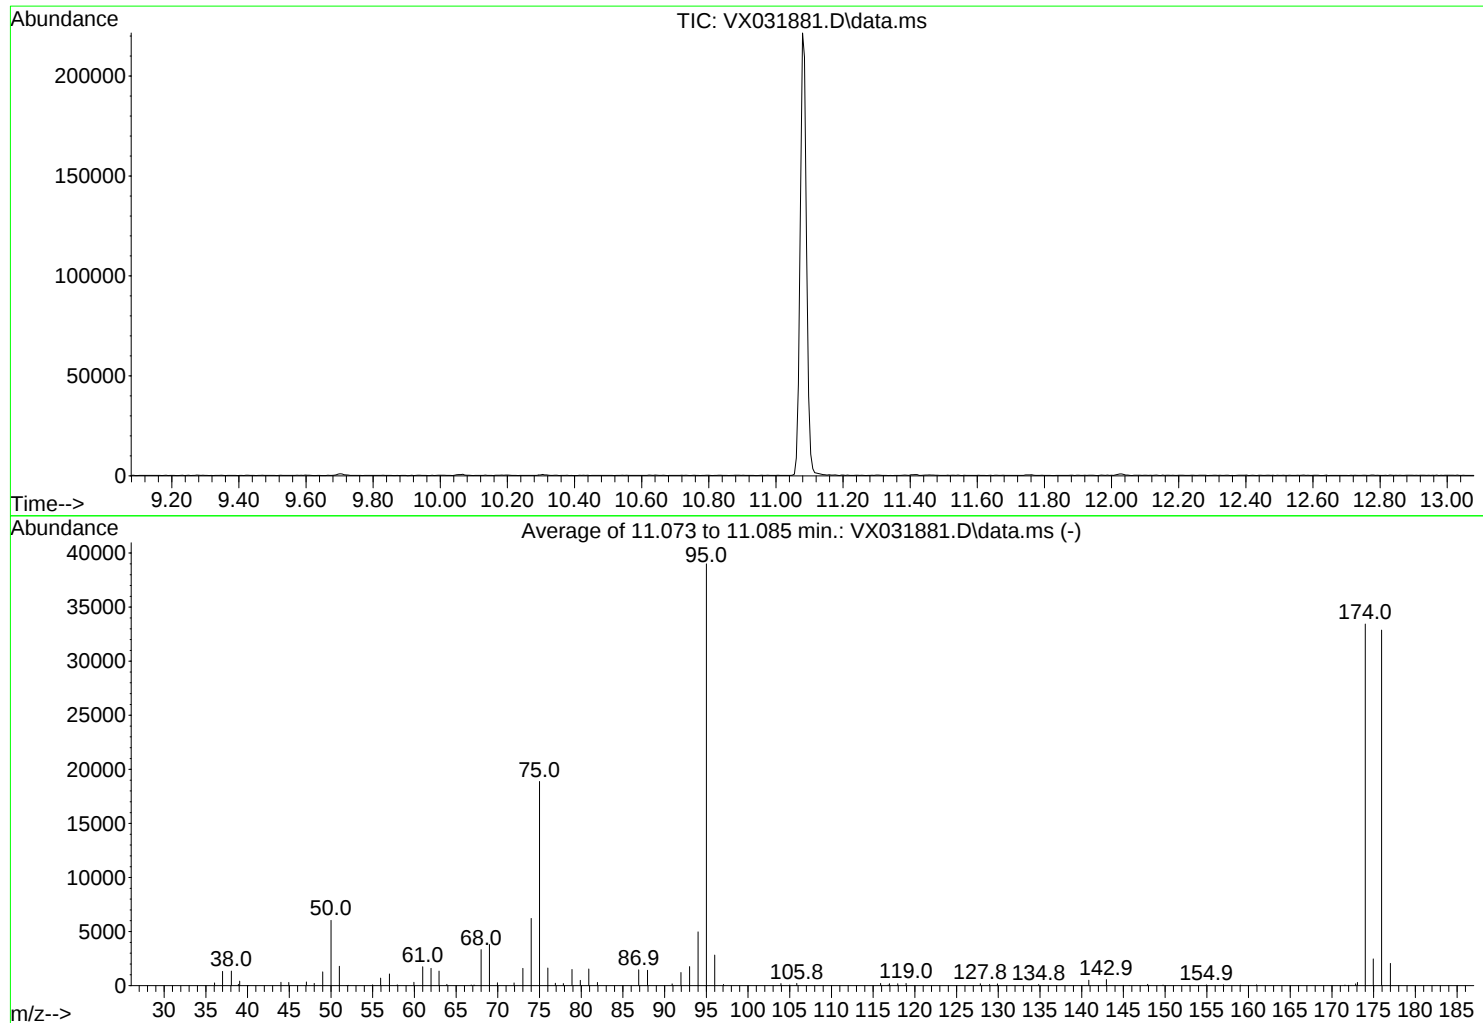

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 15.5  | 6044  | PASS      |
| 75     | 95      | 30     | 60     | 48.4  | 18874 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 39003 | PASS      |
| 96     | 95      | 5      | 9      | 7.2   | 2820  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.9   | 296   | PASS      |
| 174    | 95      | 50     | 100    | 85.7  | 33440 | PASS      |
| 175    | 174     | 5      | 9      | 7.4   | 2479  | PASS      |
| 176    | 174     | 95     | 101    | 98.3  | 32869 | PASS      |
| 177    | 176     | 5      | 9      | 6.2   | 2054  | PASS      |