



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100523\
Data File : VX038089.D
Acq On : 05 Oct 2023 08:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X092723W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Sep 28 06:08:32 2023

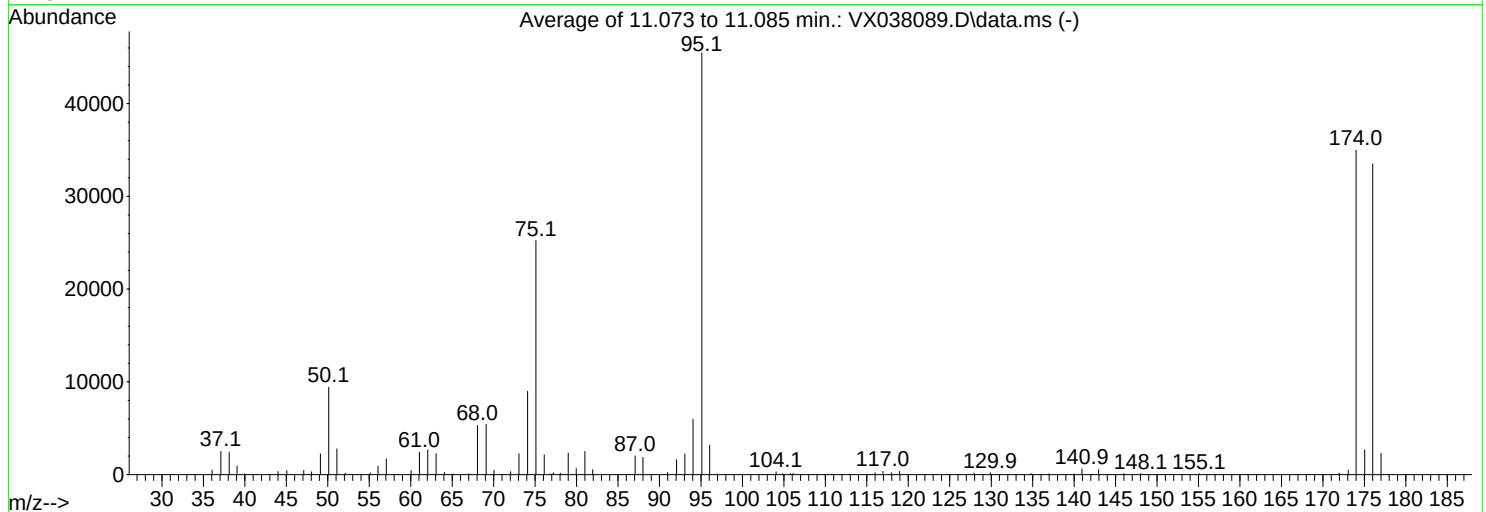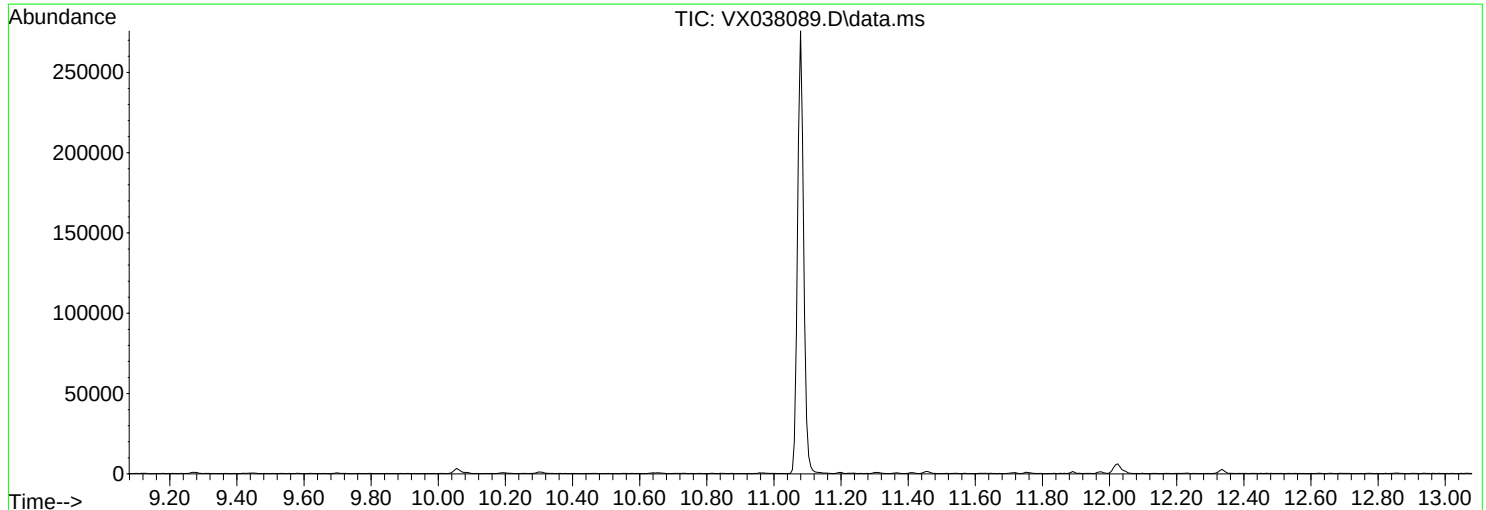

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	9412	PASS
75	95	30	60	55.5	25229	PASS
95	95	100	100	100.0	45467	PASS
96	95	5	9	7.0	3182	PASS
173	174	0.00	2	1.4	476	PASS
174	95	50	100	76.9	34979	PASS
175	174	5	9	7.6	2672	PASS
176	174	95	101	95.8	33499	PASS
177	176	5	9	6.9	2303	PASS