

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100620\
 Data File : VX018808.D
 Acq On : 06 Oct 2020 18:56
 Operator : JC/SP
 Sample : L4239-06DL 100X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6DL

Quant Time: Oct 07 01:34:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 07 01:30:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	125157	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	119254	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	62180	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	32044	4.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.60%
7) Chloroethane-d5	1.70	69	30233	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.60%
11) 1,1-Dichloroethene-d2	2.34	63	58993	3.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.60%
20) 2-Butanone-d5	4.55	46	128196	66.85	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	133.70%#
24) Chloroform-d	5.14	84	88288	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
26) 1,2-Dichloroethane-d4	6.03	65	53073	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.20%
32) Benzene-d6	6.04	84	156582	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
36) 1,2-Dichloropropane-d6	7.37	67	48435	5.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.00%
41) Toluene-d8	8.70	98	138061	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
45) trans-1,3-Dichloropropene-	8.99	79	21877	4.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.80%
48) 2-Hexanone-d5	9.43	63	101060	65.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	130.84%#
59) 1,1,2,2-Tetrachloroethane-	11.23	84	39240	5.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.60%
65) 1,2-Dichlorobenzene-d4	12.36	152	60860	5.31	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
12) 1,1-Dichloroethene	2.35	96	4780	0.767	ug/L #	1
13) Acetone	2.46	43	1029	0.983	ug/L	80
15) Methyl Acetate	2.82	43	2269	0.882	ug/L #	50
16) Methylene chloride	2.84	84	4183	0.553	ug/L	84
18) trans-1,2-Dichloroethene	3.14	96	1267	0.190	ug/L	84
19) 1,1-Dichloroethane	3.67	63	14277	1.203	ug/L	97
22) cis-1,2-Dichloroethene	4.56	96	555901	80.747	ug/L #	94
29) 1,1,1-Trichloroethane	5.46	97	849696	60.230	ug/L	100
30) Cyclohexane	5.55	56	7572	0.774	ug/L	90
33) Benzene	6.12	78	3316	0.133	ug/L	100
34) Trichloroethene	7.19	95	6332	0.859	ug/L	96
35) Methylcyclohexane	7.37	83	13197	1.263	ug/L #	19
37) 1,2-Dichloropropane	7.36	63	6848	1.095	ug/L #	83
39) cis-1,3-Dichloropropene	8.37	75	1803	0.181	ug/L	83
40) 4-Methyl-2-pentanone	8.77	43	38956	10.748	ug/L #	44
42) Toluene	8.77	91	5455621	199.647	ug/L	97
43) 1,3,5-Trimethylbenzene	11.49	105	52420	2.027	ug/L	97

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100620\
 Data File : VX018808.D
 Acq On : 06 Oct 2020 18:56
 Operator : JC/SP
 Sample : L4239-06DL 100X
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6DL

Quant Time: Oct 07 01:34:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Oct 07 01:30:09 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) 1,2,4-Trimethylbenzene	11.79	105	184553	7.030	ug/L	94
46) trans-1,3-Dichloropropene	8.77	75	44157	4.789	ug/L #	1
50) 2-Hexanone	9.43	43	12888	4.896	ug/L #	71
53) Chlorobenzene	10.12	112	2389	0.128	ug/L #	90
54) Ethylbenzene	10.24	91	43416	1.417	ug/L	97
55) m,p-xylene	10.34	106	58521	4.898	ug/L	91
56) o-xylene	10.68	106	40705	3.686	ug/L	93
57) Styrene	10.68	104	2353	0.125	ug/L #	1
58) Isopropylbenzene	11.00	105	9337	0.302	ug/L	95
66) 1,2-Dichlorobenzene	12.38	146	1841	0.130	ug/L #	87
69) 1,2,4-trichlorobenzene	13.63	180	731	0.076	ug/L #	84
70) Naphthalene	13.82	128	19095	1.210	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100620\
Data File : VX018808.D
Acq On : 06 Oct 2020 18:56
Operator : JC/SP
Sample : L4239-06DL 100X
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BG3N6DL

Quant Time: Oct 07 01:34:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Oct 07 01:30:09 2020
Response via : Initial Calibration

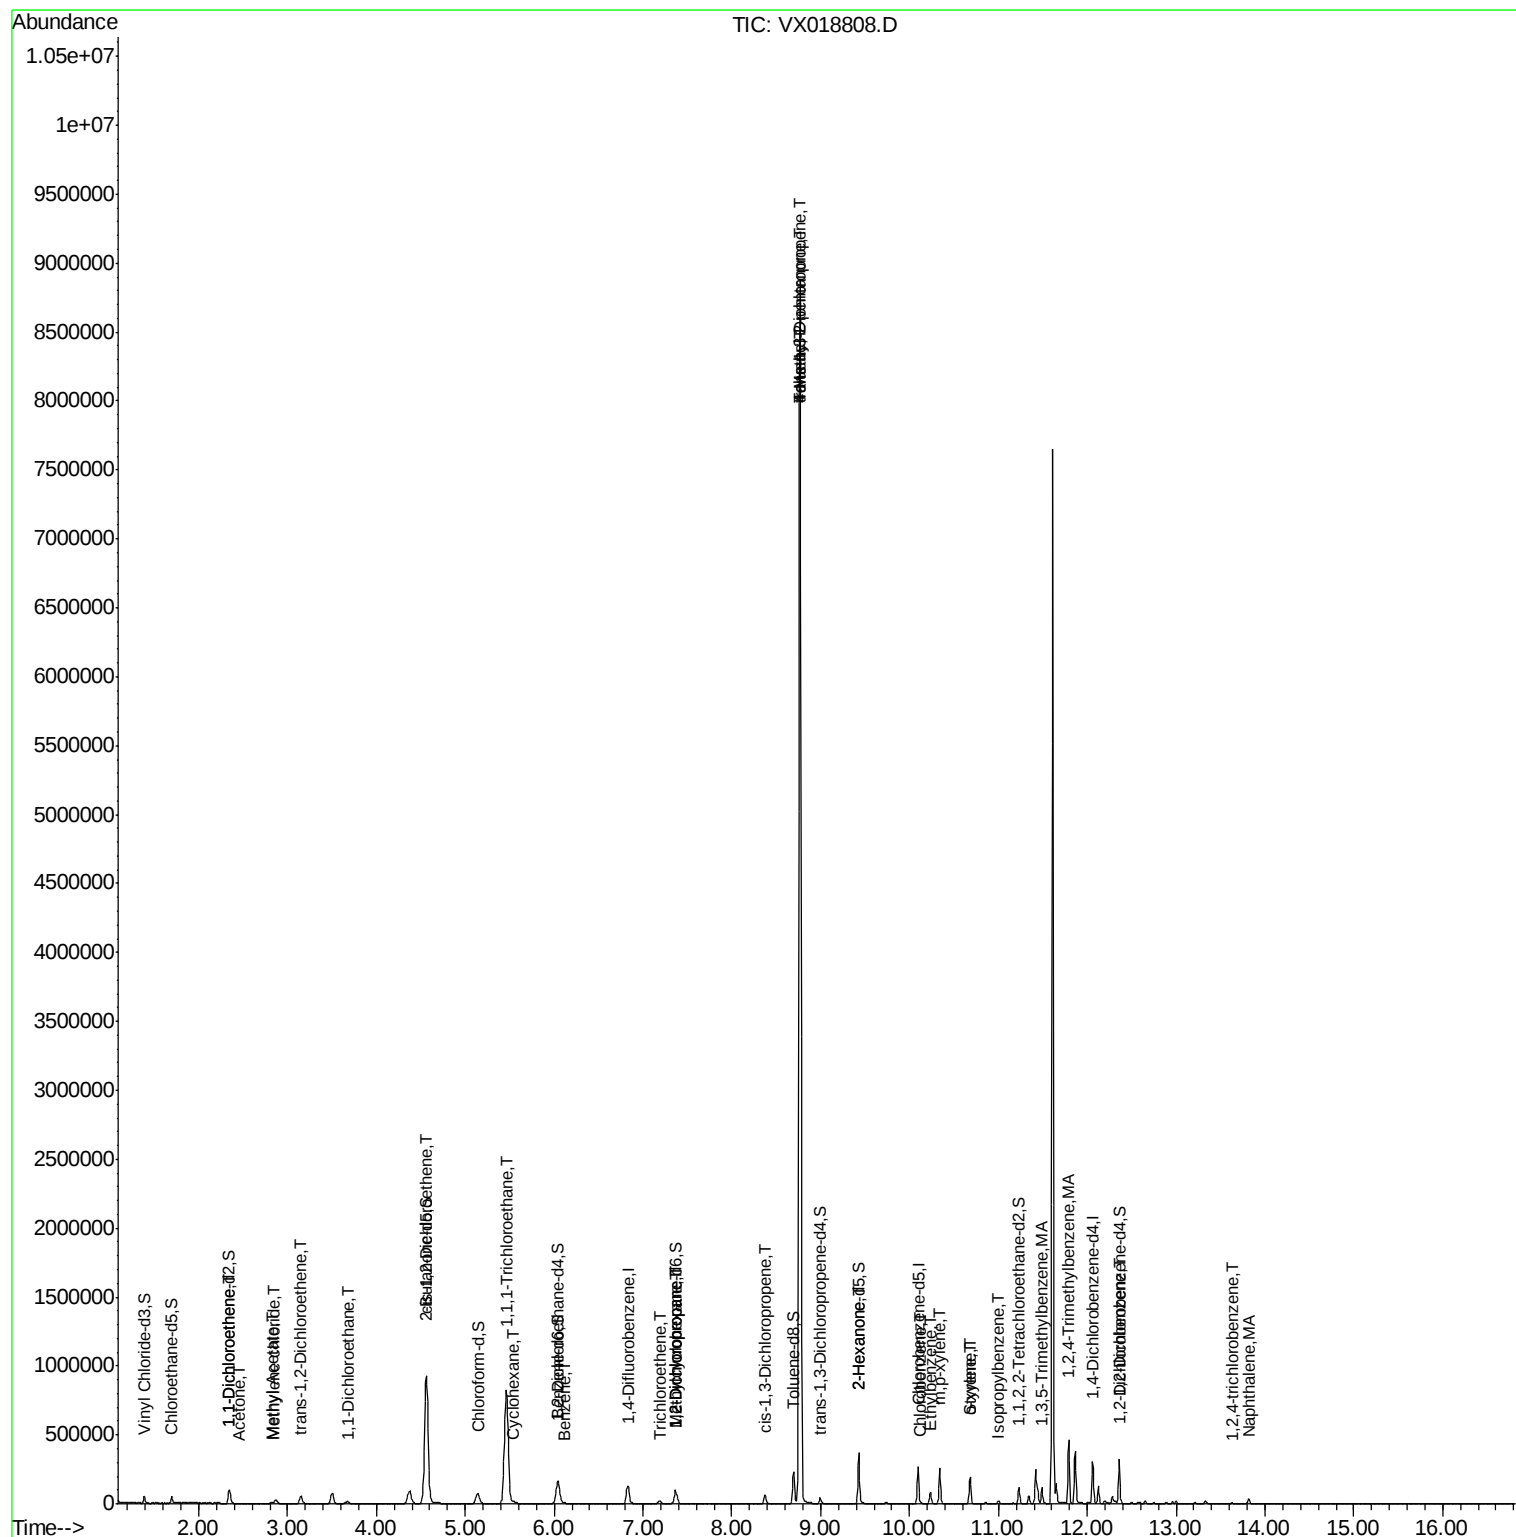

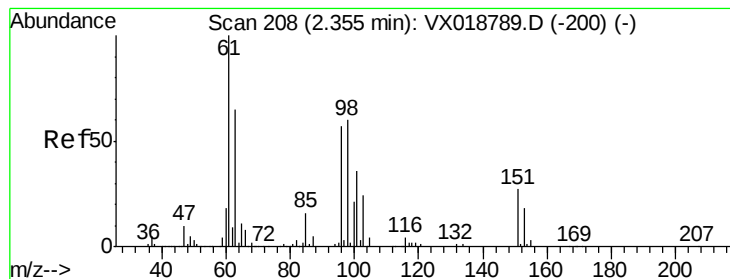

#12

1,1-Dichloroethene

Concen: 0.767 ug/L

RT: 2.35 min Scan# 207

Delta R.T. -0.01 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Instrument :

MSVOA_X

ClientSampleId :

BG3N6DL


Tot Ion: 96 Resp: 4780

Ion Ratio Lower Upper




96 100

61 262.6 133.2 247.4#

63 1238.5 115.1 213.7#



Abundance Ion 96.00 (95.70 to 96.70): VX0
Ion 61.05 (60.75 to 61.75): VX0
Ion 63.00 (62.70 to 63.70): VX0

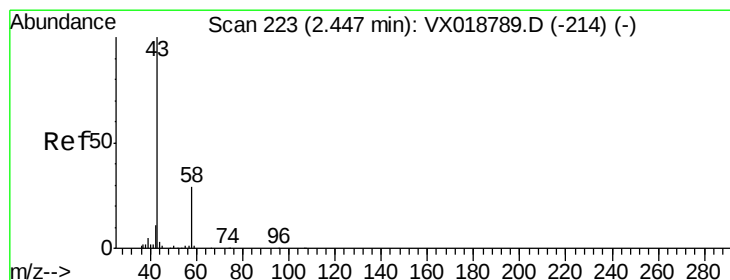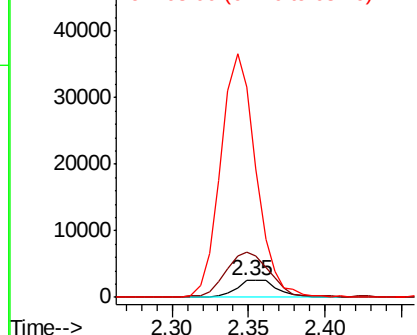

#13

Acetone

Concen: 0.983 ug/L

RT: 2.46 min Scan# 226

Delta R.T. 0.02 min

Lab File: VX018808.D


Acq: 06 Oct 2020 18:56

Tgt Ion: 43 Resp: 1029



Ion Ratio Lower Upper


43 100

58 17.6 0.0 56.4



Abundance Ion 43.05 (42.75 to 43.75): VX0
Ion 58.05 (57.75 to 58.75): VX0



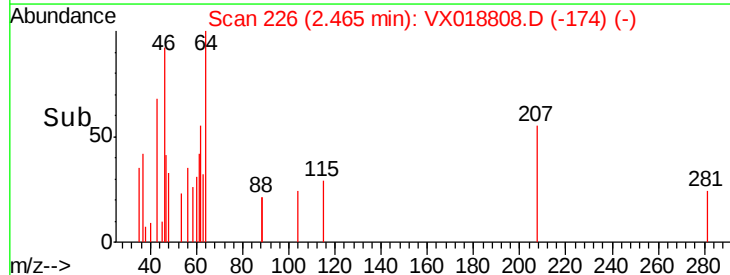
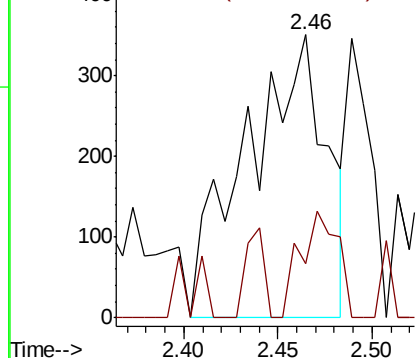


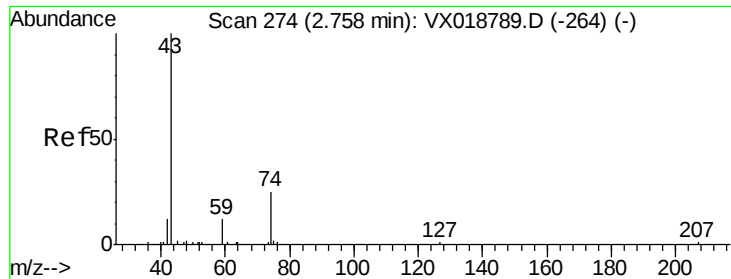

#15
Methyl Acetate
Concen: 0.882 ug/L
RT: 2.82 min Scan# 285
Delta R.T. 0.07 min
Lab File: VX018808.D
Acq: 06 Oct 2020 18:56




Instrument :
MSVOA_X
ClientSampled :
BG3N6DL


Tot Ion: 43 Resp: 2269
Ion Ratio Lower Upper
43 100
74 1.5 21.9 32.9#

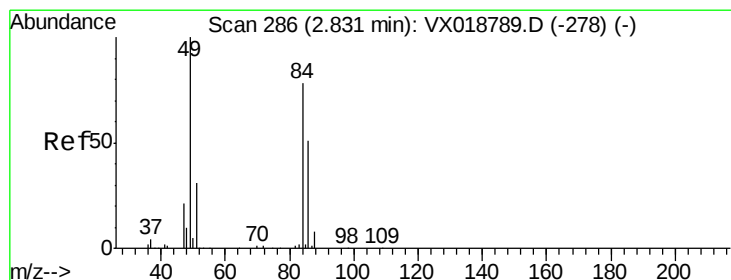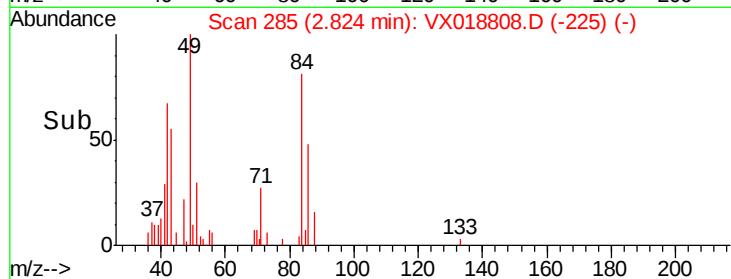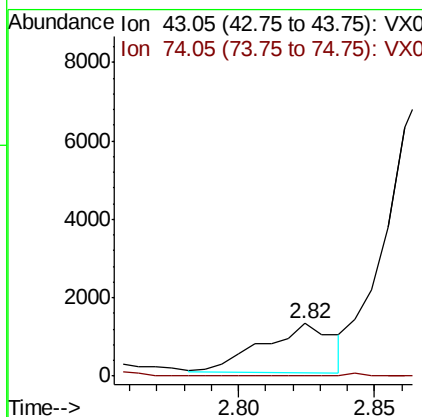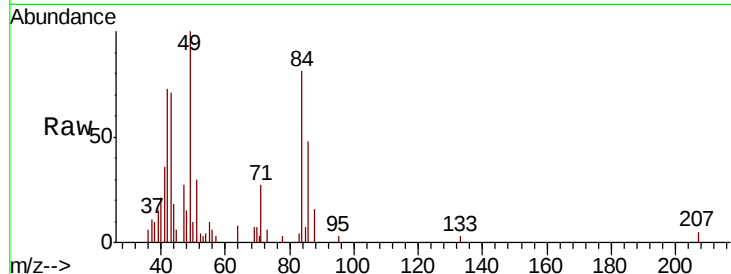

#16
Methylene chloride
Concen: 0.553 ug/L
RT: 2.84 min Scan# 287
Delta R.T. 0.01 min
Lab File: VX018808.D
Acq: 06 Oct 2020 18:56

Tgt Ion: 84 Resp: 4183
Ion Ratio Lower Upper
84 100
86 61.1 45.6 84.8
49 97.8 85.8 159.3


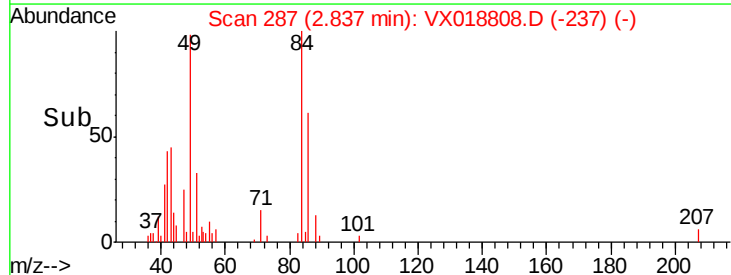
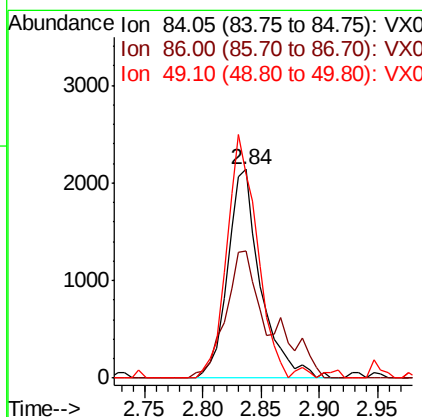





#18
trans-1,2-Dichloroethene
Concen: 0.190 ug/L
RT: 3.14 min Scan# 337
Delta R.T. -0.00 min
Lab File: VX018808.D
Acq: 06 Oct 2020 18:56




Instrument :
MSVOA_X
ClientSampleId :
BG3N6DL


Tot Ion: 96 Resp: 1267
Ion Ratio Lower Upper
96 100
61 120.8 97.6 181.4
98 75.3 43.1 80.1

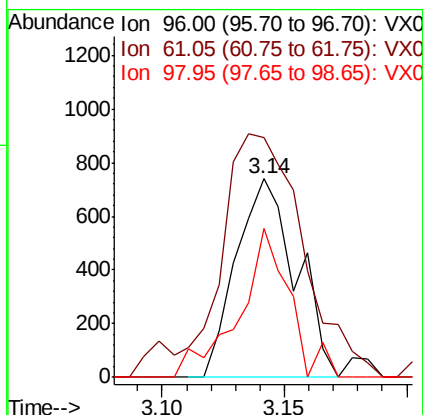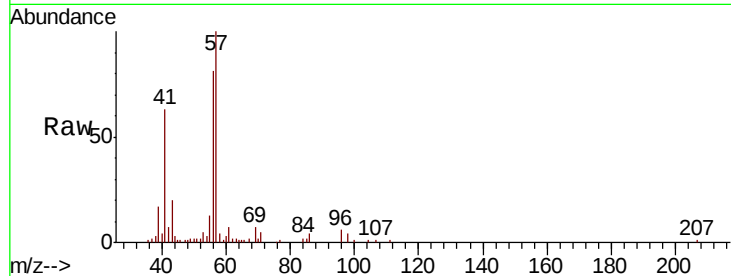

#19
1,1-Dichloroethane
Concen: 1.203 ug/L
RT: 3.67 min Scan# 424
Delta R.T. 0.01 min
Lab File: VX018808.D
Acq: 06 Oct 2020 18:56

Tgt Ion: 63 Resp: 14277
Ion Ratio Lower Upper
63 100
65 31.4 21.6 40.2
83 15.1 8.7 16.1

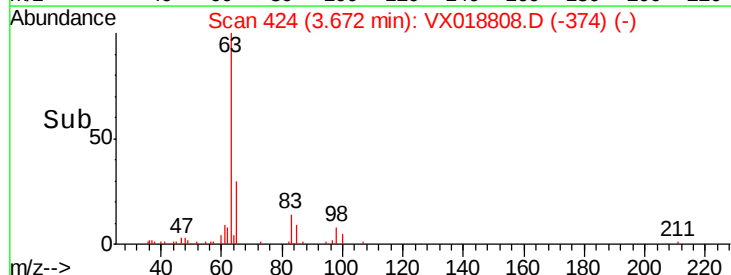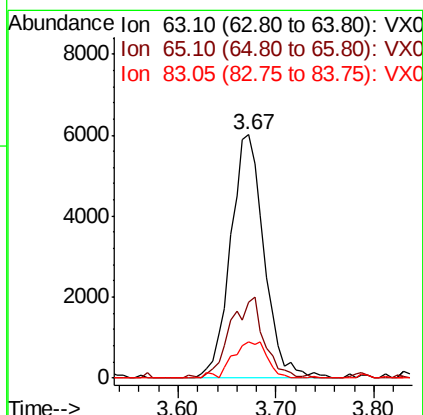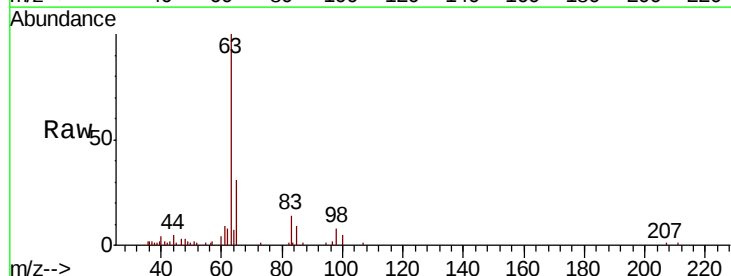




#22




cis-1,2-Dichloroethene
 Concen: 80.747 ug/L
 RT: 4.56 min Scan# 570
 Delta R.T. -0.00 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6DL

Tot Ion	Ratio	Lower	Upper
96	100		
61	130.1	86.2	160.0
68	0.0	0.3	0.7#

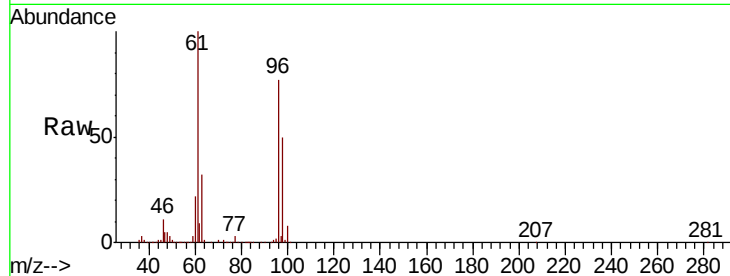


Abundance Ion 96.00 (95.70 to 96.70): VX0
 Ion 61.05 (60.75 to 61.75): VX0
 Ion 68.15 (67.85 to 68.85): VX0

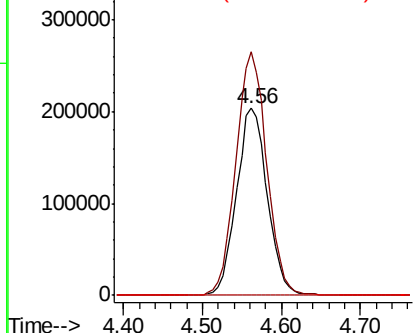



#29


1,1,1-Trichloroethane
 Concen: 60.230 ug/L
 RT: 5.46 min Scan# 718
 Delta R.T. 0.01 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Tgt Ion	Ratio	Lower	Upper
97	100		
99	64.5	51.3	76.9
61	41.8	33.3	49.9

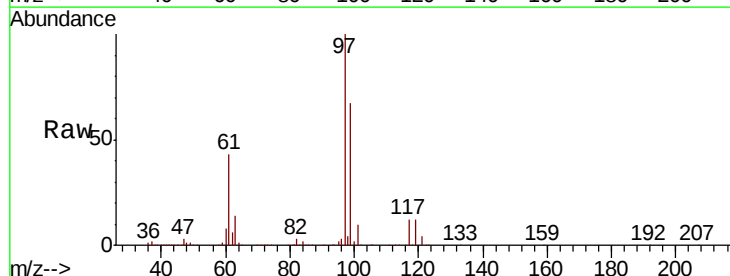

Abundance Ion 96.95 (96.65 to 97.65): VX0
 Ion 99.05 (98.75 to 99.75): VX0
 Ion 61.05 (60.75 to 61.75): VX0




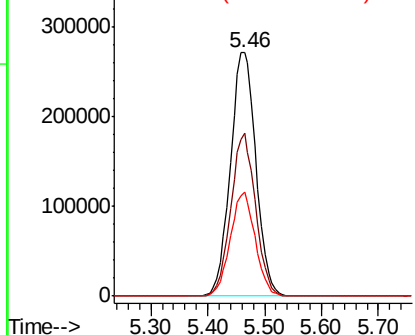




#30
Cyclohexane
Concen: 0.774 ug/L
RT: 5.55 min Scan# 732
Delta R.T. 0.01 min
Lab File: VX018808.D
Acq: 06 Oct 2020 18:56




Instrument :
MSVOA_X
ClientSampleId :
BG3N6DL


Tot Ion: 56 Resp: 7572
Ion Ratio Lower Upper
56 100
69 32.7 26.0 39.0
84 79.4 73.8 110.6

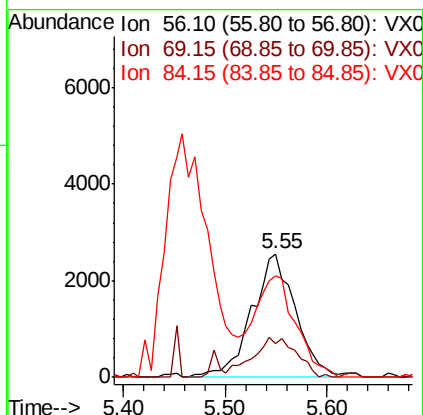

#33
Benzene
Concen: 0.133 ug/L
RT: 6.12 min Scan# 825
Delta R.T. 0.01 min
Lab File: VX018808.D
Acq: 06 Oct 2020 18:56

Tgt Ion: 78 Resp: 3316

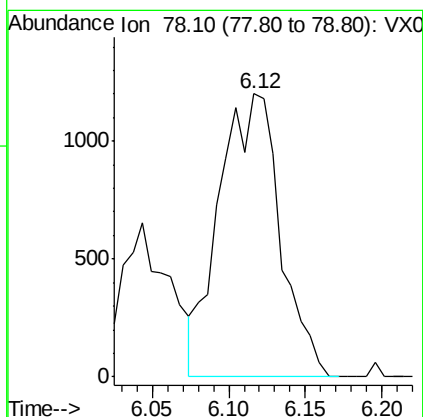







#34
 Trichloroethene
 Concen: 0.859 ug/L
 RT: 7.19 min Scan# 1001
 Delta R.T. 0.01 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6DL

Tot Ion: 95 Resp: 6332
 Ion Ratio Lower Upper
 95 100
 97 58.4 45.3 84.1
 132 97.3 68.6 127.4
 130 100.8 74.5 138.3

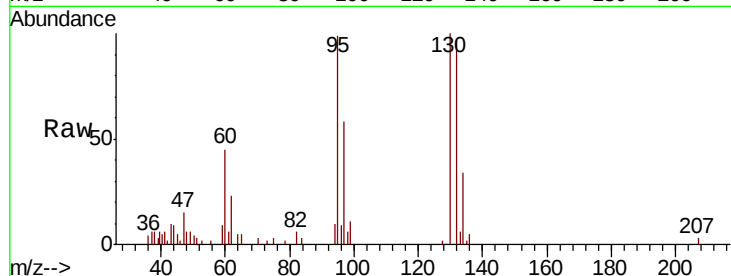


Abundance Ion 95.00 (94.70 to 95.70): VX0
 Ion 96.95 (96.65 to 97.65): VX0
 Ion 131.95 (131.65 to 132.65): V
 Ion 129.95 (129.65 to 130.65): V


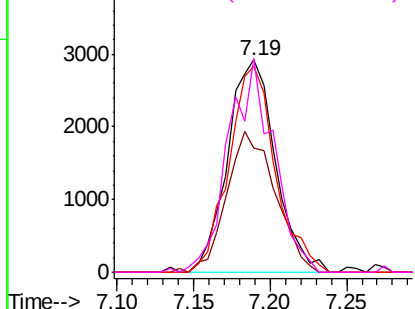



#35
 Methylcyclohexane
 Concen: 1.263 ug/L
 RT: 7.37 min Scan# 1030
 Delta R.T. -0.07 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Tgt Ion: 83 Resp: 13197
 Ion Ratio Lower Upper
 83 100
 55 0.6 60.3 90.5#
 98 0.3 39.4 59.0#



Abundance Ion 83.15 (82.85 to 83.85): VX0
 Ion 55.10 (54.80 to 55.80): VX0
 Ion 98.15 (97.85 to 98.85): VX0




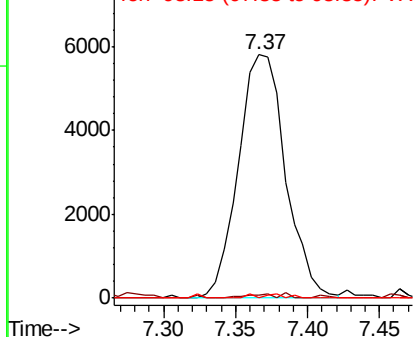




#37
 1,2-Dichloropropane
 Concen: 1.095 ug/L
 RT: 7.36 min Scan# 1029
 Delta R.T. -0.12 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56




Instrument :
 MSVOA_X
 ClientSampleId :
 BG3N6DL


Tot Ion: 63 Resp: 6848
 Ion Ratio Lower Upper
 63 100
 112 0.3 4.7 7.1#

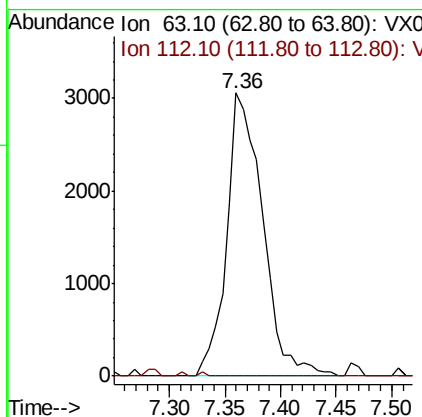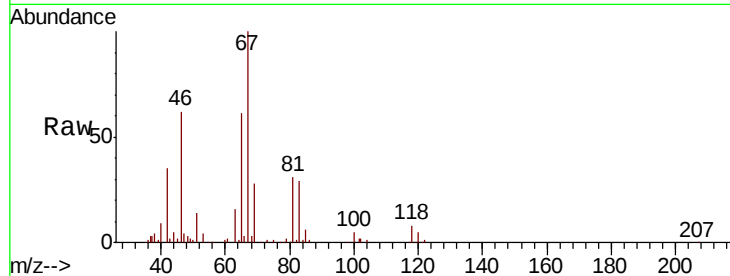

#39
 cis-1,3-Dichloropropene
 Concen: 0.181 ug/L
 RT: 8.37 min Scan# 1195
 Delta R.T. -0.04 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Tgt Ion: 75 Resp: 1803
 Ion Ratio Lower Upper
 75 100
 77 41.4 22.5 41.7



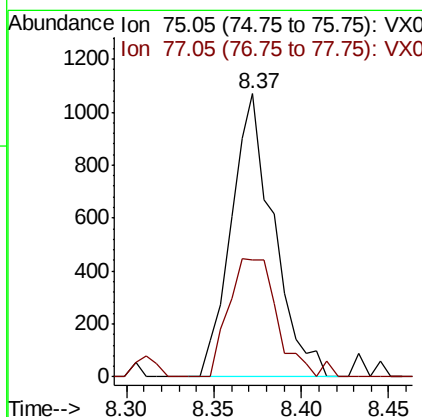
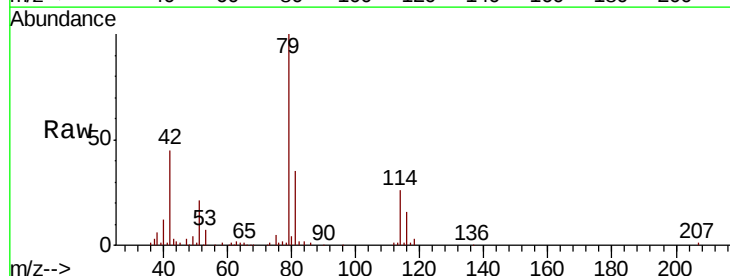




#40
 4-Methyl-2-pentanone
 Concen: 10.748 ug/L
 RT: 8.77 min Scan# 1260
 Delta R.T. 0.15 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56




Instrument :
 MSVOA_X
 ClientSampleID :
 BG3N6DL


Tot Ion	43	Resp	38956
Ion Ratio	Lower	Upper	
43	100		
58	0.3	30.8	46.2#
100	0.0	13.2	19.8#

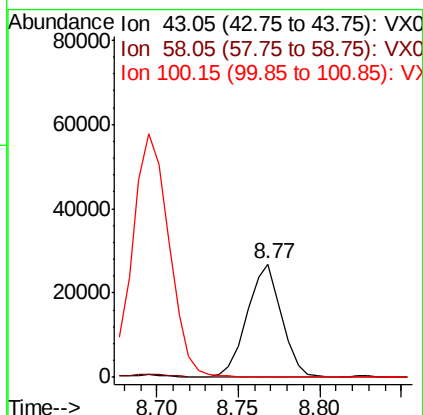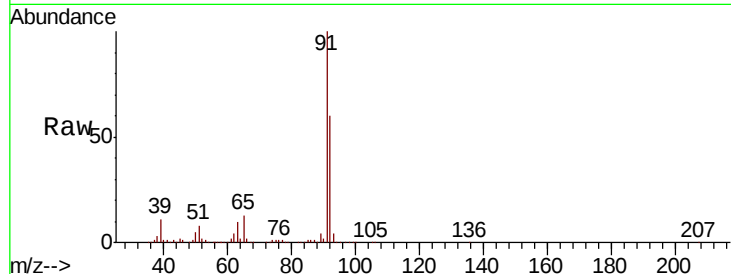

#42
 Toluene
 Concen: 199.647 ug/L
 RT: 8.77 min Scan# 1260
 Delta R.T. 0.01 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Tgt Ion	91	Resp	5455621
Ion Ratio	Lower	Upper	
91	100		
92	59.7	40.3	74.9



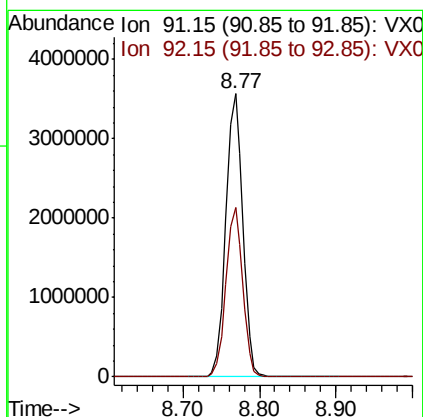
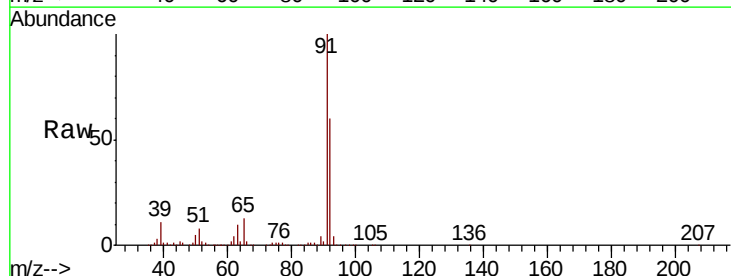




#43
 1,3,5-Trimethylbenzene
 Concen: 2.027 ug/L
 RT: 11.49 min Scan# 1707
 Delta R.T. 0.01 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56




Instrument :
 MSVOA_X
 ClientSampleID :
 BG3N6DL


Tot Ion:105 Resp: 52420
 Ion Ratio Lower Upper
 105 100
 120 49.4 37.7 56.5

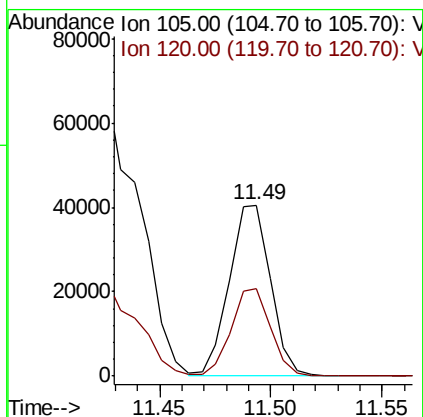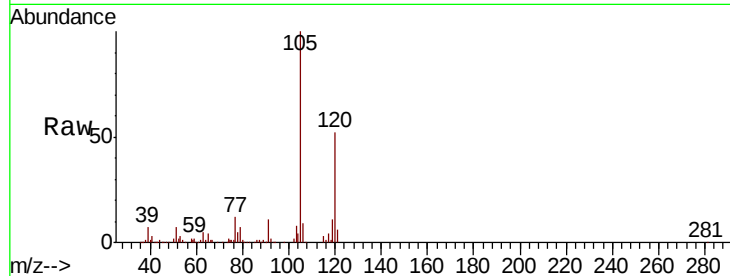

#44
 1,2,4-Trimethylbenzene
 Concen: 7.030 ug/L
 RT: 11.79 min Scan# 1756
 Delta R.T. -0.00 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Tgt Ion:105 Resp: 184553
 Ion Ratio Lower Upper
 105 100
 120 47.8 35.1 52.7

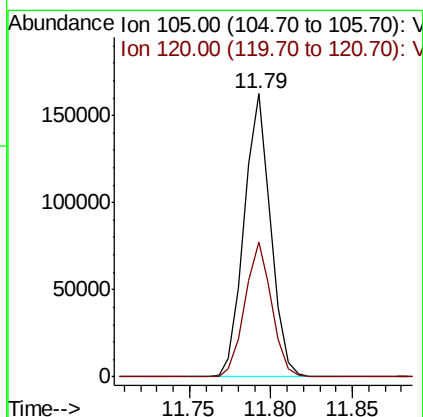



#46

trans-1,3-Dichloropropene

Concen: 4.789 ug/L

RT: 8.77 min Scan# 1260

Delta R.T. -0.25 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Instrument :

MSVOA_X

ClientSampled :


BG3N6DL

Tot Ion: 75 Resp: 44157

Ion Ratio Lower Upper




75 100

77 162.4 19.9 37.0#

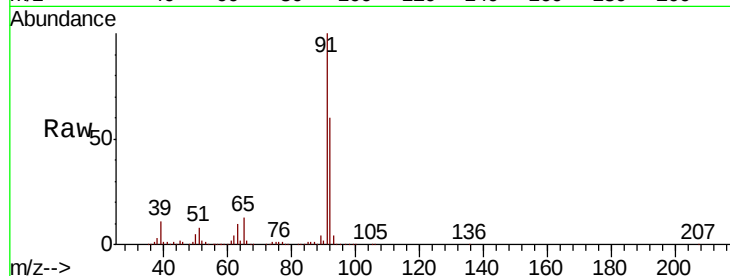

Abundance Ion 75.05 (74.75 to 75.75): VX0

Ion 77.05 (76.75 to 77.75): VX0

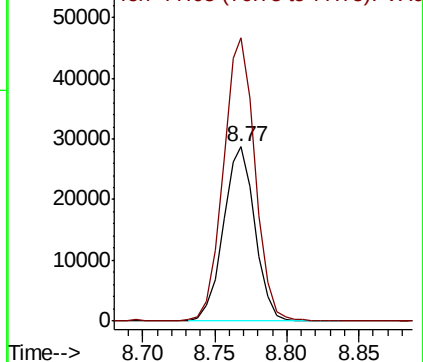

#50

2-Hexanone

Concen: 4.896 ug/L

RT: 9.43 min Scan# 1368

Delta R.T. -0.04 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Tgt Ion: 43 Resp: 12888


Ion Ratio Lower Upper

43 100

58 26.5 41.0 61.4#

57 25.8 15.9 23.9#

100 1.4 10.1 15.1#






Abundance Ion 43.05 (42.75 to 43.75): VX0

Ion 58.05 (57.75 to 58.75): VX0

Ion 57.20 (56.90 to 57.90): VX0

Ion 100.15 (99.85 to 100.85): VX0

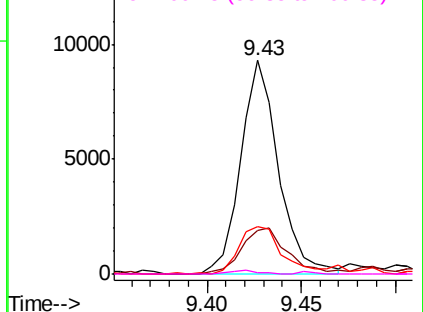



#53

Chlorobenzene

Concen: 0.128 ug/L

RT: 10.12 min Scan# 1482

Delta R.T. -0.00 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Instrument :

MSVOA_X

ClientSampleId :

BG3N6DL


Tot Ion: 112 Resp: 2389

Ion Ratio Lower Upper

112 100

114 41.0 21.3 39.5#




77 49.4 42.4 63.6

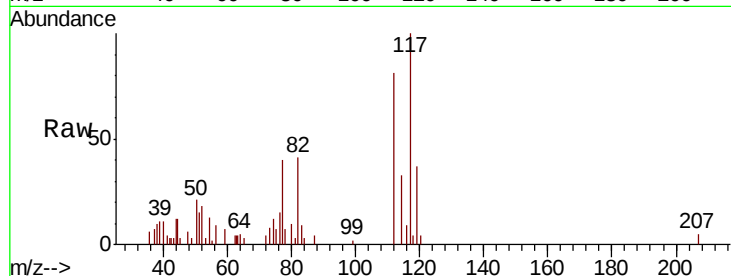

Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VX0

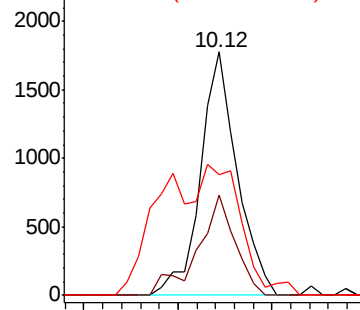

#54

Ethylbenzene

Concen: 1.417 ug/L

RT: 10.24 min Scan# 1501

Delta R.T. 0.01 min

Lab File: VX018808.D


Acq: 06 Oct 2020 18:56

Tgt Ion: 91 Resp: 43416

Ion Ratio Lower Upper



91 100


106 32.1 21.5 39.9



Abundance Ion 91.15 (90.85 to 91.85): VX0

Ion 106.15 (105.85 to 106.85): V

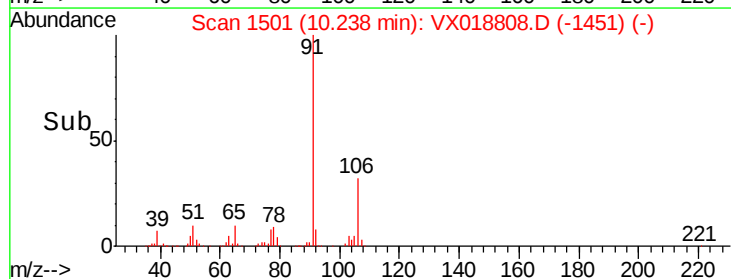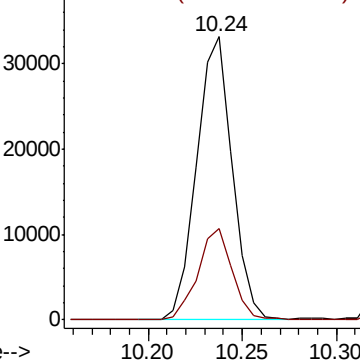

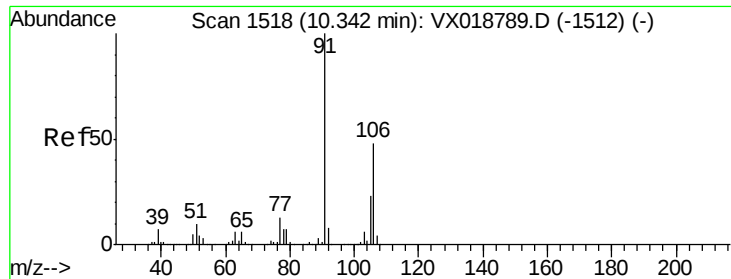

#55

m,p-xylene

Concen: 4.898 ug/L

RT: 10.34 min Scan# 1518

Delta R.T. -0.00 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Instrument :

MSVOA_X

ClientSampled :





BG3N6DL

Tot Ion:106 Resp: 58521

Ion Ratio Lower Upper

106 100

91 218.2 143.4 266.2

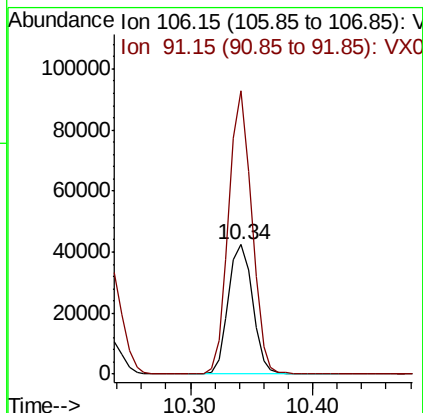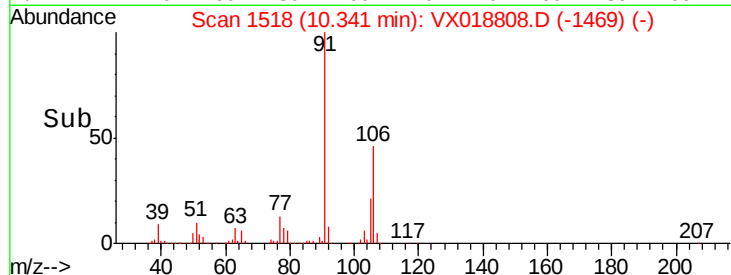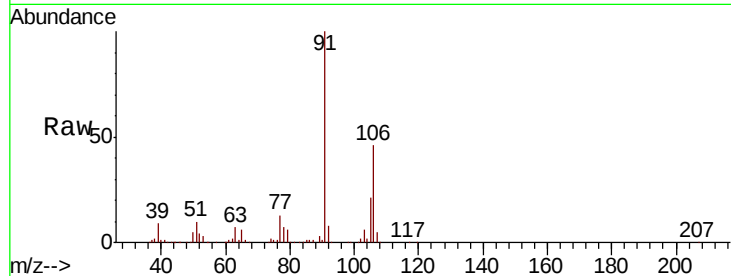

#56

o-xylene

Concen: 3.686 ug/L

RT: 10.68 min Scan# 1574

Delta R.T. -0.00 min

Lab File: VX018808.D




Acq: 06 Oct 2020 18:56


Tgt Ion:106 Resp: 40705

Ion Ratio Lower Upper

106 100

91 207.9 153.4 284.8

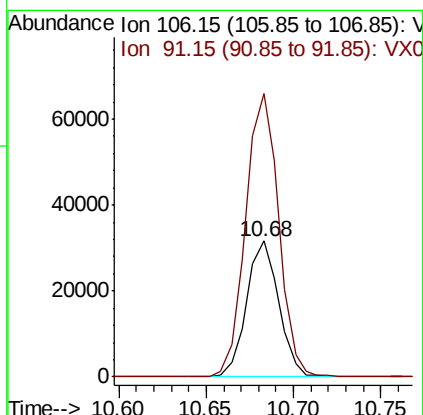

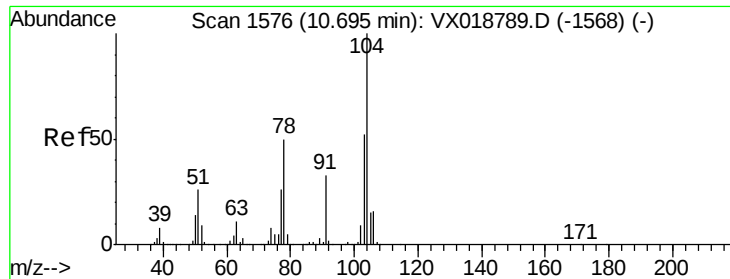

#57

Stvrene

Concen: 0.125 ug/L

RT: 10.68 min Scan# 1574

Delta R.T. -0.01 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Instrument :

MSVOA_X

ClientSampleId :


BG3N6DL

Tot Ion:104 Resp: 2353

Ion Ratio Lower Upper




104 100

78 339.5 37.1 68.9#

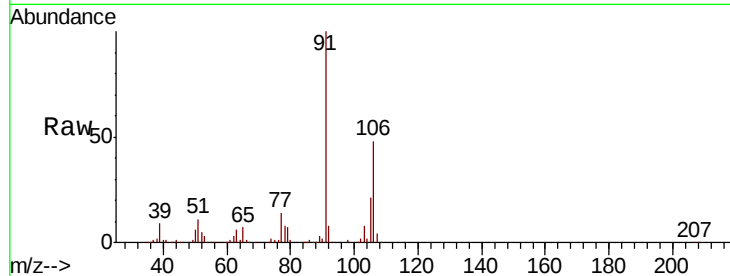

Abundance Ion 104.10 (103.80 to 104.80): V

Ion 78.10 (77.80 to 78.80): VX0

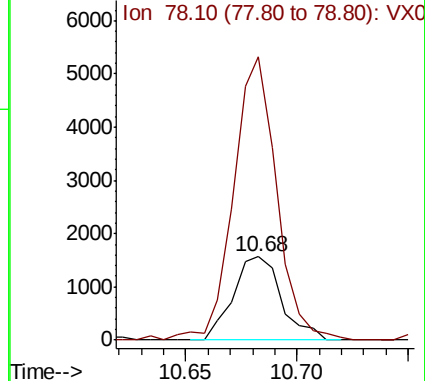

#58

Isopropylbenzene

Concen: 0.302 ug/L

RT: 11.00 min Scan# 1626

Delta R.T. -0.00 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56


Tgt Ion:105 Resp: 9337

Ion Ratio Lower Upper

105 100

120 27.9 20.2 30.2



77 18.0 13.3 19.9




Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VX0




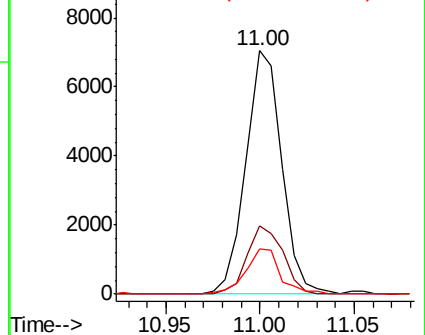




#66
 1,2-Dichlorobenzene
 Concen: 0.130 ug/L
 RT: 12.38 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56




Instrument :
 MSVOA_X
 ClientSampleID :
 BG3N6DL


Tot Ion	Ratio	Lower	Upper
146	100		
111	26.0	31.7	47.5#
148	56.2	49.0	73.6

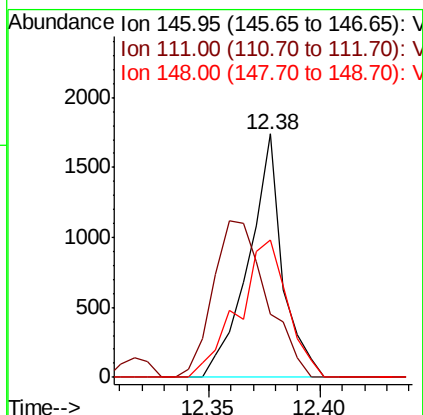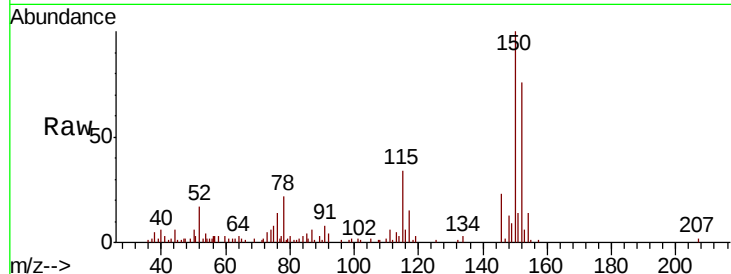

#69
 1,2,4-trichlorobenzene
 Concen: 0.076 ug/L
 RT: 13.63 min Scan# 2058
 Delta R.T. 0.01 min
 Lab File: VX018808.D
 Acq: 06 Oct 2020 18:56

Tgt Ion	Ratio	Lower	Upper
180	100		
182	80.2	80.2	120.4#
145	29.7	25.2	37.8

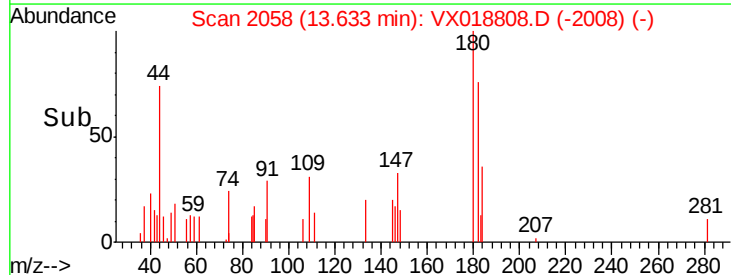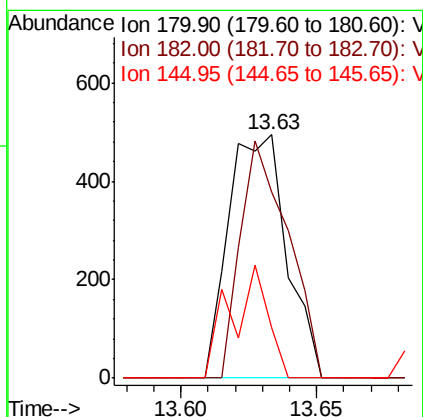

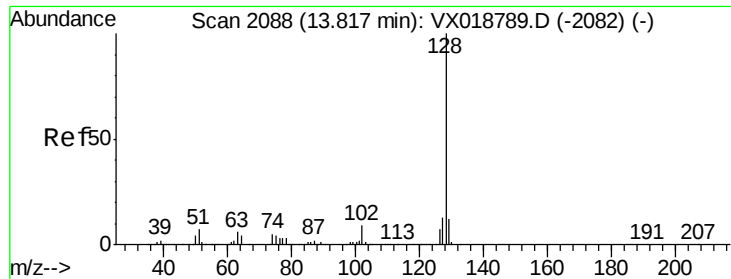

#70

Naphthalene

Concen: 1.210 ug/L

RT: 13.82 min Scan# 2088

Delta R.T. -0.00 min

Lab File: VX018808.D

Acq: 06 Oct 2020 18:56

Instrument :

MSVOA_X

ClientSampleId :

BG3N6DL


Tot Ion:128 Resp: 19095

Ion Ratio Lower Upper

128 100

129 11.5 9.0 13.4

127 13.7 10.5 15.7



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

