


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100620\
Data File : VX018788.D
Acq On : 06 Oct 2020 08:53
Operator : JC/SP
Sample : BFB78
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB78

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Oct 07 12:19:55 2020

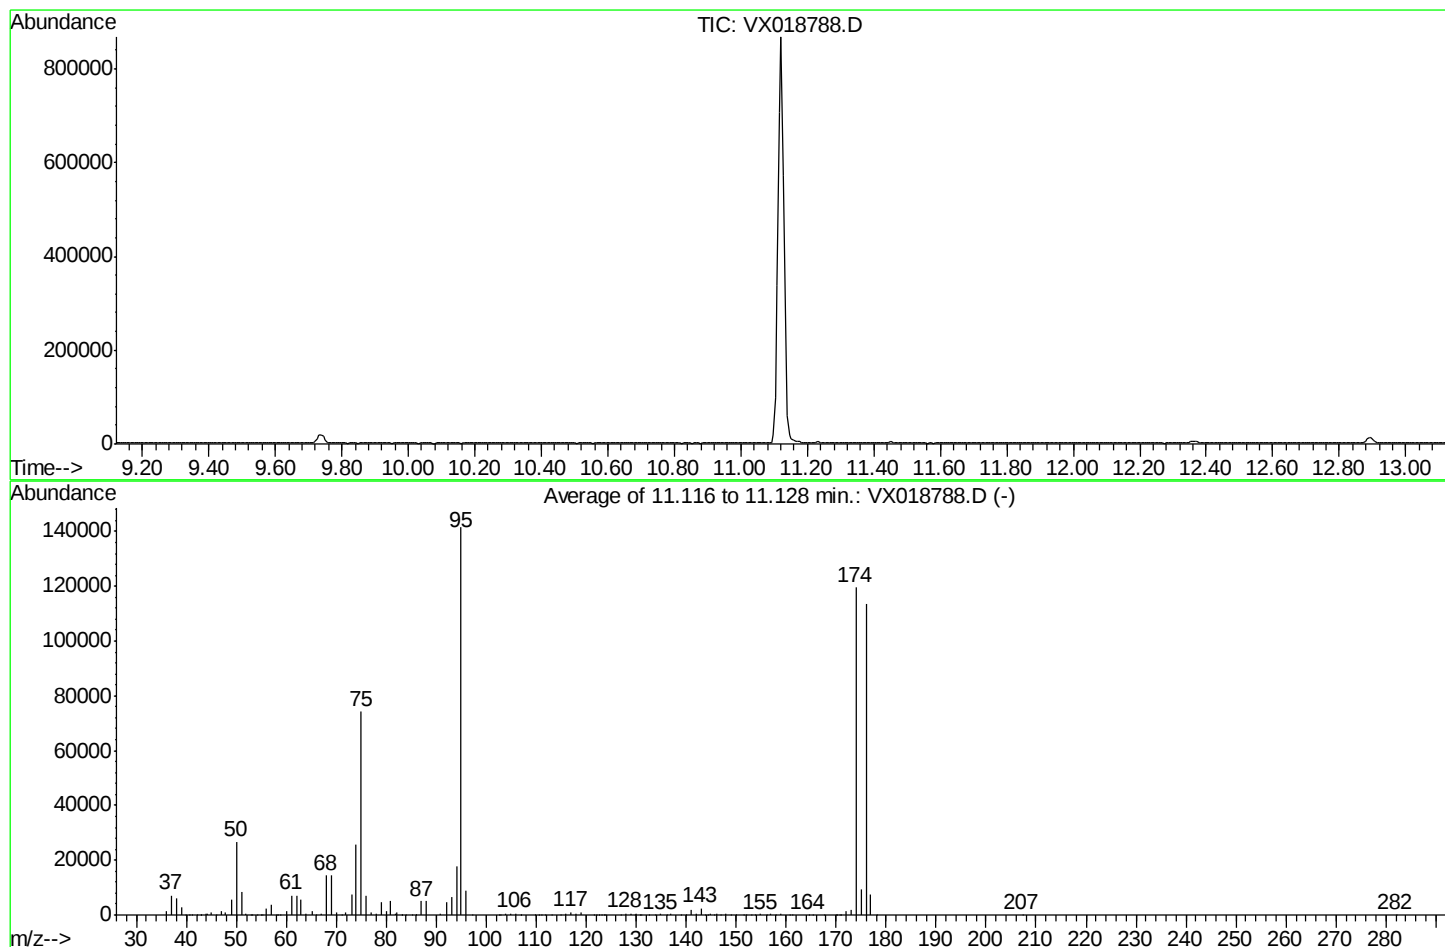

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	26730	PASS
75	95	30	80	52.4	74216	PASS
95	95	100	100	100.0	141501	PASS
96	95	5	9	6.3	8946	PASS
173	174	0.00	2	1.6	1970	PASS
174	95	50	120	84.4	119461	PASS
175	174	5	9	7.8	9347	PASS
176	174	95	101	95.1	113584	PASS
177	176	5	9	6.7	7628	PASS

m/z	Abundance
36.00	1338.0
37.00	8567.0
38.00	7052.0
39.00	3440.0
40.00	308.0
41.20	177.0
42.20	145.0
42.80	155.0
43.90	1124.0
45.00	1192.0
45.90	168.0
47.00	1641.0
47.90	1157.0
49.00	6169.0
50.00	28744.0
51.00	8952.0
52.00	391.0
53.20	203.0
54.10	207.0
55.00	422.0
56.00	2715.0
57.00	3854.0
57.90	198.0
58.80	85.0
60.00	1823.0
61.00	7875.0
62.00	8110.0
63.00	6020.0
64.00	907.0
65.10	1690.0
65.90	119.0
67.10	506.0
68.00	15372.0
69.00	15939.0
70.00	1253.0
71.00	115.0
71.90	875.0
73.00	7685.0
74.00	25456.0
75.00	78152.0
76.00	7607.0
77.00	1153.0
78.00	657.0
78.90	4564.0
79.90	1408.0
80.90	5721.0
81.80	1248.0
83.00	109.0
83.80	53.0
85.10	72.0
85.80	229.0
87.00	5054.0
87.90	4694.0
90.90	833.0
92.00	5024.0
93.00	6518.0
94.00	18112.0
95.00	141696.0
96.00	9836.0
97.10	239.0
103.00	159.0
103.90	565.0
104.90	270.0
105.90	497.0
106.80	224.0
109.90	173.0
110.60	158.0
111.10	96.0
111.80	102.0
112.90	176.0
114.80	156.0
116.00	559.0
117.00	1032.0
118.00	747.0
119.00	865.0
121.50	77.0
123.00	125.0
123.80	116.0
127.90	732.0
129.10	337.0
129.80	671.0
130.70	179.0
134.90	405.0
136.10	144.0
136.80	299.0
139.00	68.0
140.10	159.0
140.90	1856.0
141.80	238.0
142.90	2381.0
143.90	181.0
144.90	633.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78

145.70	195.0
146.10	200.0
146.80	177.0
147.90	317.0
148.90	159.0
150.10	202.0
152.10	54.0
153.00	116.0
153.80	140.0
155.00	490.0
156.90	270.0
158.90	221.0
160.70	116.0
161.10	92.0
170.80	337.0
171.90	1746.0
172.90	1819.0
174.00	107032.0
175.00	8281.0
176.00	99312.0
177.00	6756.0
178.00	187.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78

m/z	Abundance
36.00	1421.0
37.00	8361.0
38.00	6978.0
39.00	2893.0
39.90	233.0
40.80	145.0
42.10	135.0
42.80	219.0
44.10	1400.0
44.90	1292.0
45.90	241.0
46.90	1701.0
47.90	1276.0
49.00	6521.0
50.00	31480.0
51.00	10171.0
52.00	462.0
52.90	187.0
54.00	104.0
55.20	380.0
56.00	2200.0
57.00	4759.0
58.00	360.0
58.80	141.0
60.00	1449.0
61.00	8468.0
62.00	8297.0
63.00	7034.0
63.90	822.0
65.10	1524.0
65.80	127.0
67.00	487.0
68.00	17696.0
69.00	17592.0
70.00	1132.0
71.10	86.0
72.00	1023.0
73.00	9595.0
74.00	31824.0
75.00	89896.0
76.10	7949.0
77.10	797.0
77.90	651.0
78.90	6013.0
80.00	1816.0
80.90	5870.0
82.00	1316.0
83.20	198.0
85.10	98.0
86.00	246.0
87.00	6186.0
87.90	6183.0
90.90	624.0
92.00	5575.0
93.00	7811.0
94.00	21768.0
95.00	171840.0
96.00	10382.0
97.00	314.0
102.60	65.0
103.00	68.0
104.00	826.0
105.00	353.0
105.90	876.0
107.00	176.0
109.80	215.0
110.90	174.0
111.90	216.0
113.00	216.0
114.90	169.0
115.90	729.0
117.00	1461.0
118.00	683.0
118.90	1110.0
122.00	131.0
122.70	94.0
123.10	66.0
123.90	138.0
127.00	59.0
127.90	656.0
129.00	337.0
130.00	844.0
130.90	342.0
132.50	80.0
133.90	100.0
135.00	482.0
136.00	121.0
136.90	405.0
139.10	84.0
139.90	127.0
140.90	2438.0
141.90	315.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78

143.00	3261.0
143.70	251.0
144.80	627.0
146.10	392.0
146.80	114.0
148.00	538.0
149.00	118.0
149.90	186.0
152.00	76.0
152.90	129.0
153.90	167.0
154.80	509.0
156.90	509.0
158.10	95.0
159.00	383.0
161.10	175.0
164.50	75.0
167.70	71.0
170.20	81.0
170.80	315.0
172.00	1828.0
173.00	1993.0
174.00	144192.0
175.00	12417.0
176.00	139968.0
176.90	9354.0
177.90	193.0
282.10	51.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78

m/z	Abundance
36.00	911.0
37.00	4551.0
38.00	3884.0
39.00	1931.0
40.00	227.0
40.70	111.0
41.10	114.0
42.30	139.0
43.00	239.0
43.90	926.0
45.00	822.0
46.90	945.0
47.90	552.0
49.00	3913.0
50.00	19968.0
51.00	5724.0
51.90	337.0
52.90	211.0
54.00	52.0
55.00	234.0
55.90	1520.0
57.00	2351.0
57.80	119.0
58.20	119.0
58.90	84.0
59.90	1042.0
61.00	5055.0
62.00	4907.0
63.00	4204.0
63.90	595.0
65.10	717.0
65.90	91.0
67.00	293.0
68.00	10166.0
69.00	10293.0
70.00	922.0
71.00	101.0
72.00	559.0
73.00	4713.0
74.00	19752.0
75.00	54600.0
76.00	4858.0
76.90	510.0
78.00	318.0
78.90	3305.0
79.90	991.0
80.90	3987.0
82.00	955.0
83.10	93.0
86.00	186.0
87.00	3960.0
88.00	4220.0
90.80	603.0
92.00	3635.0
93.00	5249.0
94.00	12839.0
95.00	110968.0
96.00	6620.0
97.20	166.0
102.90	91.0
103.90	539.0
105.10	226.0
105.90	757.0
106.90	187.0
110.00	73.0
110.80	185.0
112.00	116.0
113.00	186.0
114.80	122.0
115.90	445.0
116.90	933.0
117.90	588.0
118.80	1053.0
122.00	77.0
122.60	53.0
123.10	91.0
123.60	74.0
127.00	75.0
127.90	460.0
129.00	507.0
130.00	482.0
130.70	164.0
131.00	164.0
134.80	304.0
136.00	73.0
136.80	239.0
139.00	62.0
139.80	219.0
140.90	1584.0
142.00	297.0
142.90	2093.0
144.20	233.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78

145.00	380.0
146.10	250.0
146.90	146.0
148.10	328.0
149.10	150.0
149.80	184.0
151.60	59.0
152.90	137.0
154.90	415.0
156.10	101.0
157.00	148.0
157.90	64.0
159.10	201.0
160.80	141.0
164.50	52.0
165.40	50.0
169.90	144.0
171.00	215.0
171.90	1281.0
173.10	2098.0
174.00	107160.0
175.00	7343.0
175.90	101472.0
177.00	6776.0
178.10	240.0
207.30	109.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78

m/z	Abundance
36.60	80.0
37.30	58.0
37.70	65.0
38.90	120.0
39.80	176.0
40.60	72.0
42.40	110.0
43.90	394.0
45.20	53.0
45.80	73.0
46.50	75.0
47.20	50.0
47.80	96.0
49.60	95.0
50.50	55.0
52.90	62.0
53.60	63.0
59.50	66.0
60.60	87.0
63.90	57.0
66.60	56.0
71.50	78.0
73.30	68.0
206.90	127.0

Instrument :
MSVOA_X
ClientSampleId :
BFB78