

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100621\  
 Data File : VX024625.D  
 Acq On : 06 Oct 2021 18:08  
 Operator : JC/MD  
 Sample : M4088-01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 16 Sample Multiplier: 1


Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 WC-20211005-WATER

Quant Time: Oct 07 07:48:24 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X092321W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Sep 23 18:24:34 2021  
 Response via : Initial Calibration

| Compound                      | R.T.           | QIon | Response           | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|--------------------|-----------|--------|----------|
| -----                         |                |      |                    |           |        |          |
| Internal Standards            |                |      |                    |           |        |          |
| 1) Pentafluorobenzene         | 5.562          | 168  | 127347             | 50.00     | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.769          | 114  | 222123             | 50.00     | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055         | 117  | 220958             | 50.00     | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 99197              | 50.00     | ug/l   | 0.00     |
|                               |                |      |                    |           |        |          |
| System Monitoring Compounds   |                |      |                    |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.964          | 65   | 96995              | 54.04     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 78 - 117 |      | Recovery = 108.08% |           |        |          |
| 35) Dibromofluoromethane      | 5.397          | 113  | 75786              | 51.36     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = 102.72% |           |        |          |
| 50) Toluene-d8                | 8.653          | 98   | 277602             | 51.11     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 92 - 112 |      | Recovery = 102.22% |           |        |          |
| 62) 4-Bromofluorobenzene      | 11.085         | 95   | 104696             | 49.03     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = 98.06%  |           |        |          |
|                               |                |      |                    |           |        |          |
| Target Compounds              |                |      |                    |           | Qvalue |          |
| 3) Chloromethane              | 1.300          | 50   | 248                | 0.21      | ug/l # | 42       |
| 5) Bromomethane               | 1.617          | 94   | 271                | 0.32      | ug/l   | 90       |
| 6) Chloroethane               | 1.678          | 64   | 261                | 0.57      | ug/l # | 43       |
| 11) Tert butyl alcohol        | 2.983          | 59   | 148                | Below Cal | #      | 73       |
| 13) Acrolein                  | 2.264          | 56   | 21                 | 10.27     | ug/l # | 14       |
| 14) Allyl chloride            | 2.648          | 41   | 534                | 0.25      | ug/l # | 41       |
| 16) Acetone                   | 2.386          | 43   | 6369               | Below Cal |        | 91       |
| 17) Carbon Disulfide          | 2.520          | 76   | 588                | 0.42      | ug/l # | 75       |
| 20) Methylene Chloride        | 2.788          | 84   | 420                | Below Cal | #      | 81       |
| 25) 2-Butanone                | 4.580          | 43   | 3387               | 2.74      | ug/l   | 100      |
| 28) Bromochloromethane        | 5.111          | 49   | 2783               | 2.53      | ug/l # | 9        |
| 30) Chloroform                | 5.105          | 83   | 32880              | 12.30     | ug/l   | 96       |
| 31) Cyclohexane               | 5.556          | 56   | 2702               | 1.26      | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 5.562          | 75   | 10261              | 4.82      | ug/l # | 50       |
| 37) Ethyl Acetate             | 4.580          | 43   | 3387               | 1.27      | ug/l # | 64       |
| 38) Carbon Tetrachloride      | 5.568          | 117  | 13214              | 5.70      | ug/l # | 16       |
| 47) Bromodichloromethane      | 7.830          | 83   | 1682               | 0.78      | ug/l   | 96       |
| 52) Toluene                   | 8.720          | 92   | 1249               | 0.32      | ug/l   | 90       |
| 60) Dibromochloromethane      | 9.531          | 129  | 19                 | 1.20      | ug/l # | 11       |
| 68) m/p-Xylenes               | 10.305         | 106  | 1865               | 0.60      | ug/l   | 99       |
| 69) o-Xylene                  | 10.646         | 106  | 1018               | 0.33      | ug/l   | 78       |
| 76) 1,2,3-Trichloropropane    | 11.085         | 75   | 57169              | 25.38     | ug/l # | 38       |
| 81) trans-1,4-Dichloro-2-b... | 11.085         | 75   | 57169              | 69.18     | ug/l # | 12       |
| 84) 1,2,4-Trimethylbenzene    | 11.756         | 105  | 5606               | 0.94      | ug/l   | 96       |
| 90) Hexachloroethane          | 12.536         | 117  | 218                | 0.21      | ug/l # | 9        |
| 95) Naphthalene               | 13.780         | 128  | 57123              | 8.25      | ug/l   | 99       |
| -----                         |                |      |                    |           |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed









#1  
Pentafluorobenzene  
Concen: 50.00 ug/l  
RT: 5.562 min Scan# 734  
Delta R.T. 0.006 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion:168 Resp: 127347  
Ion Ratio Lower Upper  
168 100  
99 57.9 45.8 68.6

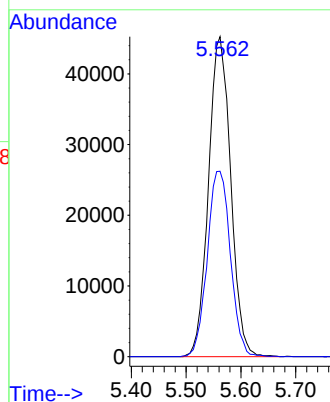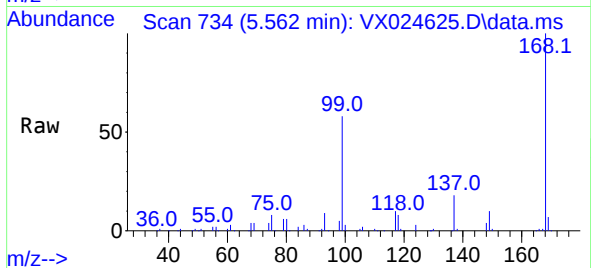

#3  
Chloromethane  
Concen: 0.21 ug/l  
RT: 1.300 min Scan# 35  
Delta R.T. 0.006 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 50 Resp: 248  
Ion Ratio Lower Upper  
50 100  
52 0.0 26.4 39.6#


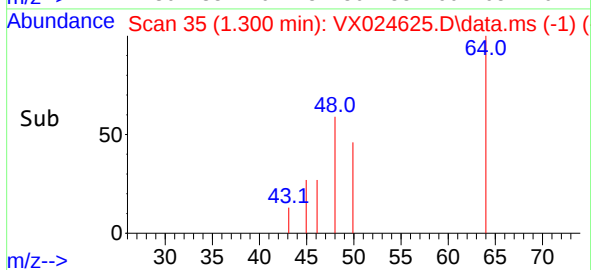




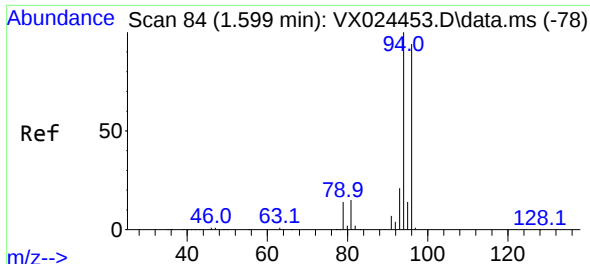

#5  
Bromomethane  
Concen: 0.32 ug/l  
RT: 1.617 min Scan# 87  
Delta R.T. 0.018 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 94 Resp: 271  
Ion Ratio Lower Upper  
94 100  
96 86.2 76.4 114.6

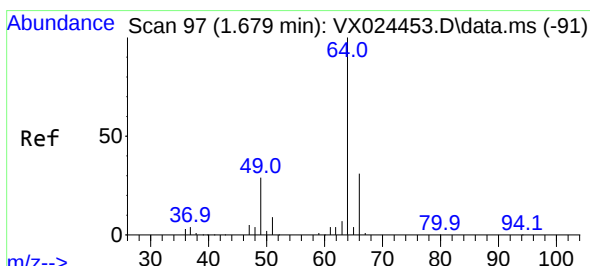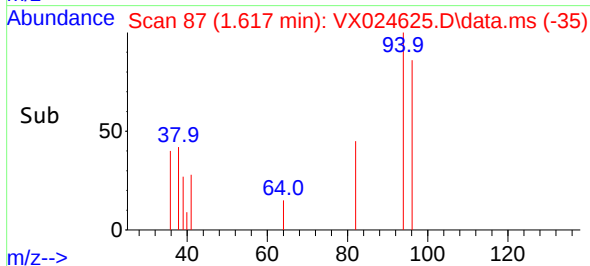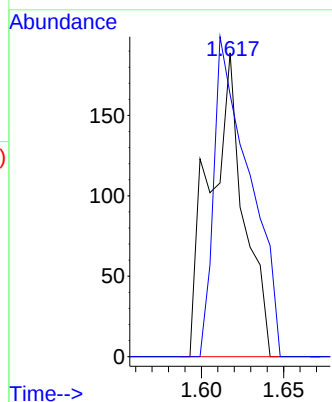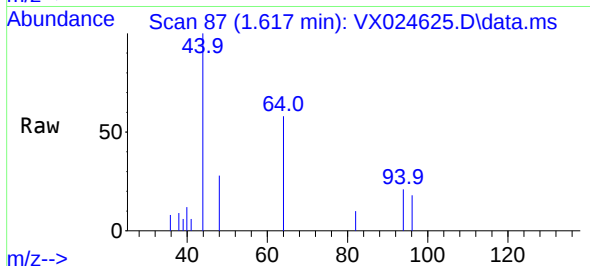

#6  
Chloroethane  
Concen: 0.57 ug/l  
RT: 1.678 min Scan# 97  
Delta R.T. -0.001 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 64 Resp: 261  
Ion Ratio Lower Upper  
64 100  
66 0.0 25.4 38.0#

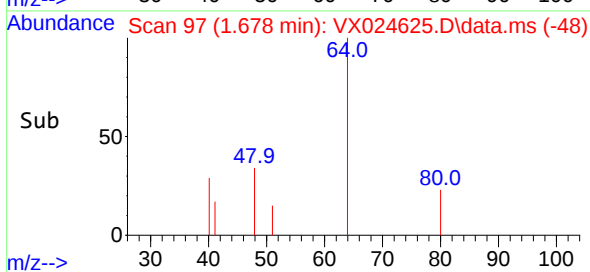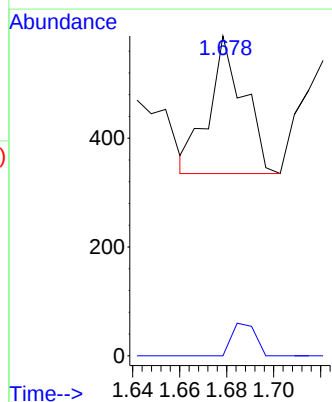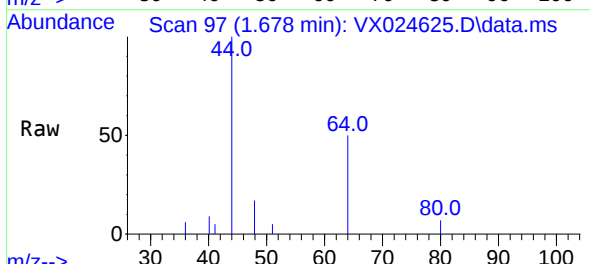







#11

Tert butyl alcohol  
Concen: Below Cal  
RT: 2.983 min Scan# 311  
Delta R.T. 0.006 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER




Tgt Ion: 59 Resp: 148  
Ion Ratio Lower Upper  
59 100  
57 0.0 7.8 11.8#

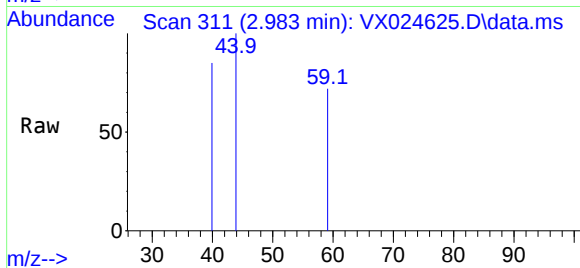


#13

Acrolein  
Concen: 10.27 ug/l  
RT: 2.264 min Scan# 193  
Delta R.T. 0.025 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 56 Resp: 21  
Ion Ratio Lower Upper  
56 100  
55 0.0 56.4 84.6#


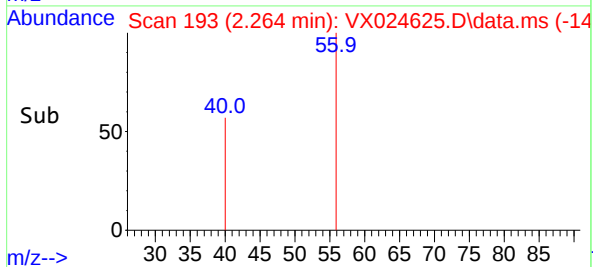

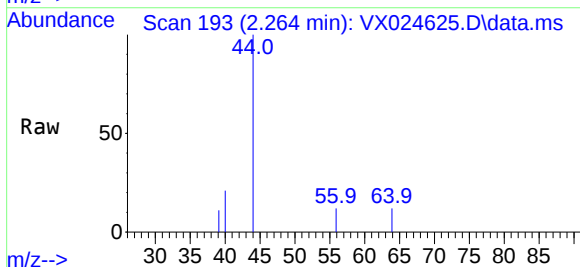




#14  
Allyl chloride  
Concen: 0.25 ug/l  
RT: 2.648 min Scan# 256  
Delta R.T. -0.018 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 41    | Resp: | 534   |
| Ion      | Ratio | Lower | Upper |
| 41       | 100   |       |       |
| 39       | 19.9  | 51.6  | 77.4# |
| 76       | 0.0   | 30.5  | 45.7# |

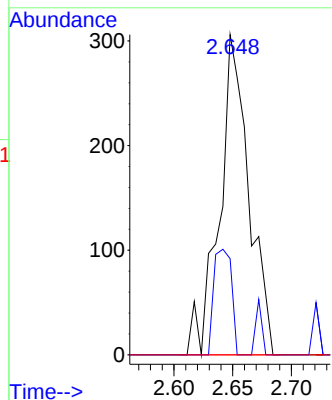

#16  
Acetone  
Concen: Below Cal  
RT: 2.386 min Scan# 213  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 6369  |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 58       | 29.7  | 27.8  | 41.8  |


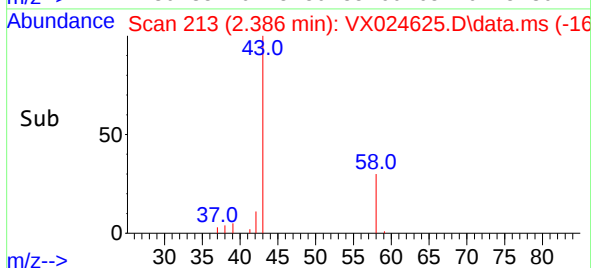
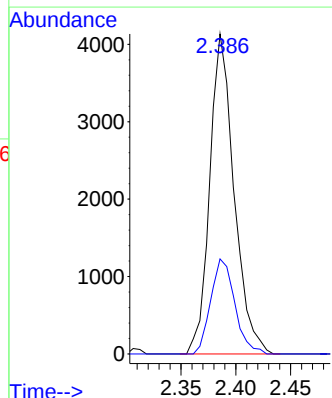





#17  
Carbon Disulfide  
Concen: 0.42 ug/l  
RT: 2.520 min Scan# 235  
Delta R.T. 0.006 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 76 Resp: 588  
Ion Ratio Lower Upper  
76 100  
78 0.0 7.2 10.8#

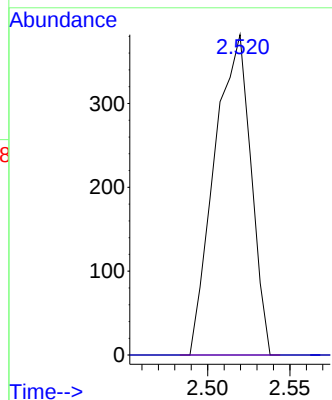

#20  
Methylene Chloride  
Concen: Below Cal  
RT: 2.788 min Scan# 279  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 84 Resp: 420  
Ion Ratio Lower Upper  
84 100  
49 83.9 88.6 132.8#  
51 24.3 27.0 40.6#  
86 69.9 50.3 75.5


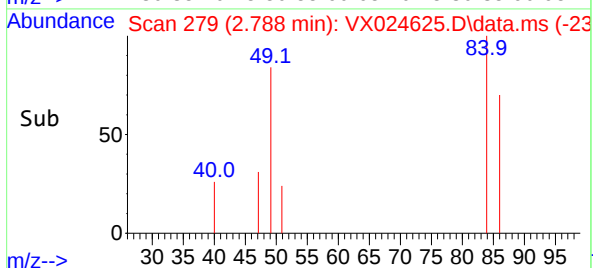
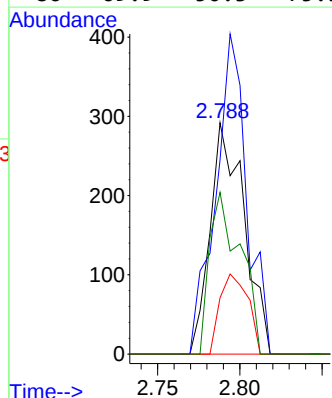





#25  
2-Butanone  
Concen: 2.74 ug/l  
RT: 4.580 min Scan# 573  
Delta R.T. 0.012 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 43 Resp: 3387  
Ion Ratio Lower Upper  
43 100  
72 29.6 23.7 35.5

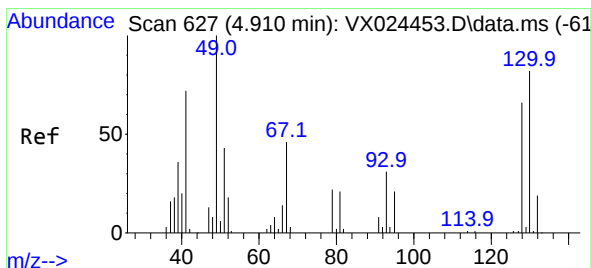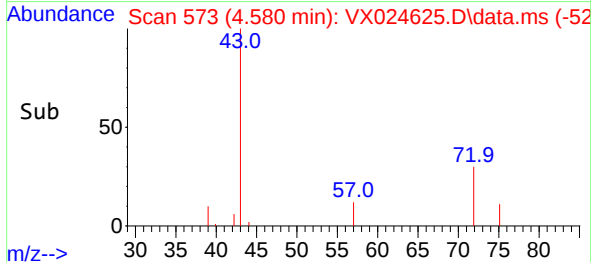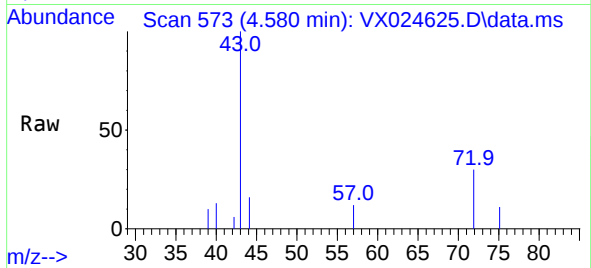

#28  
Bromochloromethane  
Concen: 2.53 ug/l  
RT: 5.111 min Scan# 660  
Delta R.T. 0.201 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 49 Resp: 2783  
Ion Ratio Lower Upper  
49 100  
129 0.0 0.0 4.0  
130 0.0 68.2 102.2#

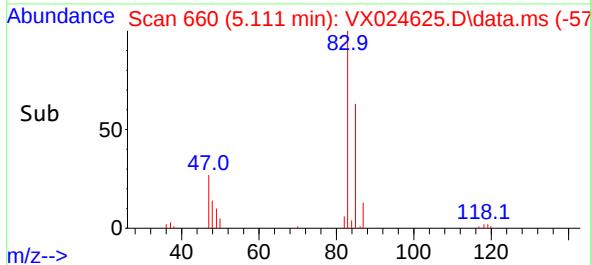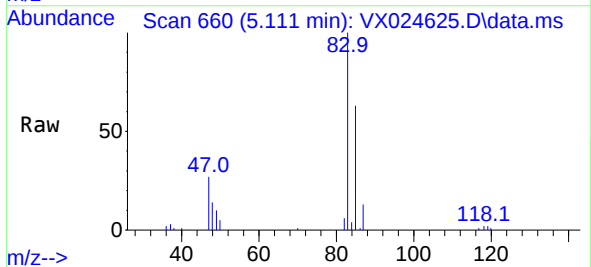



#30

Chloroform

Concen: 12.30 ug/l

RT: 5.105 min Scan# 659

Delta R.T. -0.000 min

Lab File: VX024625.D





Acq: 06 Oct 2021 18:08

Tgt Ion: 83 Resp: 32880

Ion Ratio Lower Upper

83 100

85 68.0 52.0 78.0

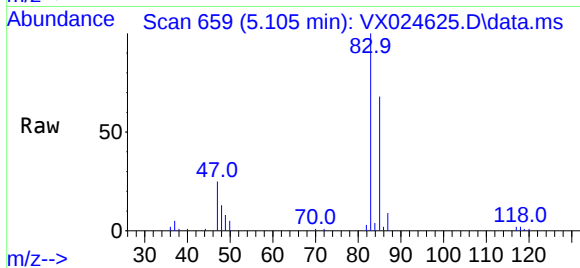

#31

Cyclohexane

Concen: 1.26 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.079 min

Lab File: VX024625.D

Acq: 06 Oct 2021 18:08




Tgt Ion: 56 Resp: 2702


Ion Ratio Lower Upper

56 100

69 156.6 25.3 37.9#

84 169.9 71.4 107.0#


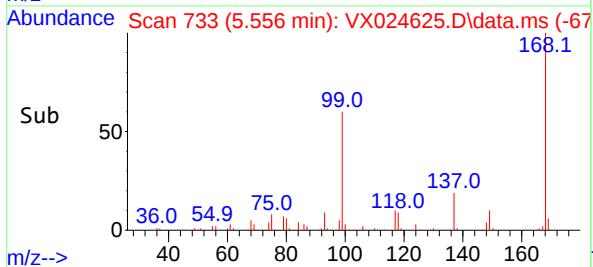

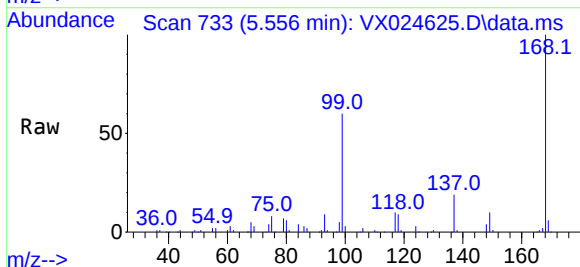




#33  
1,2-Dichloroethane-d4  
Concen: 54.04 ug/l  
RT: 5.964 min Scan# 800  
Delta R.T. 0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 65 Resp: 96995  
Ion Ratio Lower Upper  
65 100  
67 49.8 0.0 105.4

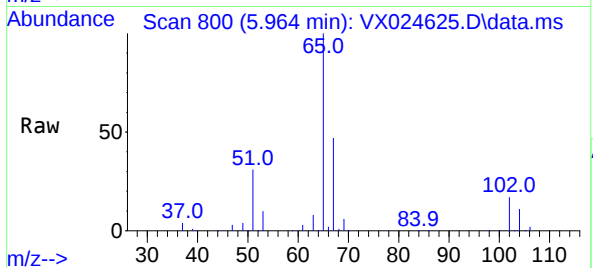

#34  
1,4-Difluorobenzene  
Concen: 50.00 ug/l  
RT: 6.769 min Scan# 932  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 114 Resp: 222123  
Ion Ratio Lower Upper  
114 100  
63 20.6 0.0 40.8  
88 17.2 0.0 32.8

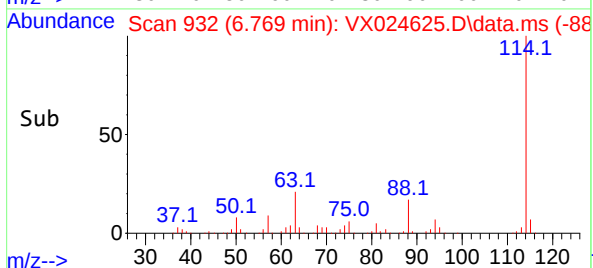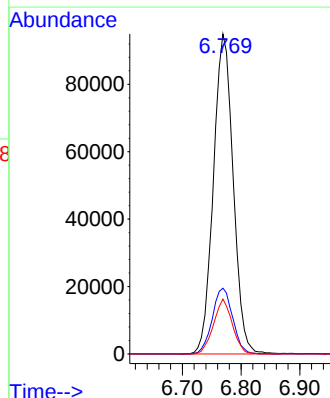







#35  
Dibromofluoromethane  
Concen: 51.36 ug/l  
RT: 5.397 min Scan# 707  
Delta R.T. 0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER

Tgt Ion:113 Resp: 75786




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 113 | 100   |       |       |
| 111 | 102.3 | 81.9  | 122.9 |
| 192 | 19.4  | 16.7  | 25.1  |

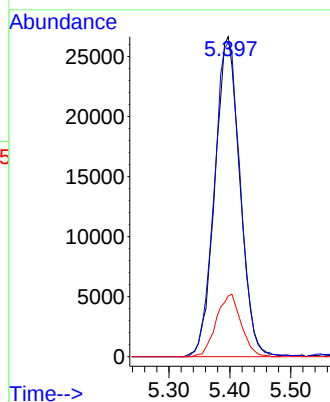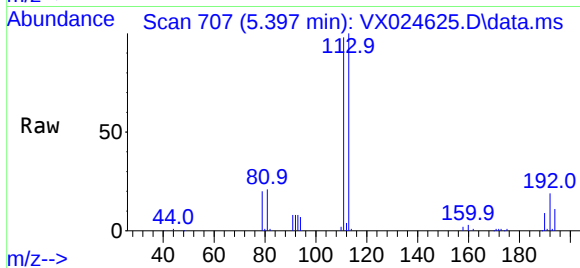


#36  
1,1-Dichloropropene  
Concen: 4.82 ug/l  
RT: 5.562 min Scan# 734  
Delta R.T. -0.134 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 75 Resp: 10261

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 75  | 100   |       |       |
| 110 | 10.5  | 18.1  | 54.4# |
| 77  | 0.0   | 25.3  | 37.9# |


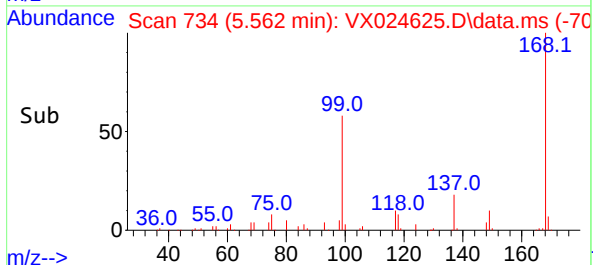

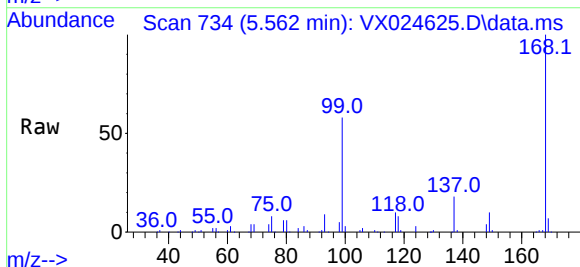




#37  
Ethyl Acetate  
Concen: 1.27 ug/l  
RT: 4.580 min Scan# 573  
Delta R.T. -0.147 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 43    | Resp: | 3387  |
| Ion      | Ratio | Lower | Upper |
| 43       | 100   |       |       |
| 61       | 0.0   | 12.8  | 19.2# |
| 70       | 0.0   | 10.5  | 15.7# |



#38  
Carbon Tetrachloride  
Concen: 5.70 ug/l  
RT: 5.568 min Scan# 735  
Delta R.T. -0.122 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 117   | Resp: | 13214  |
| Ion      | Ratio | Lower | Upper  |
| 117      | 100   |       |        |
| 119      | 4.1   | 76.2  | 114.2# |
| 121      | 0.0   | 24.8  | 37.2#  |


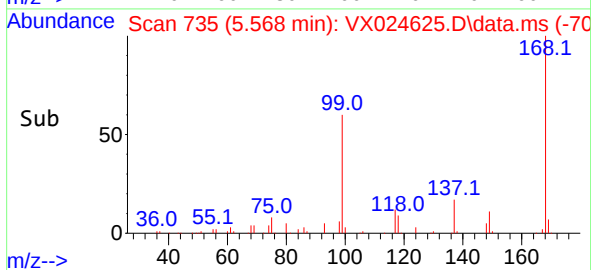






#47  
Bromodichloromethane  
Concen: 0.78 ug/l  
RT: 7.830 min Scan# 1106  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 83    | Resp: | 1682  |
| Ion      | Ratio | Lower | Upper |
| 83       | 100   |       |       |
| 85       | 60.2  | 51.4  | 77.0  |
| 127      | 8.5   | 6.8   | 10.2  |

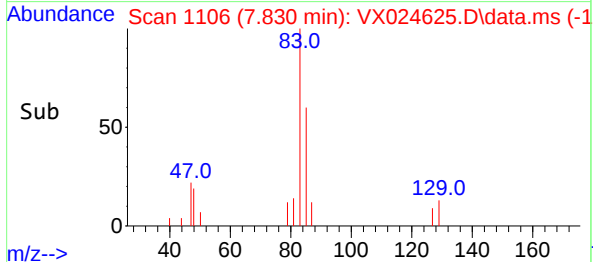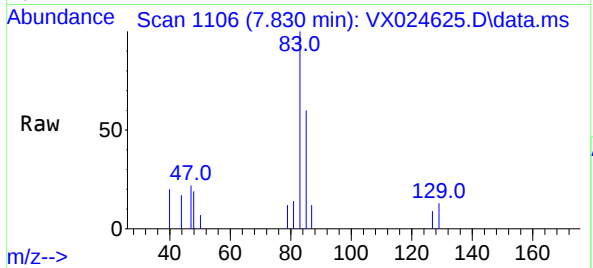

#50  
Toluene-d8  
Concen: 51.11 ug/l  
RT: 8.653 min Scan# 1241  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 98    | Resp: | 277602 |
| Ion      | Ratio | Lower | Upper  |
| 98       | 100   |       |        |
| 100      | 63.8  | 51.9  | 77.9   |


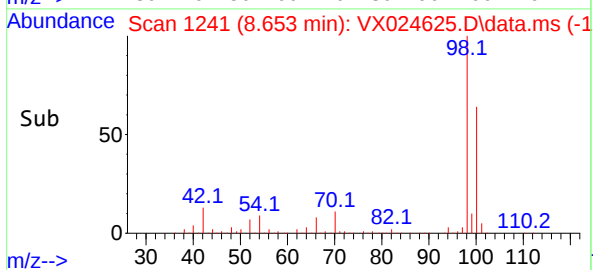






#52  
Toluene  
Concen: 0.32 ug/l  
RT: 8.720 min Scan# 1252  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 92 Resp: 1249  
Ion Ratio Lower Upper  
92 100  
91 158.0 137.1 205.7

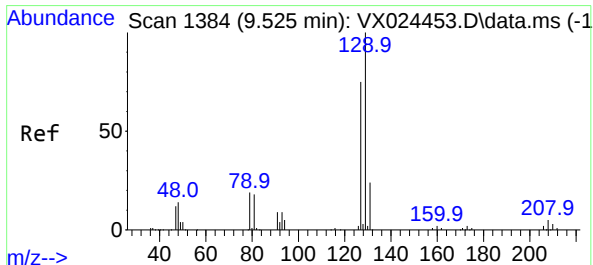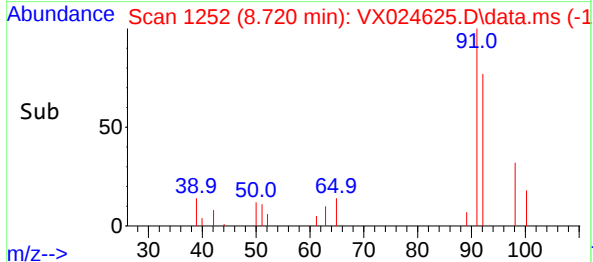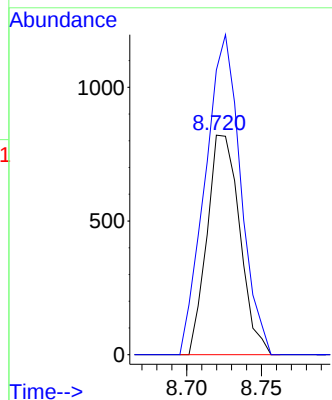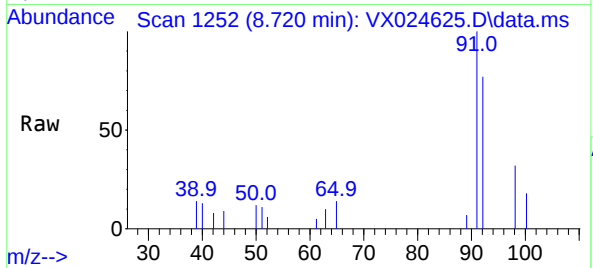

#60  
Dibromochloromethane  
Concen: 1.20 ug/l  
RT: 9.531 min Scan# 1385  
Delta R.T. 0.006 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 129 Resp: 19  
Ion Ratio Lower Upper  
129 100  
127 0.0 38.4 115.2#


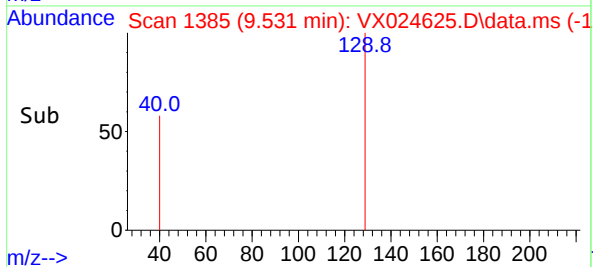
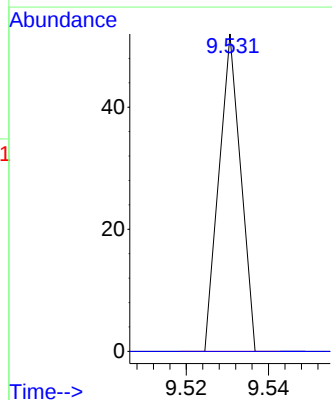
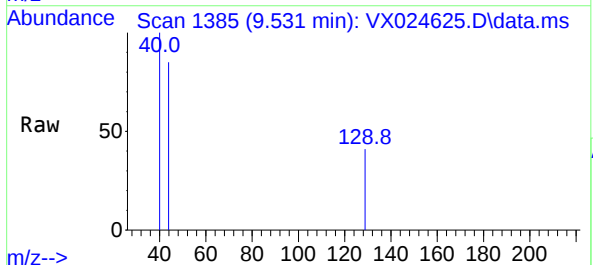




#62  
4-Bromofluorobenzene  
Concen: 49.03 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 95 Resp: 104696  
Ion Ratio Lower Upper  
95 100  
174 80.8 0.0 154.6  
176 77.8 0.0 155.8



#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 117 Resp: 220958  
Ion Ratio Lower Upper  
117 100  
82 59.1 47.4 71.2  
119 31.2 26.6 39.8


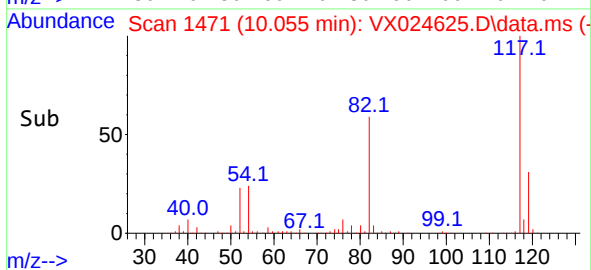






#68  
m/p-Xylenes  
Concen: 0.60 ug/l  
RT: 10.305 min Scan# 1512  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion:106 Resp: 1865  
Ion Ratio Lower Upper  
106 100  
91 201.6 162.8 244.2

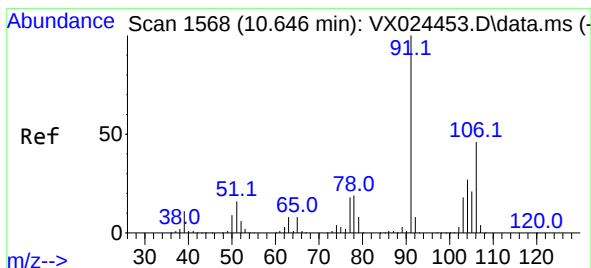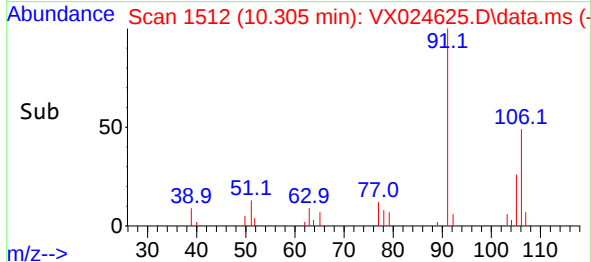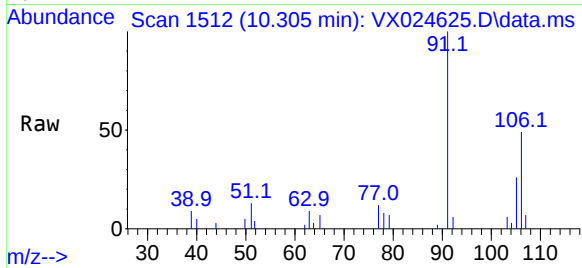

#69  
o-Xylene  
Concen: 0.33 ug/l  
RT: 10.646 min Scan# 1568  
Delta R.T. 0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion:106 Resp: 1018  
Ion Ratio Lower Upper  
106 100  
91 181.7 108.1 324.2


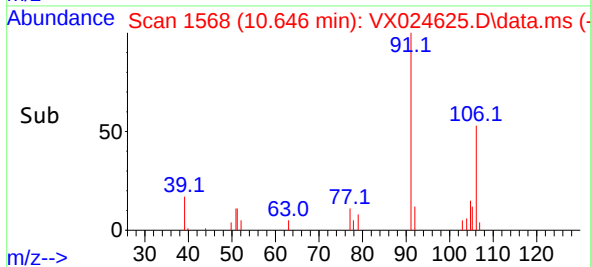

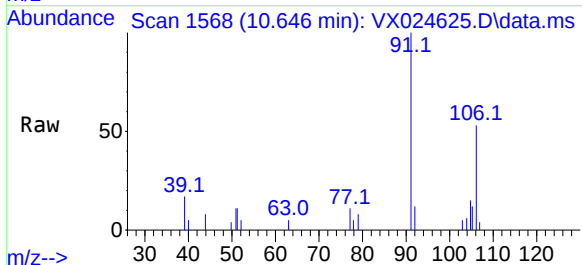




#72  
1,4-Dichlorobenzene-d4  
Concen: 50.00 ug/l  
RT: 12.024 min Scan# 1794  
Delta R.T. 0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion:152 Resp: 99197  
Ion Ratio Lower Upper  
152 100  
115 60.8 41.1 123.3  
150 161.0 0.0 349.0

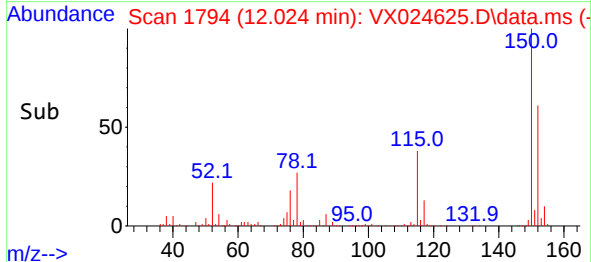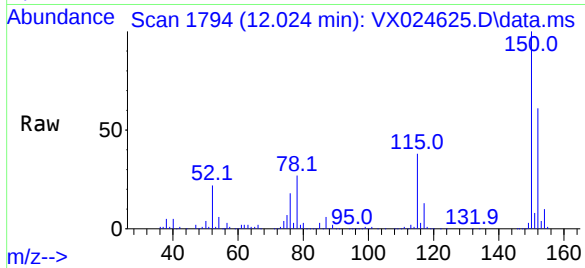

#76  
1,2,3-Trichloropropane  
Concen: 25.38 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. -0.159 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 75 Resp: 57169  
Ion Ratio Lower Upper  
75 100  
77 1.0 19.1 57.5#


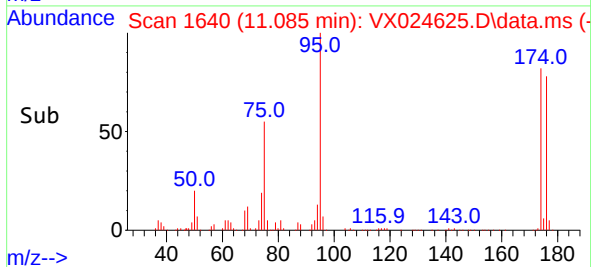

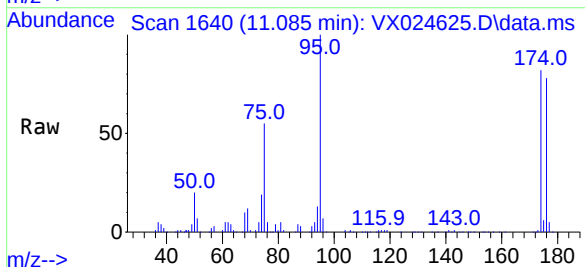




#81  
trans-1,4-Dichloro-2-butene  
Concen: 69.18 ug/l  
RT: 11.085 min Scan# 1640  
Delta R.T. 0.061 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08




Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER


Tgt Ion: 75 Resp: 57169  
Ion Ratio Lower Upper  
75 100  
53 0.0 74.5 111.7#  
89 0.0 37.9 56.9#

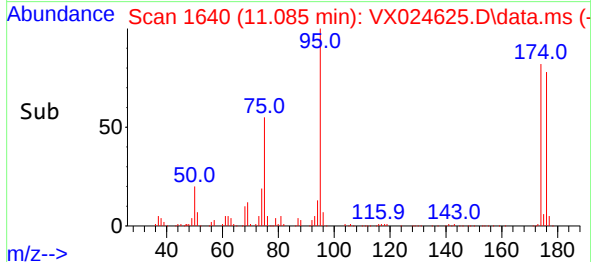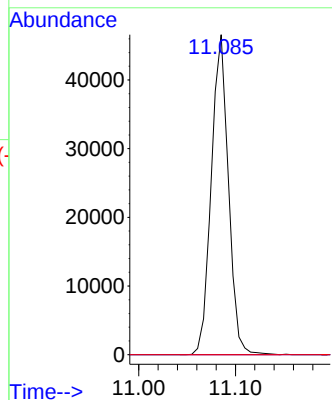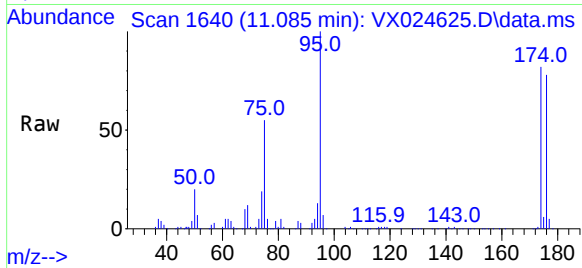

#84  
1,2,4-Trimethylbenzene  
Concen: 0.94 ug/l  
RT: 11.756 min Scan# 1750  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion: 105 Resp: 5606  
Ion Ratio Lower Upper  
105 100  
120 42.2 22.4 67.3


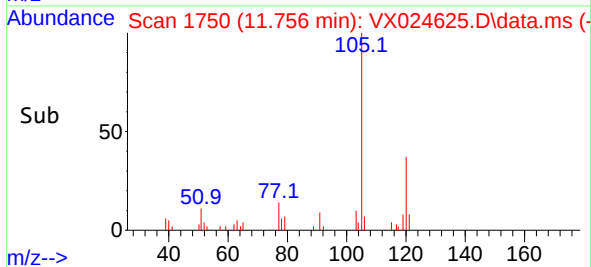
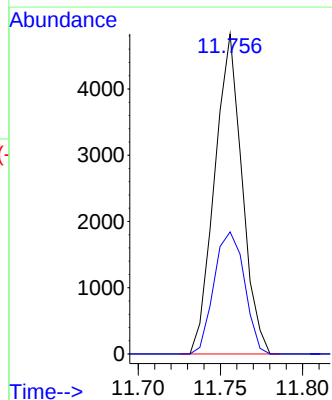
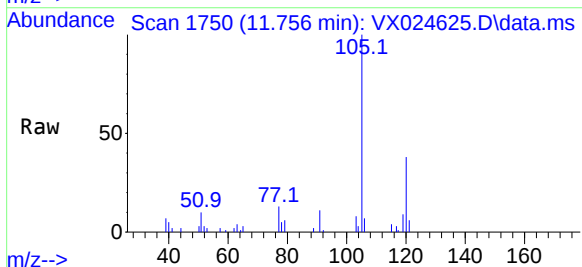




#90  
Hexachloroethane  
Concen: 0.21 ug/l  
RT: 12.536 min Scan# 1878  
Delta R.T. -0.006 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Instrument :  
MSVOA\_X  
ClientSampleId :  
WC-20211005-WATER

Tgt Ion:117 Resp: 218  
Ion Ratio Lower Upper  
117 100  
201 0.0 40.4 121.2#

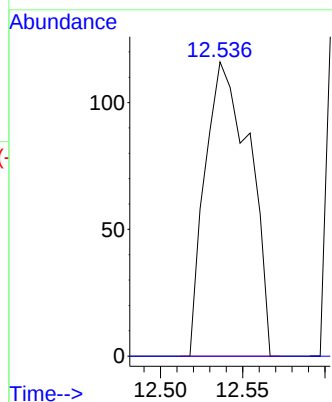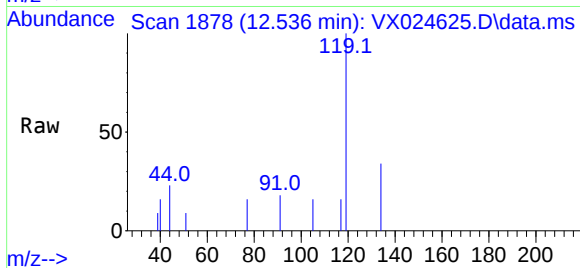

#95  
Naphthalene  
Concen: 8.25 ug/l  
RT: 13.780 min Scan# 2082  
Delta R.T. -0.000 min  
Lab File: VX024625.D  
Acq: 06 Oct 2021 18:08

Tgt Ion:128 Resp: 57123  
Ion Ratio Lower Upper  
128 100  
127 12.5 10.3 15.5  
129 10.7 8.8 13.2

