

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
 Data File : VX024621.D
 Acq On : 06 Oct 2021 16:34
 Operator : JC/MD
 Sample : M4055-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-RW8-MW01D3-GW-20210929

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	32	rBV	12191	19104	2.12%	0.403%
2	2.063	154	160	167	rBV	25771	39236	4.36%	0.827%
3	2.544	230	239	249	rVB2	7265	14313	1.59%	0.302%
4	5.391	694	706	721	rBV	113860	314375	34.94%	6.627%
5	5.556	721	733	747	rBV2	158119	451283	50.15%	9.513%
6	5.964	787	800	816	rBV	111905	300897	33.44%	6.343%
7	6.763	919	931	943	rBV	273750	644627	71.63%	13.588%
8	8.653	1234	1241	1251	rBV	576619	899884	100.00%	18.969%
9	10.055	1465	1471	1486	rBV	563674	748962	83.23%	15.788%
10	11.085	1634	1640	1652	rBV	500949	621945	69.11%	13.110%
11	12.024	1789	1794	1804	rVB	560903	689366	76.61%	14.531%




Sum of corrected areas: 4743992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024621.D
Acq On : 06 Oct 2021 16:34
Operator : JC/MD
Sample : M4055-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW8-MW01D3-GW-20210929

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

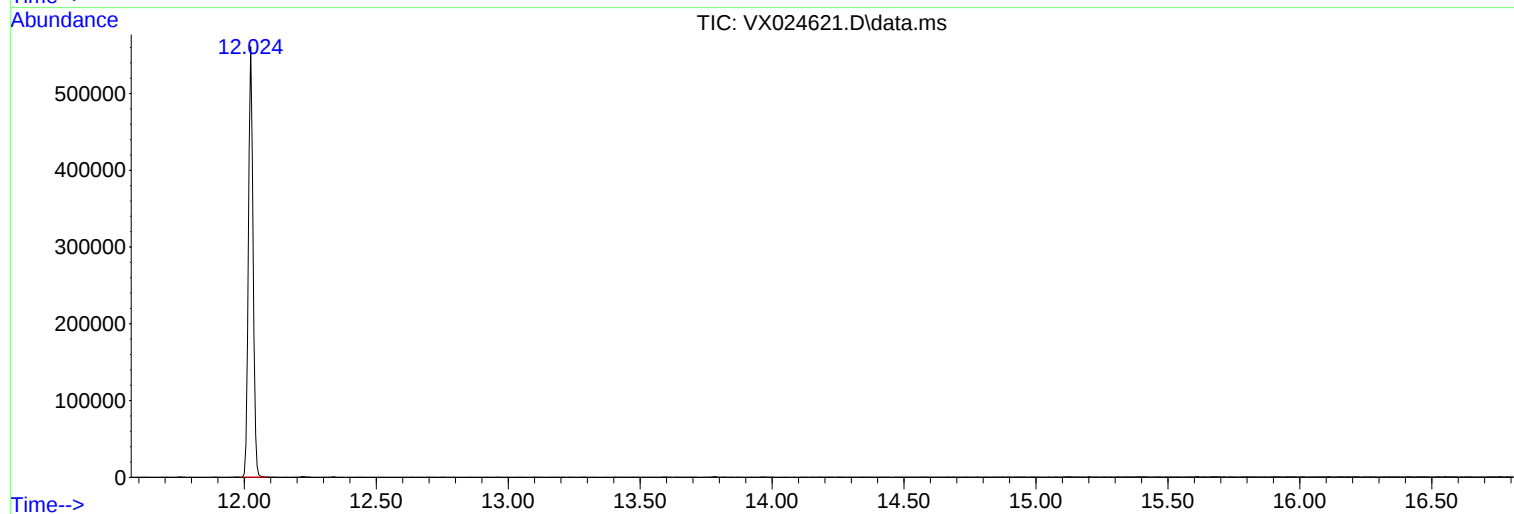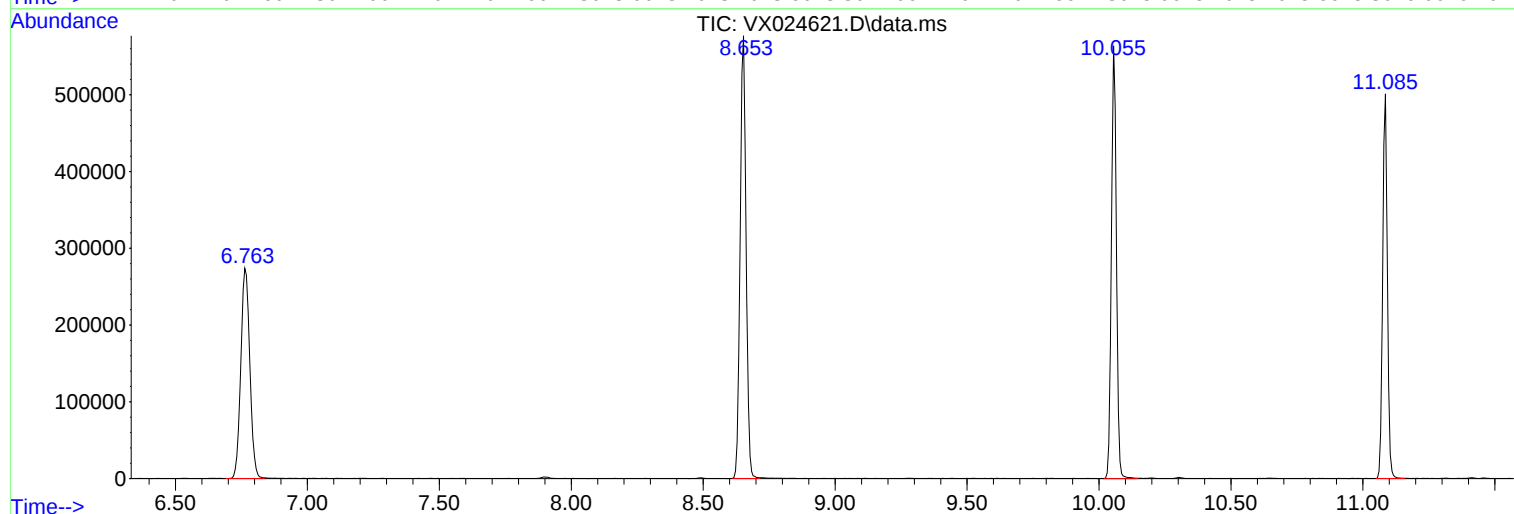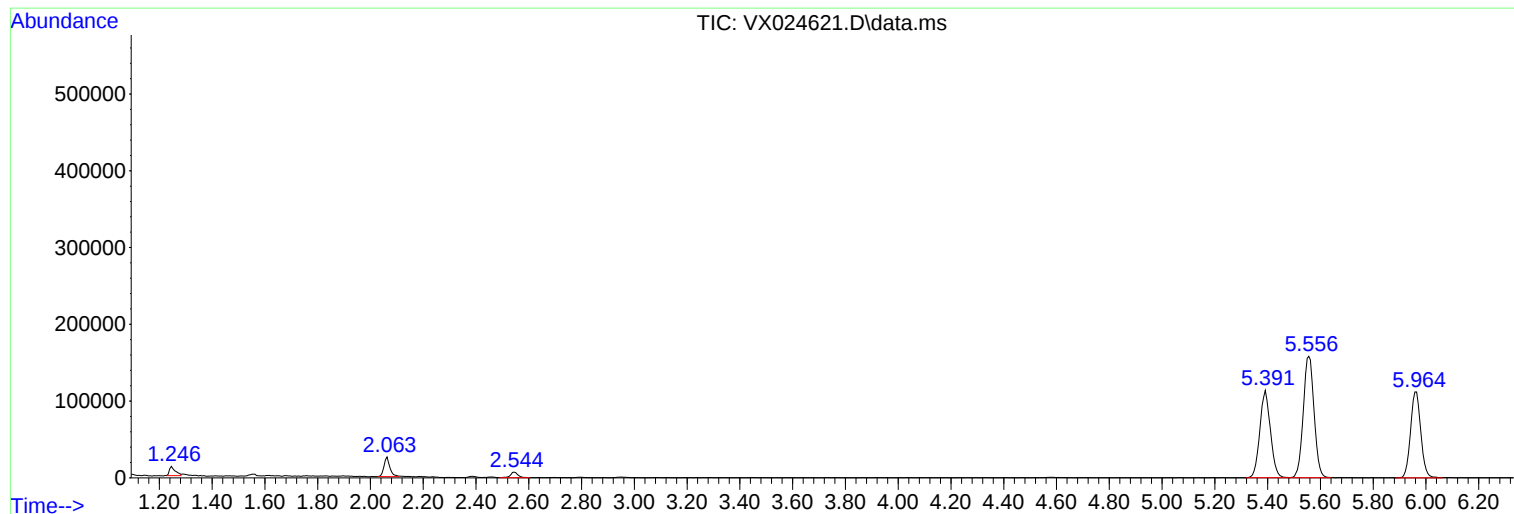

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024621.D
Acq On : 06 Oct 2021 16:34
Operator : JC/MD
Sample : M4055-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW8-MW01D3-GW-20210929

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024621.D
Acq On : 06 Oct 2021 16:34
Operator : JC/MD
Sample : M4055-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW8-MW01D3-GW-20210929

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
