

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
 Data File : VX024622.D
 Acq On : 06 Oct 2021 16:58
 Operator : JC/MD
 Sample : M4055-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TB-20210927

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024622.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	22	27	32	rBV2	20033	26480	3.12%	0.592%
2	2.550	234	240	248	rBV	21008	37919	4.46%	0.848%
3	2.946	298	305	316	rBV	5933	13563	1.60%	0.303%
4	4.586	564	574	589	rBV	3345	10939	1.29%	0.245%
5	5.397	694	707	720	rBV	99627	291476	34.29%	6.519%
6	5.562	722	734	751	rVB	145862	415989	48.94%	9.304%
7	5.964	789	800	817	rBV	113274	291353	34.28%	6.516%
8	6.769	921	932	948	rBV	240653	568537	66.89%	12.716%
9	8.653	1234	1241	1250	rBV	550575	850006	100.00%	19.011%
10	10.055	1465	1471	1487	rBV	532968	722438	84.99%	16.158%
11	11.085	1634	1640	1651	rBV	473998	594884	69.99%	13.305%
12	12.024	1789	1794	1803	rBV	521176	647504	76.18%	14.482%




Sum of corrected areas: 4471088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024622.D
Acq On : 06 Oct 2021 16:58
Operator : JC/MD
Sample : M4055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20210927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

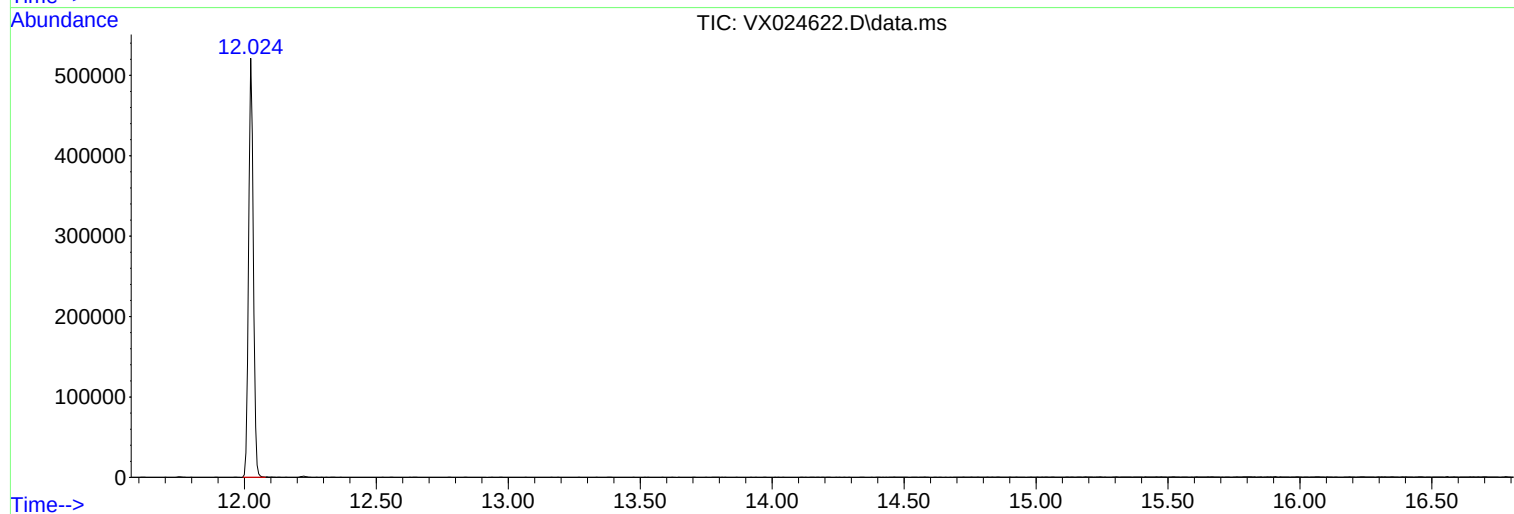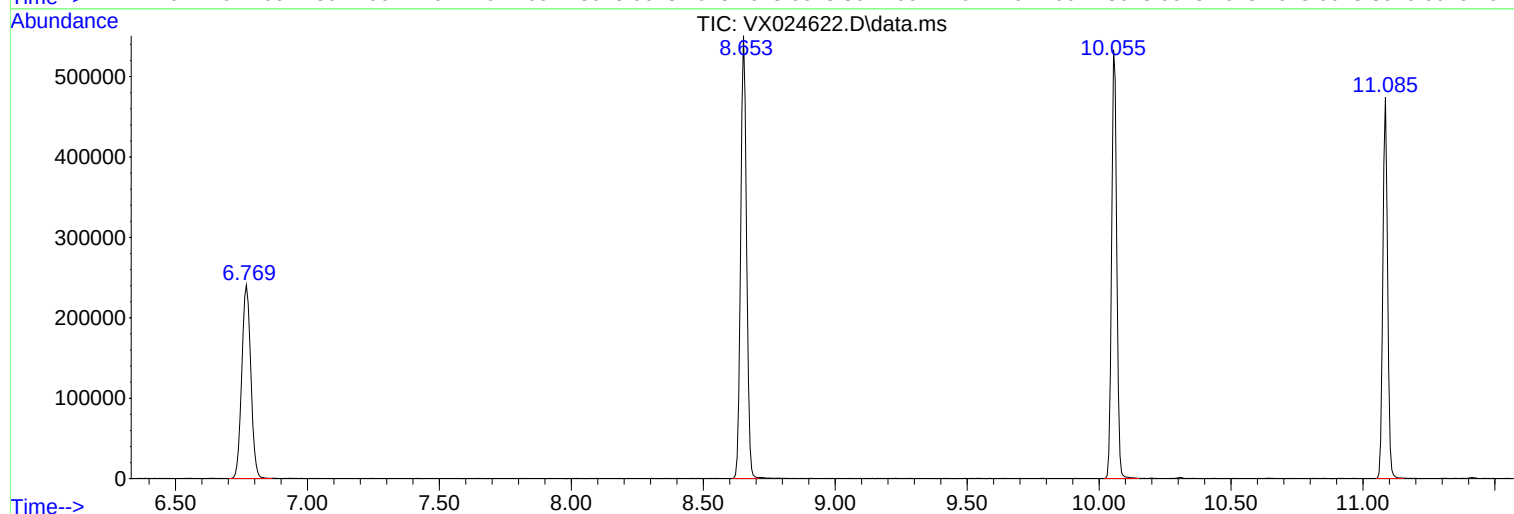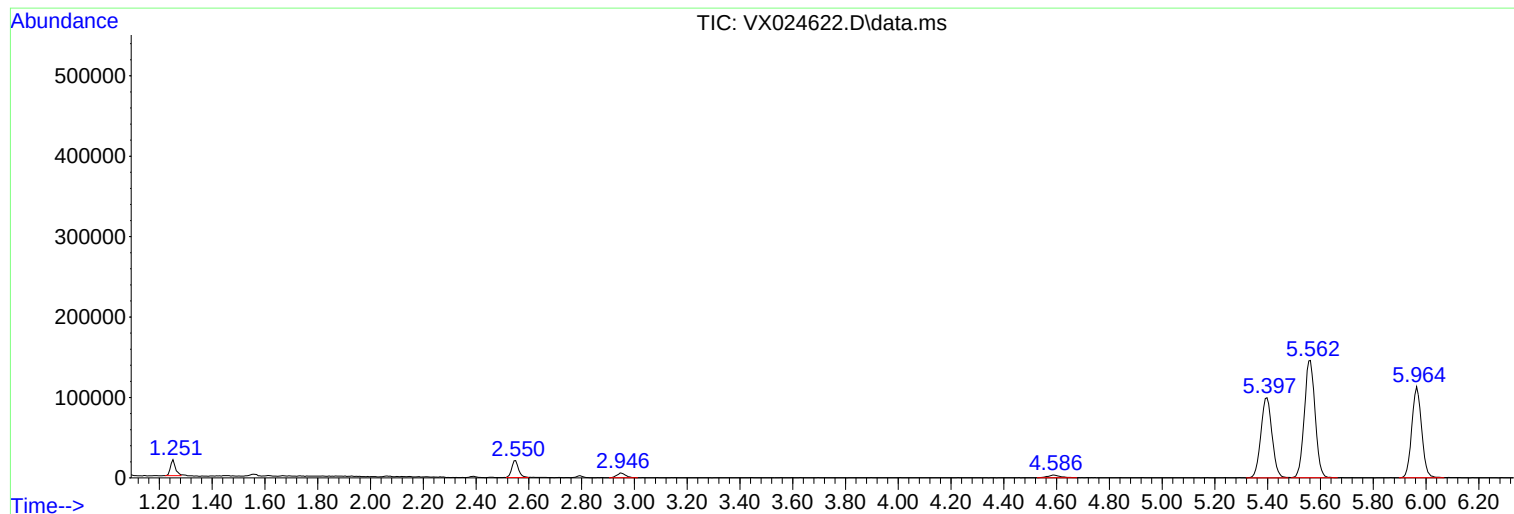

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024622.D
Acq On : 06 Oct 2021 16:58
Operator : JC/MD
Sample : M4055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20210927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024622.D
Acq On : 06 Oct 2021 16:58
Operator : JC/MD
Sample : M4055-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TB-20210927

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
