

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
 Data File : VX024623.D
 Acq On : 06 Oct 2021 17:21
 Operator : JC/MD
 Sample : M4047-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	38	rVB	10575	18000	2.14%	0.413%
2	5.397	695	707	720	rBV2	95312	275884	32.86%	6.325%
3	5.562	722	734	747	rVV	150212	418477	49.84%	9.593%
4	5.964	789	800	817	rBV	109892	282138	33.60%	6.468%
5	6.769	919	932	946	rBV	259366	607393	72.35%	13.924%
6	8.653	1233	1241	1249	rBV	538596	839573	100.00%	19.247%
7	10.055	1465	1471	1479	rBV	536106	734484	87.48%	16.838%
8	11.085	1634	1640	1655	rVB	436922	549589	65.46%	12.599%
9	12.024	1789	1794	1803	rVB	529388	636603	75.82%	14.594%




Sum of corrected areas: 4362141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024623.D
Acq On : 06 Oct 2021 17:21
Operator : JC/MD
Sample : M4047-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

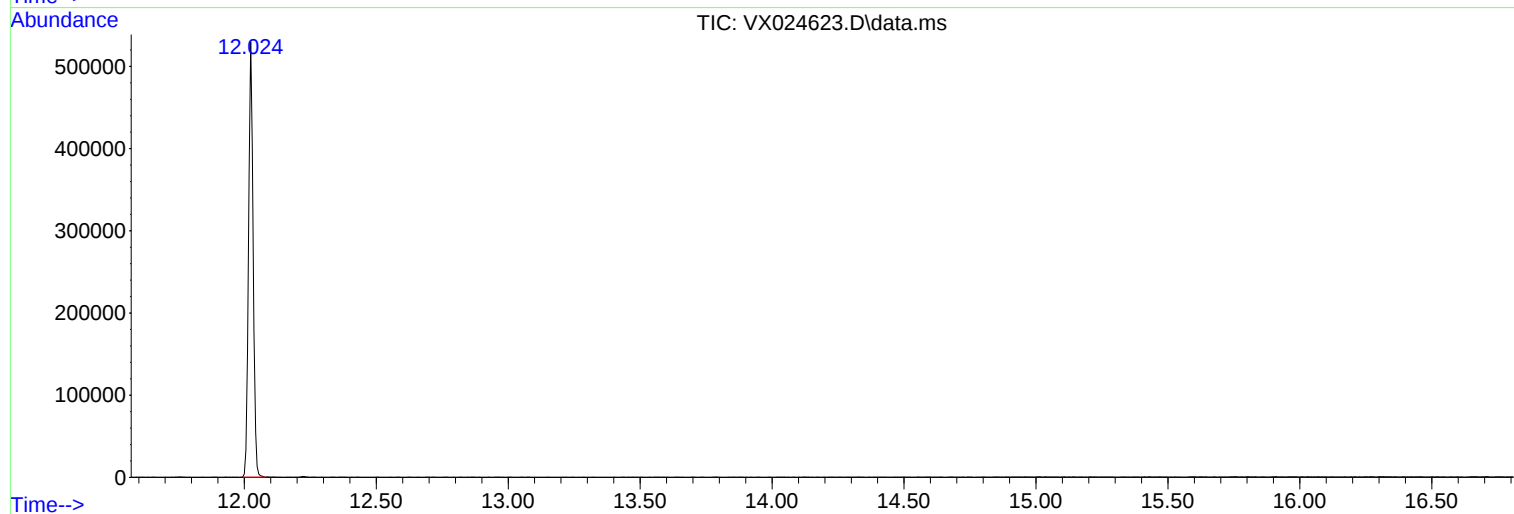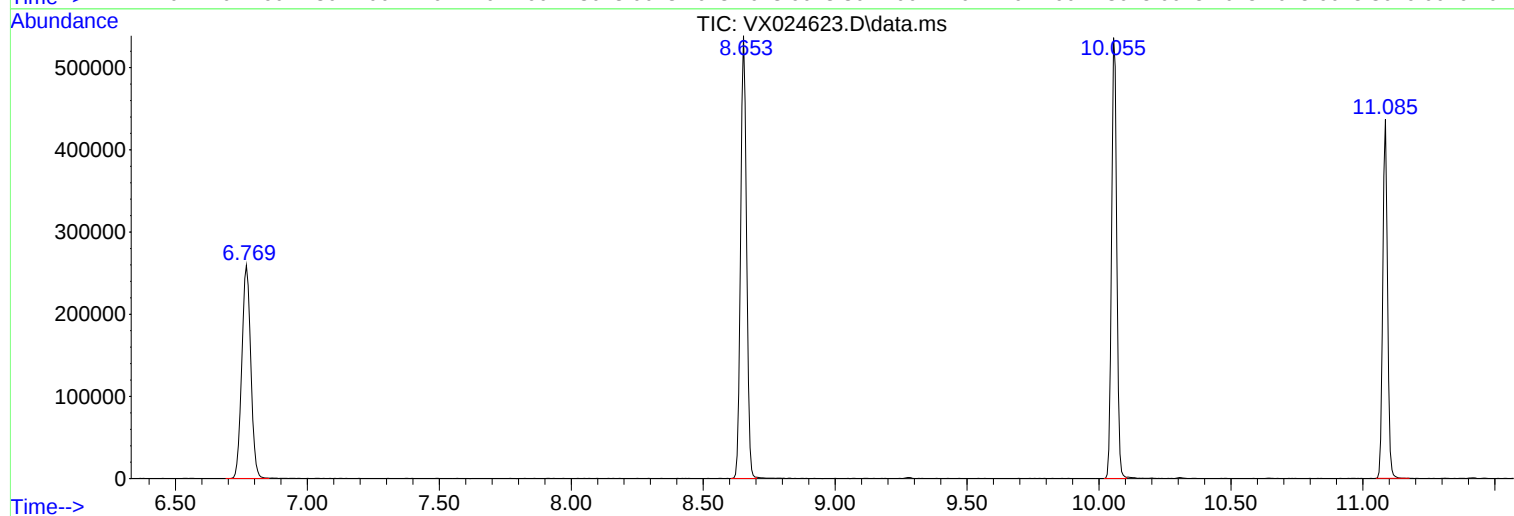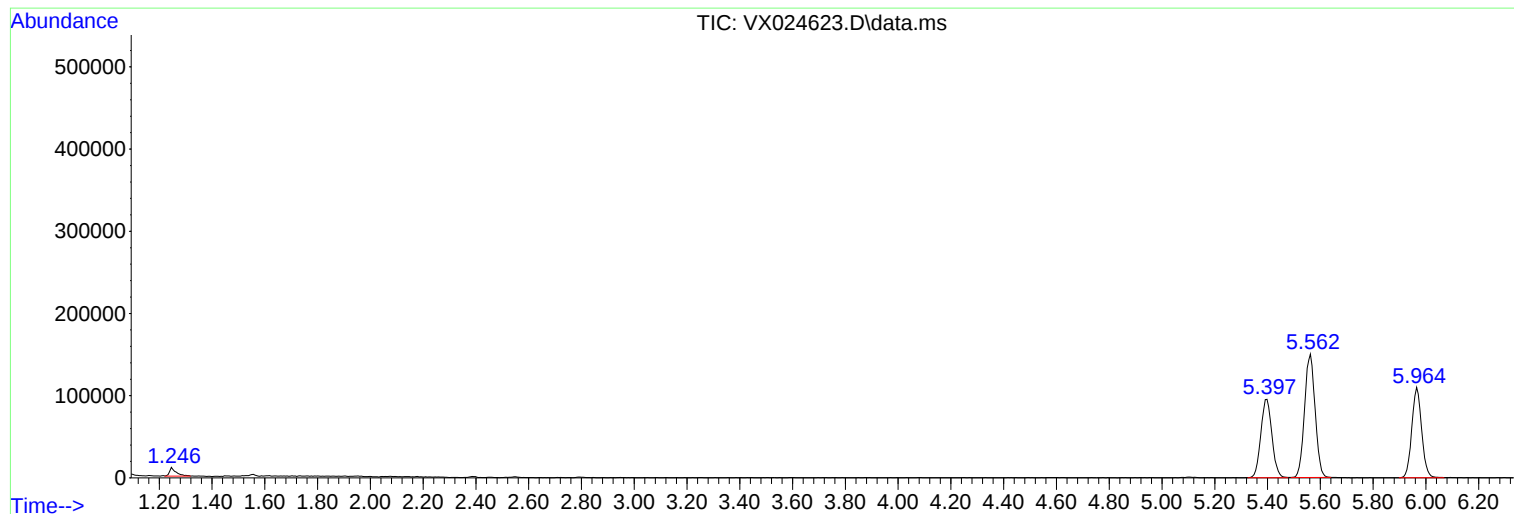

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024623.D
Acq On : 06 Oct 2021 17:21
Operator : JC/MD
Sample : M4047-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024623.D
Acq On : 06 Oct 2021 17:21
Operator : JC/MD
Sample : M4047-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------