

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
 Data File : VX024625.D
 Acq On : 06 Oct 2021 18:08
 Operator : JC/MD
 Sample : M4088-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-20211005-WATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	10902	16622	2.23%	0.358%
2	2.386	203	213	222	rBV	6809	10787	1.45%	0.232%
3	5.105	648	659	674	rVB	27726	82065	10.99%	1.767%
4	5.397	695	707	719	rBV2	88321	254764	34.13%	5.487%
5	5.562	722	734	748	rVB	135935	386038	51.72%	8.314%
6	5.964	789	800	817	rBV	96633	253673	33.99%	5.463%
7	6.769	921	932	950	rBV	226485	532650	71.36%	11.471%
8	8.653	1234	1241	1249	rBV	485893	746396	100.00%	16.075%
9	10.055	1466	1471	1485	rBV	497673	678631	90.92%	14.615%
10	10.305	1507	1512	1517	rVB	8316	10609	1.42%	0.228%
11	11.085	1634	1640	1650	rBV	424109	527833	70.72%	11.368%
12	11.384	1684	1689	1697	rBV2	4550	8661	1.16%	0.187%
13	11.756	1746	1750	1755	rBV	12707	15699	2.10%	0.338%
14	12.024	1789	1794	1801	rBV	526731	628396	84.19%	13.533%
15	12.091	1801	1805	1810	rVB	6373	7853	1.05%	0.169%
16	12.244	1825	1830	1834	rBV2	6501	9048	1.21%	0.195%
17	12.414	1853	1858	1863	rBV	11280	14078	1.89%	0.303%
18	13.170	1978	1982	1986	rVB	7563	8894	1.19%	0.192%
19	13.292	1997	2002	2007	rVV2	21435	27402	3.67%	0.590%
20	13.426	2018	2024	2030	rBV2	25855	33570	4.50%	0.723%
21	13.780	2076	2082	2091	rBV	92318	118582	15.89%	2.554%
22	13.853	2091	2094	2102	rBV2	7168	12195	1.63%	0.263%
23	13.926	2102	2106	2110	rVV2	8227	9700	1.30%	0.209%
24	14.079	2125	2131	2137	rBV2	5593	7707	1.03%	0.166%
25	14.231	2149	2156	2163	rBV2	26536	40659	5.45%	0.876%
26	14.371	2175	2179	2184	rVB	7341	9747	1.31%	0.210%
27	14.481	2192	2197	2204	rBV2	24122	31401	4.21%	0.676%
28	14.639	2215	2223	2227	rBV	45631	63423	8.50%	1.366%
29	14.780	2240	2246	2251	rBV2	35875	47138	6.32%	1.015%
30	15.182	2306	2312	2315	rBV	10744	17893	2.40%	0.385%
31	15.481	2358	2361	2364	rVV3	6159	9162	1.23%	0.197%
32	15.615	2379	2383	2387	rBV3	7525	10807	1.45%	0.233%
33	15.743	2399	2404	2408	rVB6	5817	11200	1.50%	0.241%


Sum of corrected areas: 4643283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024625.D
Acq On : 06 Oct 2021 18:08
Operator : JC/MD
Sample : M4088-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-20211005-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

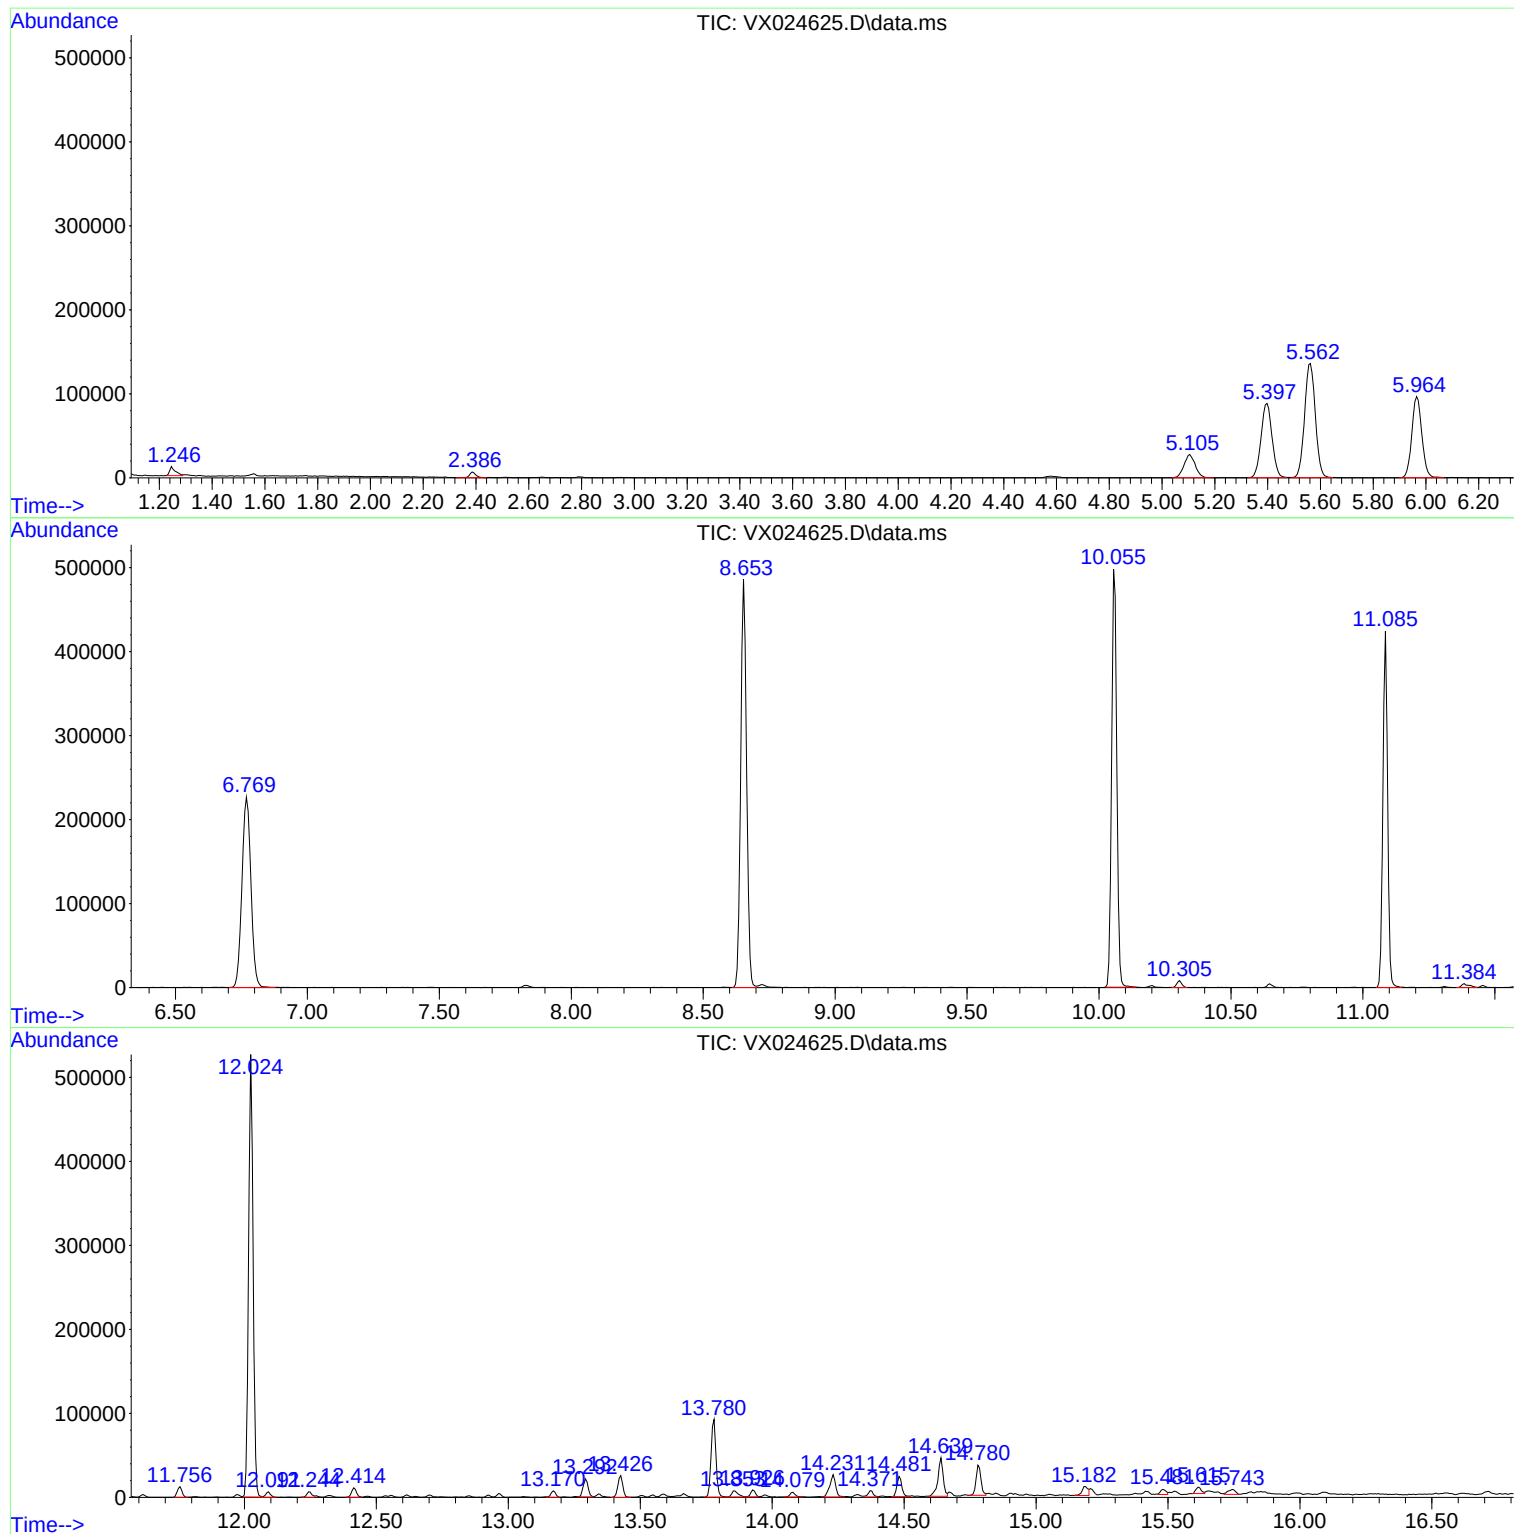

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024625.D
Acq On : 06 Oct 2021 18:08
Operator : JC/MD
Sample : M4088-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-20211005-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024625.D
Acq On : 06 Oct 2021 18:08
Operator : JC/MD
Sample : M4088-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-20211005-WATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc