

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
 Data File : VX024631.D
 Acq On : 06 Oct 2021 20:29
 Operator : JC/MD
 Sample : M4060-01
 Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TR-05-100421

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	36	rBV2	10274	23090	3.22%	0.597%
2	1.581	71	81	82	rBV5	5020	12662	1.77%	0.327%
3	5.397	695	707	718	rBV2	76520	225797	31.53%	5.840%
4	5.556	721	733	746	rVB	133015	375642	52.45%	9.716%
5	5.964	789	800	817	rBV	90801	243829	34.05%	6.306%
6	6.373	860	867	880	rBV5	2475	7562	1.06%	0.196%
7	6.763	921	931	947	rBV	217275	512153	71.52%	13.246%
8	8.653	1234	1241	1253	rBV	458688	716135	100.00%	18.522%
9	10.055	1465	1471	1484	rBV	463502	644107	89.94%	16.659%
10	11.085	1634	1640	1652	rBV	391617	501395	70.01%	12.968%
11	12.024	1789	1794	1802	rBV	488350	603967	84.34%	15.621%




Sum of corrected areas: 3866339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024631.D
Acq On : 06 Oct 2021 20:29
Operator : JC/MD
Sample : M4060-01
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-05-100421

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

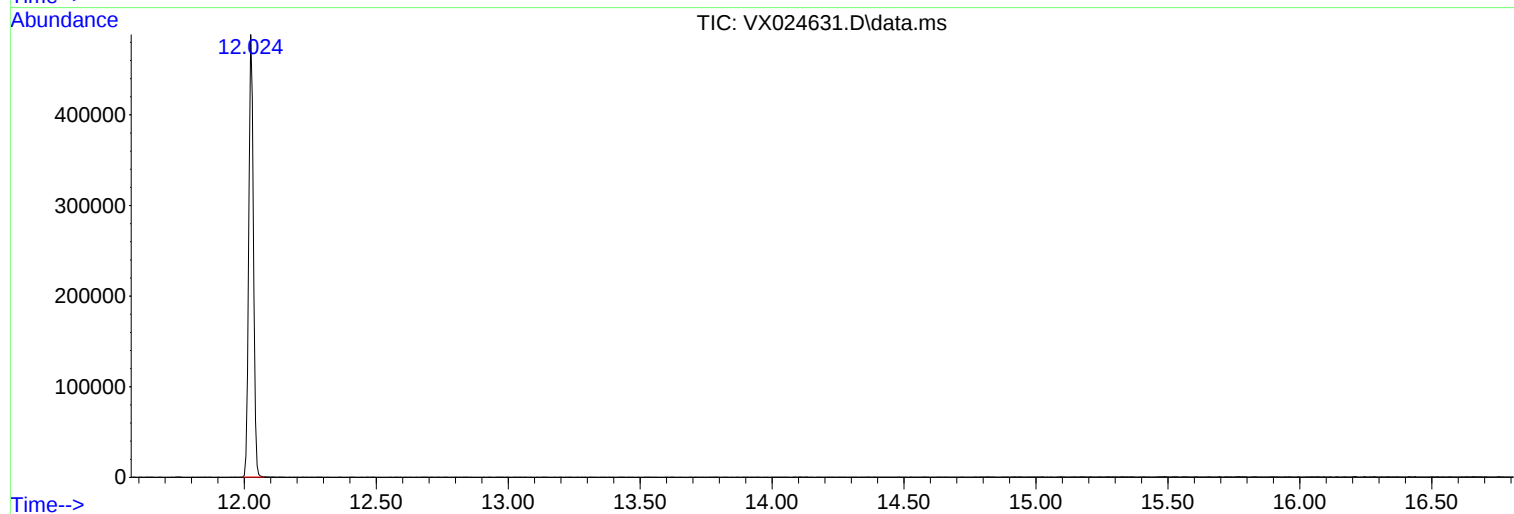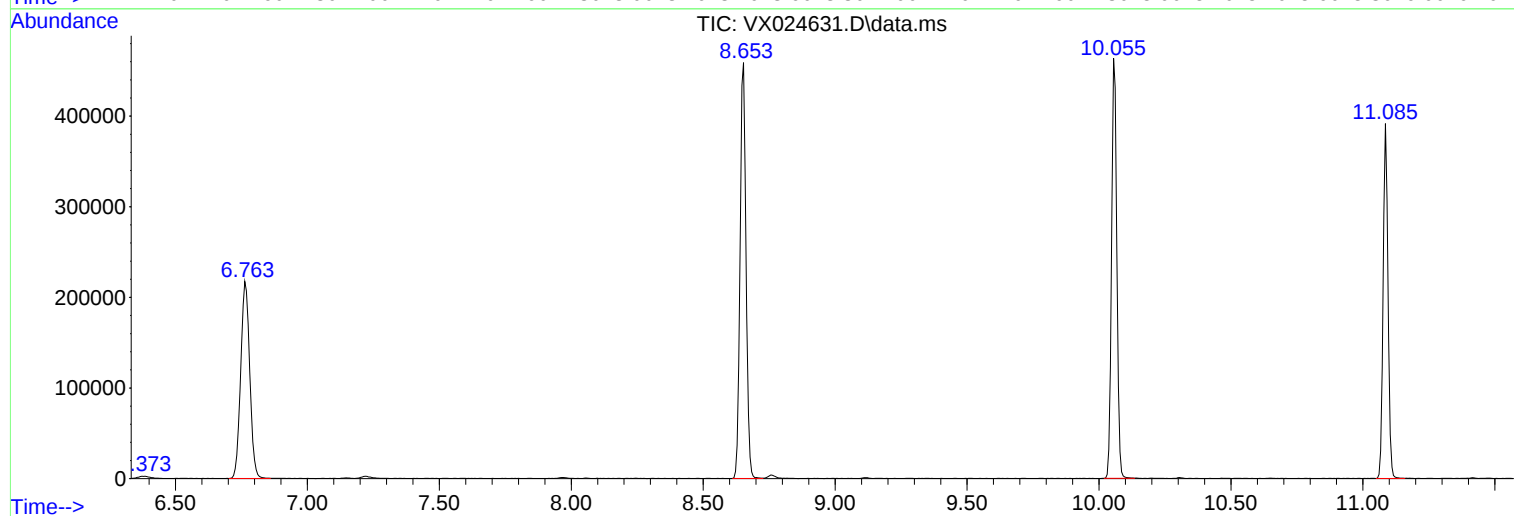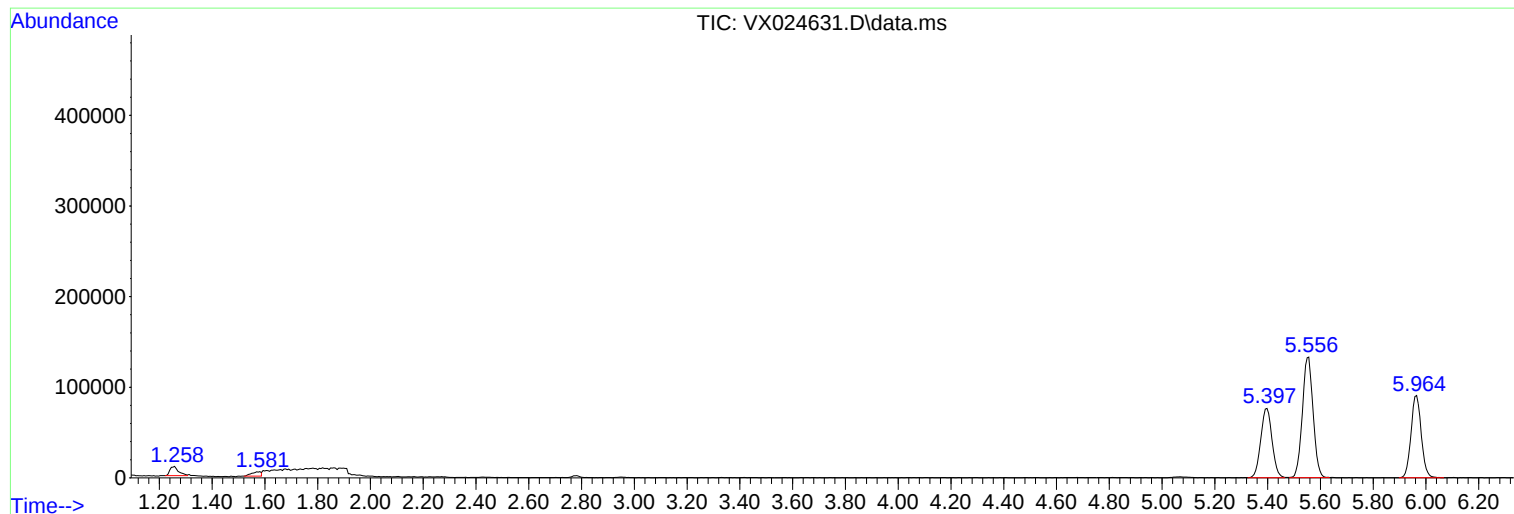

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024631.D
Acq On : 06 Oct 2021 20:29
Operator : JC/MD
Sample : M4060-01
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-05-100421

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100621\
Data File : VX024631.D
Acq On : 06 Oct 2021 20:29
Operator : JC/MD
Sample : M4060-01
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR-05-100421

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc