

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
 Data File : VX031933.D
 Acq On : 06 Oct 2022 21:14
 Operator : JC/MD
 Sample : N4882-13 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-124

Quant Time: Oct 07 08:08:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	54525	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	92129	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	98530	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	61963	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	65009	57.732	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 115.460%			
35) Dibromofluoromethane	5.385	113	53161	50.977	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.960%			
50) Toluene-d8	8.647	98	185739	49.497	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 99.000%			
62) 4-Bromofluorobenzene	11.079	95	67454	50.846	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 101.700%			
Target Compounds						Qvalue
5) Bromomethane	1.611	94	305	Below Cal		96
6) Chloroethane	1.679	64	202	0.239 ug/l #		43
11) Tert butyl alcohol	2.941	59	5650	40.328 ug/l #		73
16) Acetone	2.386	43	1259	3.290 ug/l		91
18) Methyl Acetate	2.782	43	269	0.213 ug/l #		52
19) Methyl tert-butyl Ether	3.117	73	9821	3.524 ug/l		95
20) Methylene Chloride	2.788	84	632	0.628 ug/l #		83
25) 2-Butanone	4.587	43	586	0.980 ug/l		96
31) Cyclohexane	5.471	56	1511	1.123 ug/l #		86
36) 1,1-Dichloropropene	5.550	75	4391	3.175 ug/l #		49
38) Carbon Tetrachloride	5.556	117	5627	3.980 ug/l #		16
39) Methylcyclohexane	7.385	83	1931	1.171 ug/l #		75
40) Benzene	6.037	78	15541	3.838 ug/l		99
42) 1,2-Dichloroethane	6.105	62	603	0.409 ug/l #		75
51) 4-Methyl-2-Pentanone	8.574	43	472	0.361 ug/l		92
52) Toluene	8.720	92	19741	7.456 ug/l		98
53) t-1,3-Dichloropropene	8.714	75	237	1.369 ug/l #		1
67) Ethyl Benzene	10.195	91	153310	30.355 ug/l		96
68) m/p-Xylenes	10.299	106	128320	63.935 ug/l		98
69) o-Xylene	10.640	106	37513	19.230 ug/l		99
70) Styrene	10.640	104	2224	0.713 ug/l #		1
73) Isopropylbenzene	10.963	105	3367	0.720 ug/l		95
74) N-amyl acetate	10.896	43	1244	0.872 ug/l #		50
76) 1,2,3-Trichloropropane	11.079	75	33664	26.509 ug/l #		37
78) n-propylbenzene	11.305	91	11887	2.236 ug/l		96
79) 2-Chlorotoluene	11.378	91	7366	2.303 ug/l #		41
80) 1,3,5-Trimethylbenzene	11.451	105	45428	11.720 ug/l		98
81) trans-1,4-Dichloro-2-b...	11.079	75	33664	90.898 ug/l #		11
82) 4-Chlorotoluene	11.451	91	5286	1.443 ug/l #		44
83) tert-Butylbenzene	11.713	119	2418	0.630 ug/l		85
84) 1,2,4-Trimethylbenzene	11.756	105	79832	20.275 ug/l		98
85) sec-Butylbenzene	11.756	105	79832	16.809 ug/l #		56
89) n-Butylbenzene	12.317	91	2723	0.813 ug/l #		3
90) Hexachloroethane	12.530	117	532	2.123 ug/l #		15
95) Naphthalene	13.774	128	37918	8.366 ug/l		100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031933.D
Acq On : 06 Oct 2022 21:14
Operator : JC/MD
Sample : N4882-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-124

Quant Time: Oct 07 08:08:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031933.D
Acq On : 06 Oct 2022 21:14
Operator : JC/MD
Sample : N4882-13 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-124

Quant Time: Oct 07 08:08:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




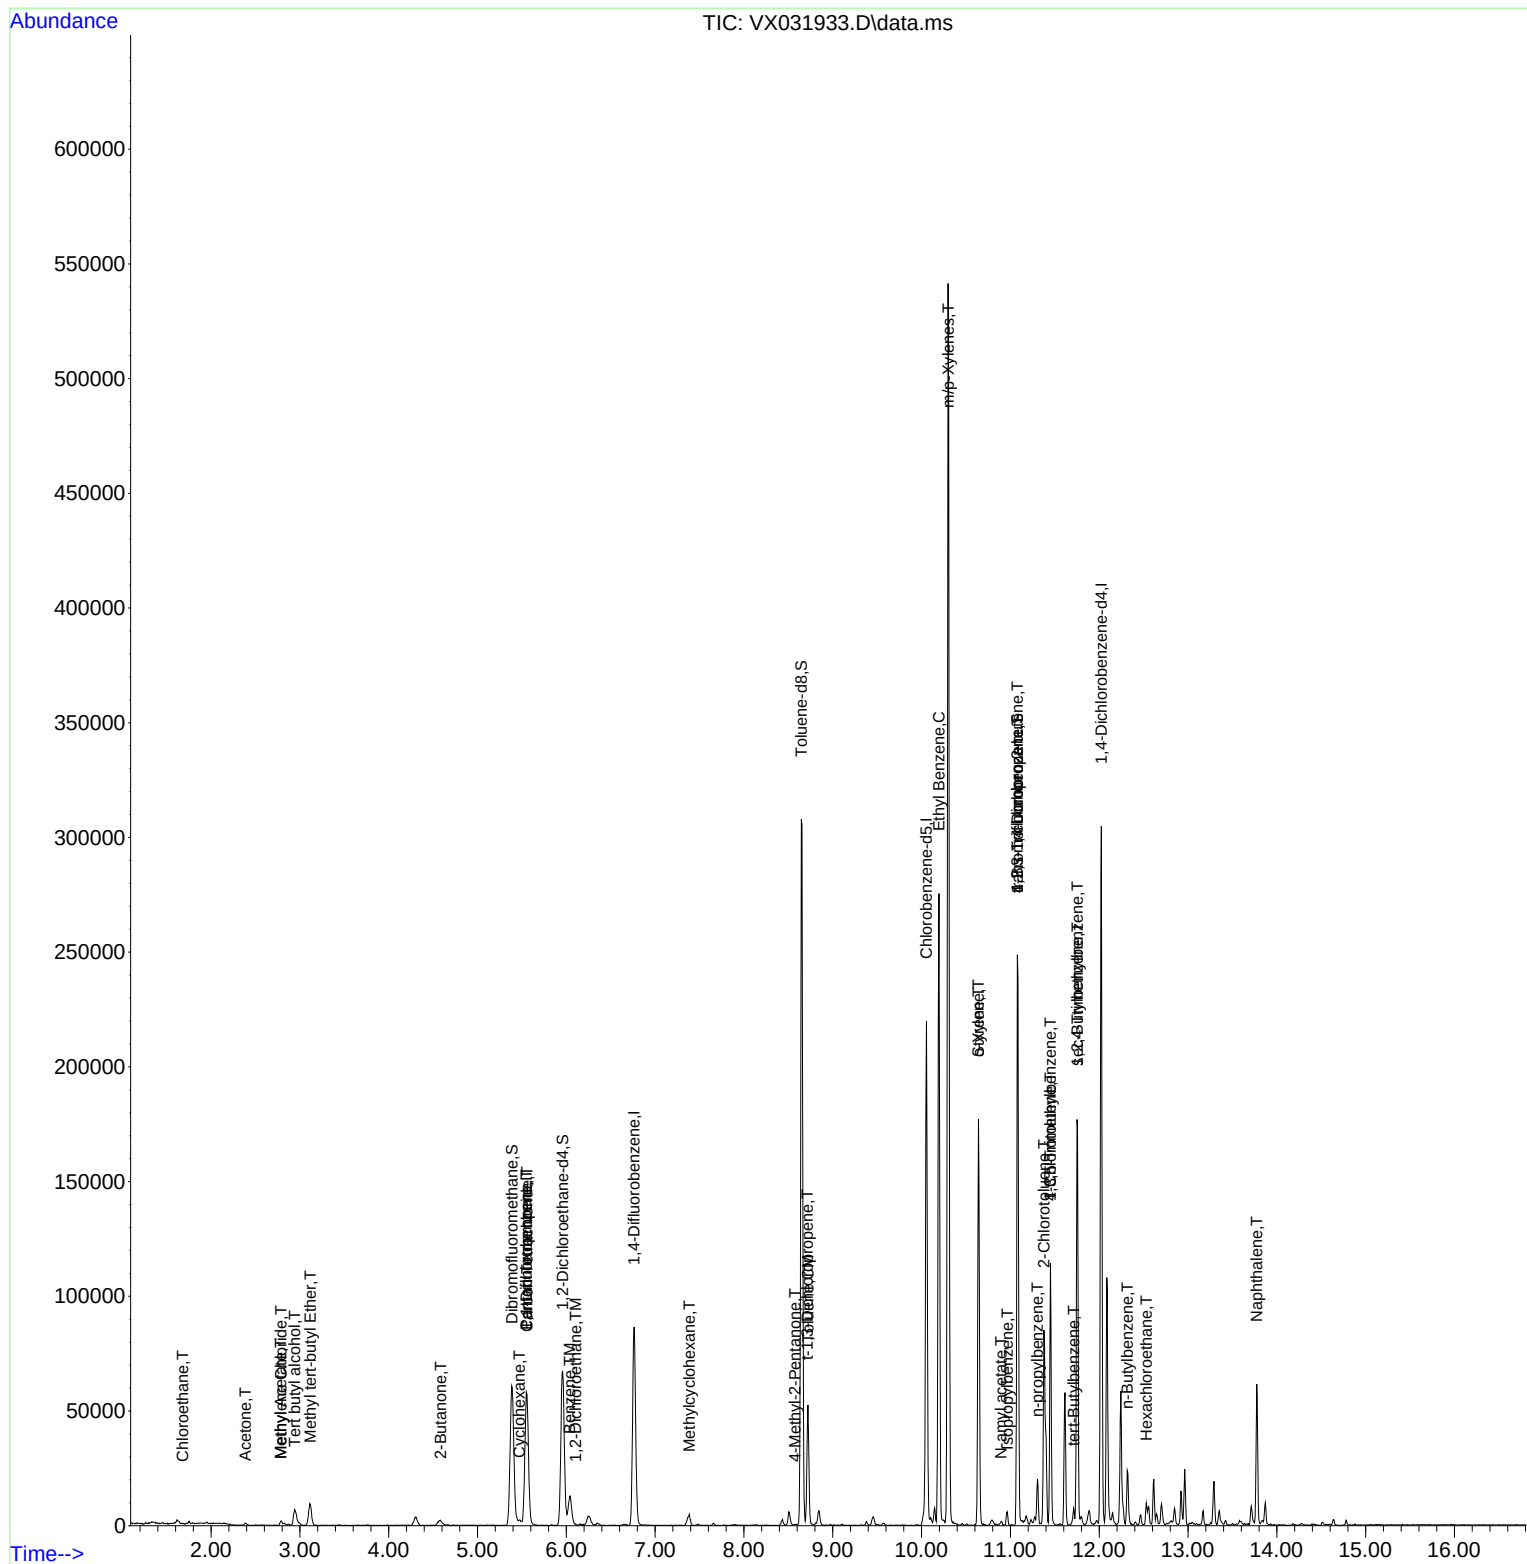




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion:168 Resp: 54525
Ion Ratio Lower Upper
168 100
99 59.0 48.8 73.2

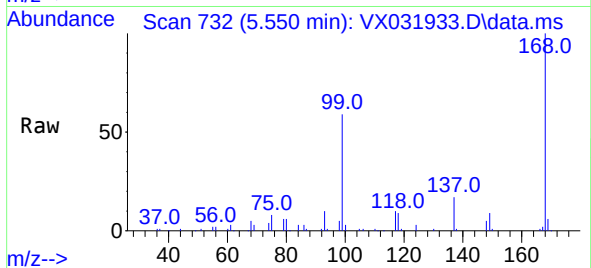

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 94 Resp: 305
Ion Ratio Lower Upper
94 100
96 97.2 74.4 111.6


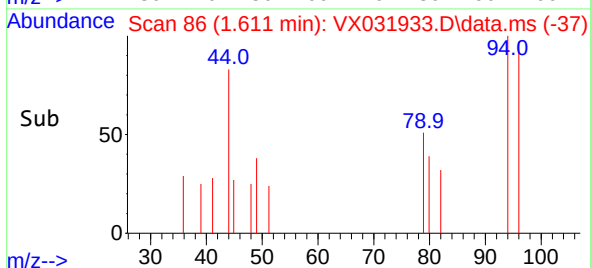
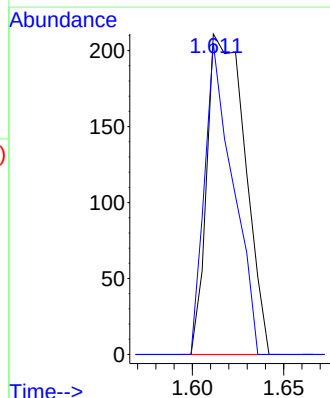



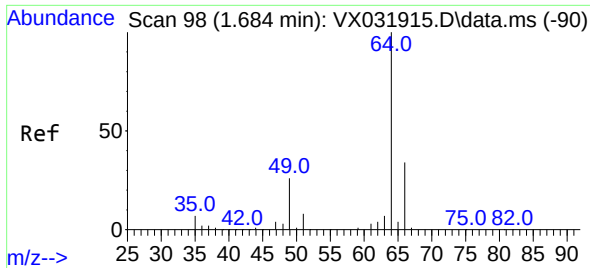

#6
Chloroethane
Concen: 0.239 ug/l
RT: 1.679 min Scan# 91
Delta R.T. -0.005 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 64 Resp: 202
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

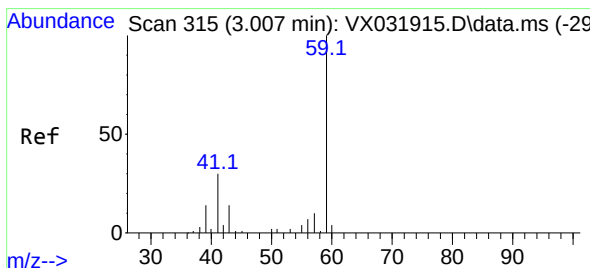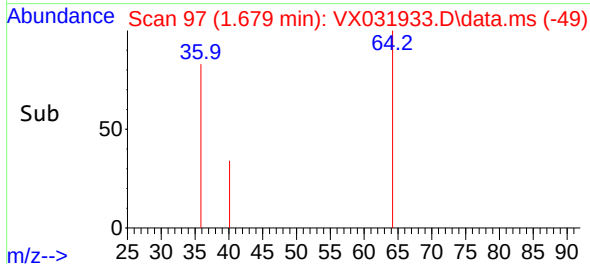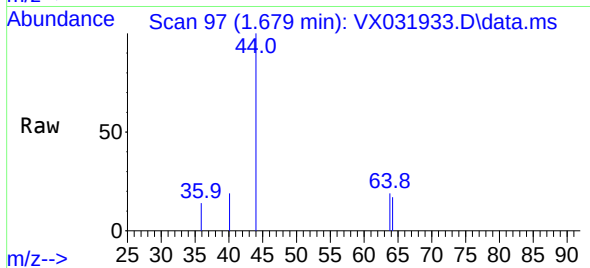

#11
Tert butyl alcohol
Concen: 40.328 ug/l
RT: 2.941 min Scan# 304
Delta R.T. -0.067 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 59 Resp: 5650
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#


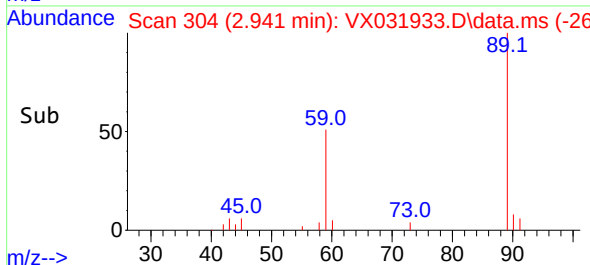
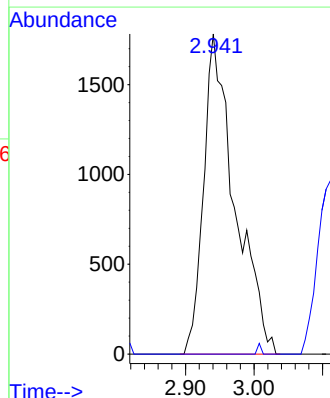
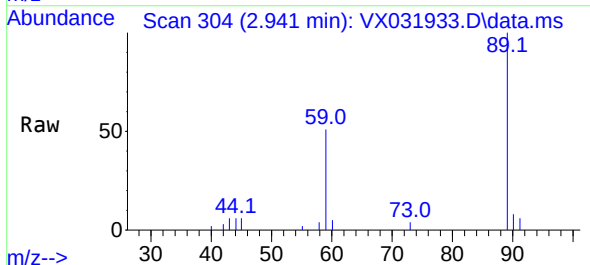




#16
Acetone
Concen: 3.290 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 43 Resp: 1259
Ion Ratio Lower Upper
43 100
58 25.0 23.8 35.8



#18
Methyl Acetate
Concen: 0.213 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.073 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 43 Resp: 269
Ion Ratio Lower Upper
43 100
74 0.0 18.6 27.8#

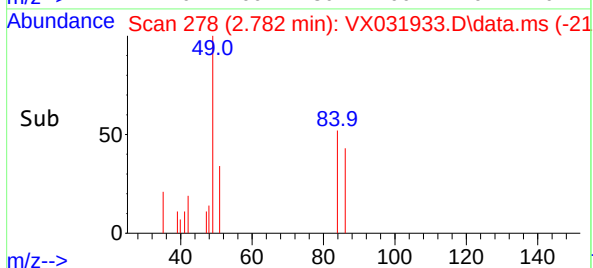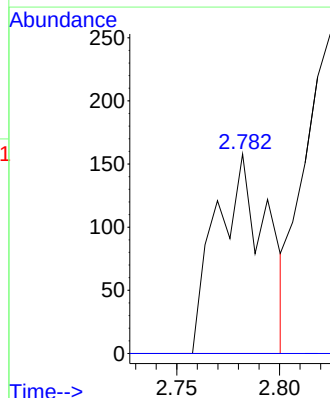



#19

Methyl tert-butyl Ether

Concen: 3.524 ug/l

RT: 3.117 min Scan# 31

Delta R.T. 0.000 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14

Instrument :

MSVOA_X

ClientSampleId :





MW-124

Tgt Ion: 73 Resp: 9821

Ion Ratio Lower Upper

73 100

57 23.7 17.2 25.8

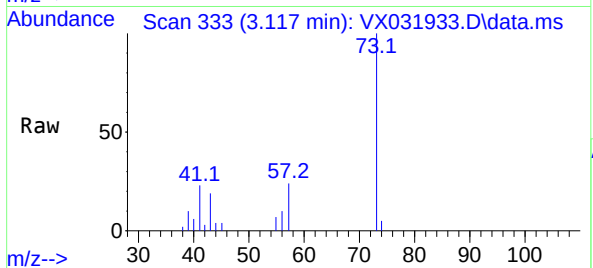

#20

Methylene Chloride

Concen: 0.628 ug/l

RT: 2.788 min Scan# 279

Delta R.T. 0.000 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14

Tgt Ion: 84 Resp: 632




Ion Ratio Lower Upper


84 100

49 111.2 105.9 158.9

51 32.8 32.2 48.2

86 49.3 50.8 76.2#

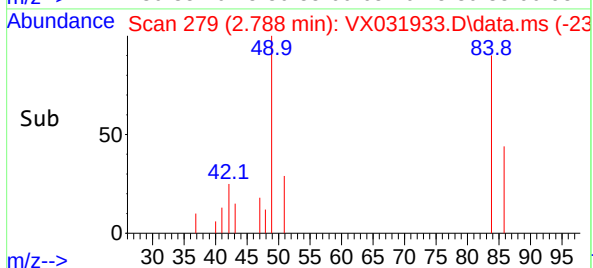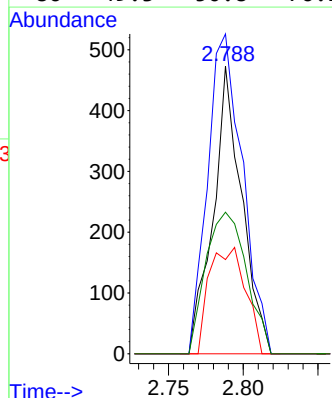



#25

2-Butanone

Concen: 0.980 ug/l

RT: 4.587 min Scan# 51

Delta R.T. 0.025 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14

Instrument :

MSVOA_X

ClientSampleId :





MW-124

Tgt Ion: 43 Resp: 586

Ion Ratio Lower Upper

43 100

72 24.5 21.1 31.7

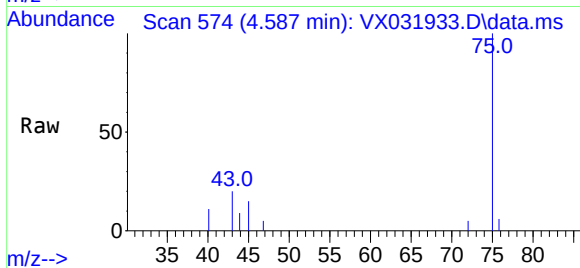

#31

Cyclohexane

Concen: 1.123 ug/l

RT: 5.471 min Scan# 719

Delta R.T. 0.001 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14




Tgt Ion: 56 Resp: 1511


Ion Ratio Lower Upper

56 100

69 19.7 25.1 37.7#

84 98.9 70.2 105.4

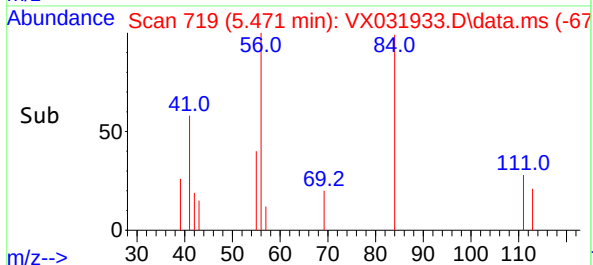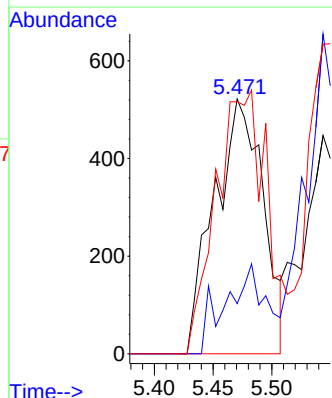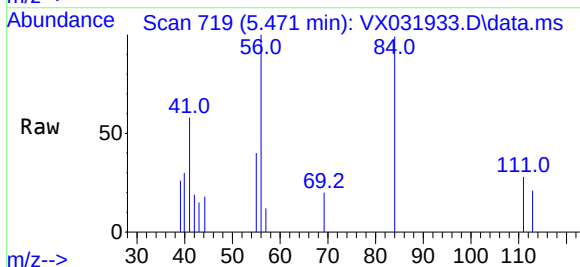



#33

1,2-Dichloroethane-d4

Concen: 57.732 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14

Instrument :

MSVOA_X

ClientSampleId :





MW-124

Tgt Ion: 65 Resp: 65009

Ion Ratio Lower Upper

65 100

67 50.8 0.0 102.4

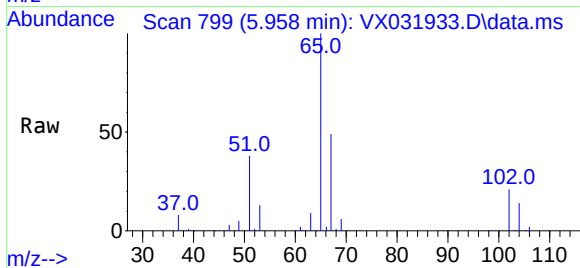

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14




Tgt Ion: 114 Resp: 92129


Ion Ratio Lower Upper

114 100

63 19.3 0.0 42.6

88 14.4 0.0 33.0

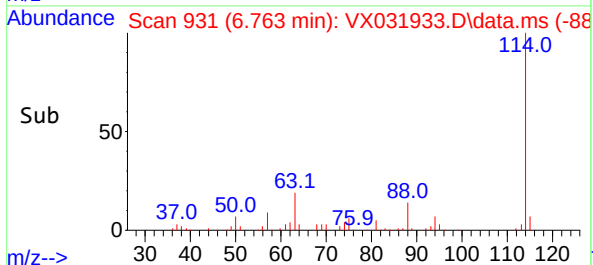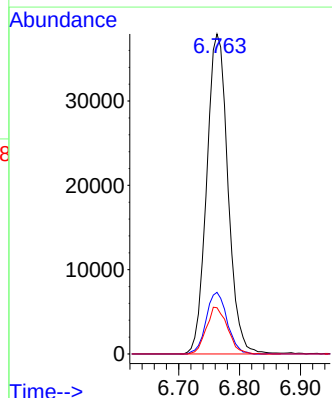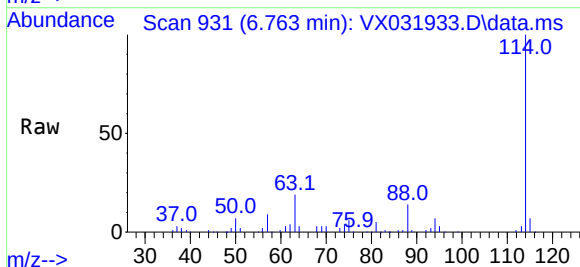

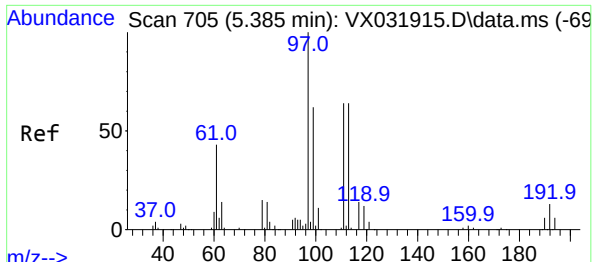

#35

Dibromofluoromethane

Concen: 50.977 ug/l

RT: 5.385 min Scan# 705

Delta R.T. 0.000 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14

Instrument :

MSVOA_X

ClientSampleId :

MW-124





Tgt Ion:113 Resp: 53161

Ion Ratio Lower Upper

113 100

111 102.9 82.4 123.6

192 18.2 14.1 21.1

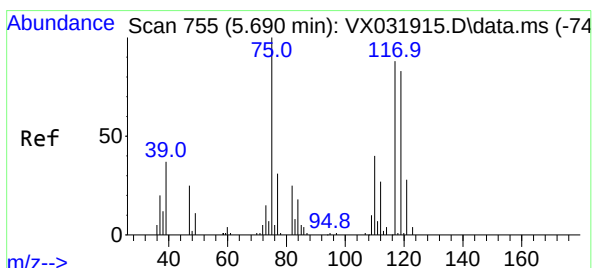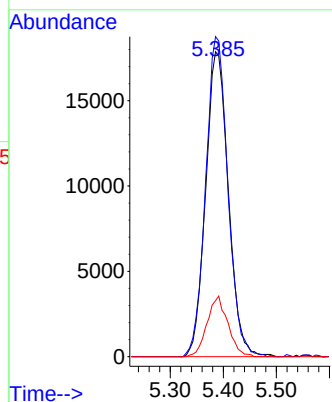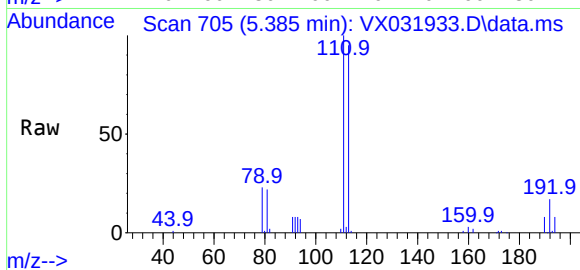

#36

1,1-Dichloropropene

Concen: 3.175 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14




Tgt Ion: 75 Resp: 4391


Ion Ratio Lower Upper

75 100

110 8.2 17.5 52.5#


77 0.0 24.9 37.3#

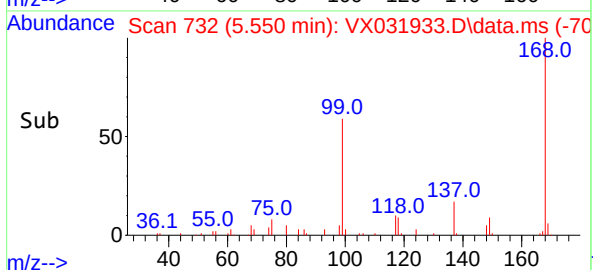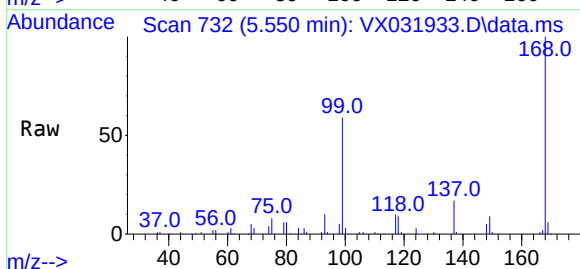






#38
Carbon Tetrachloride
Concen: 3.980 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.121 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Instrument :
MSVOA_X
ClientSampleId :
MW-124



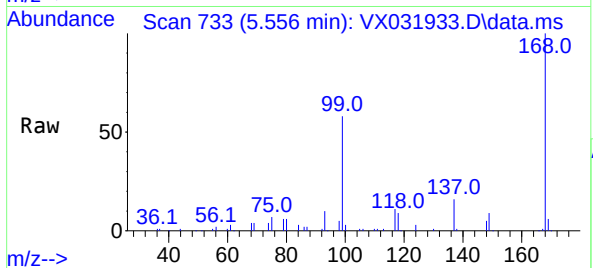



Tgt Ion:117 Resp: 5627
Ion Ratio Lower Upper
117 100
119 3.8 74.6 112.0#
121 0.0 25.3 37.9#



#39
Methylcyclohexane
Concen: 1.171 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 83 Resp: 1931
Ion Ratio Lower Upper
83 100
55 55.0 61.0 91.4#
98 63.4 37.7 56.5#


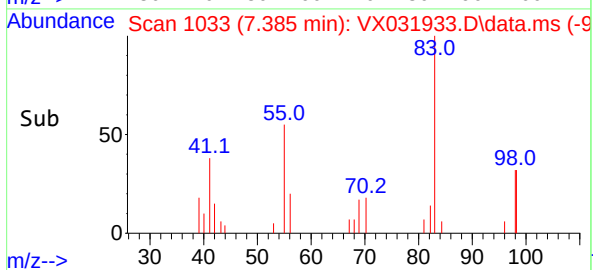






#40
Benzene
Concen: 3.838 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 78 Resp: 15541
Ion Ratio Lower Upper
78 100
77 22.9 18.7 28.1

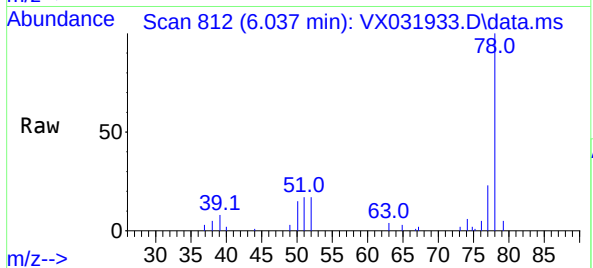

#42
1,2-Dichloroethane
Concen: 0.409 ug/l
RT: 6.105 min Scan# 823
Delta R.T. 0.013 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 62 Resp: 603
Ion Ratio Lower Upper
62 100
98 0.0 0.0 17.8


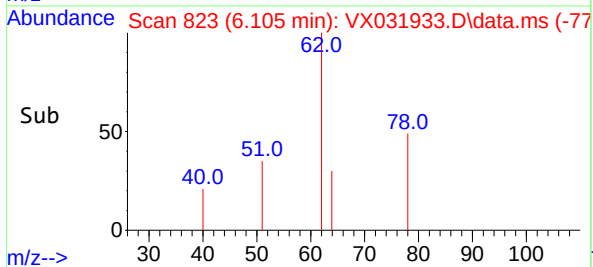

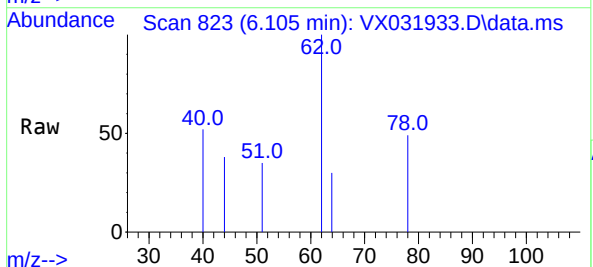




#50
Toluene-d8
Concen: 49.497 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 98 Resp: 185739
Ion Ratio Lower Upper
98 100
100 66.6 52.5 78.7

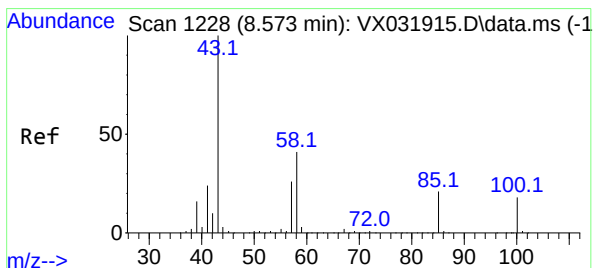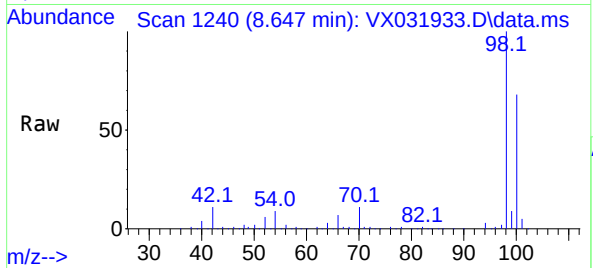

#51
4-Methyl-2-Pentanone
Concen: 0.361 ug/l
RT: 8.574 min Scan# 1228
Delta R.T. 0.001 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 43 Resp: 472
Ion Ratio Lower Upper
43 100
58 33.3 30.6 46.0


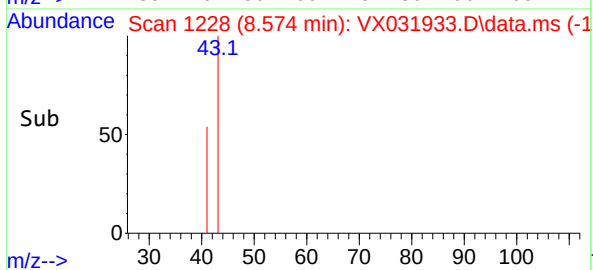

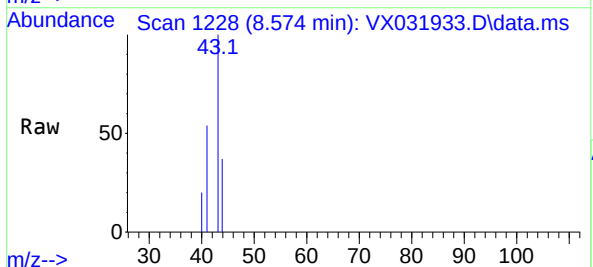




#52
Toluene
Concen: 7.456 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 92 Resp: 19741
Ion Ratio Lower Upper
92 100
91 169.3 137.1 205.7

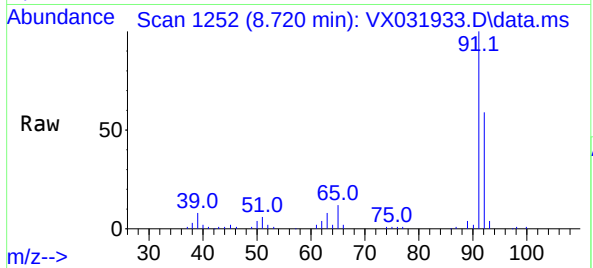

#53
t-1,3-Dichloropropene
Concen: 1.369 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.268 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 75 Resp: 237
Ion Ratio Lower Upper
75 100
77 114.4 24.8 37.2#


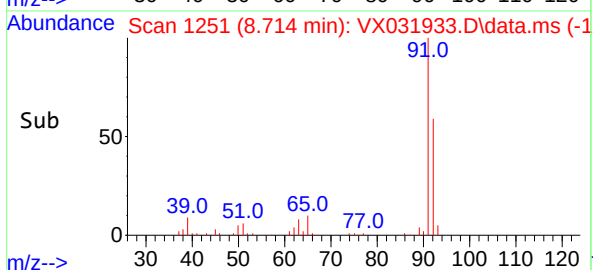






#62
4-Bromofluorobenzene
Concen: 50.846 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 95 Resp: 67454
Ion Ratio Lower Upper
95 100
174 78.0 0.0 153.2
176 74.7 0.0 144.0

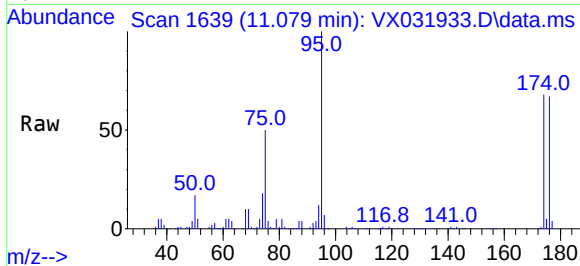

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 117 Resp: 98530
Ion Ratio Lower Upper
117 100
82 51.2 46.8 70.2
119 32.1 26.4 39.6


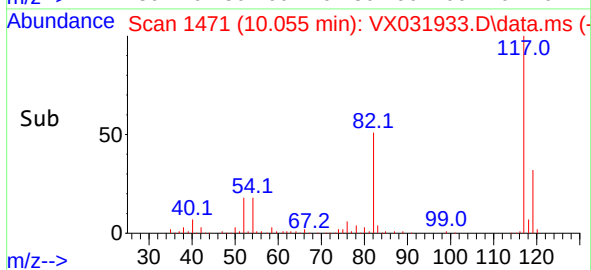

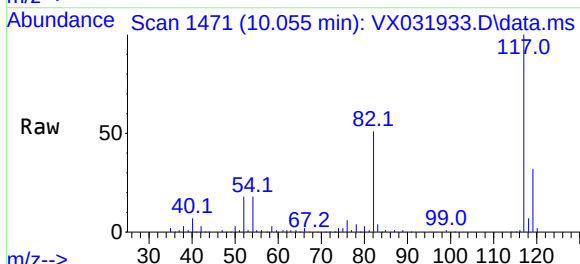




#67
Ethyl Benzene
Concen: 30.355 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 91 Resp: 153310
Ion Ratio Lower Upper
91 100
106 33.8 25.2 37.8

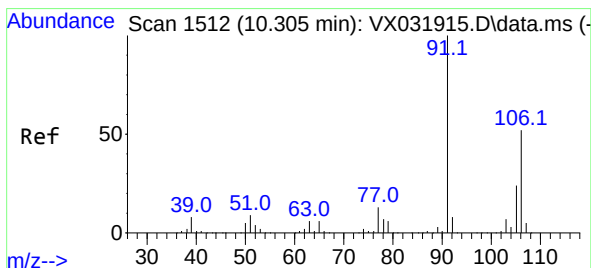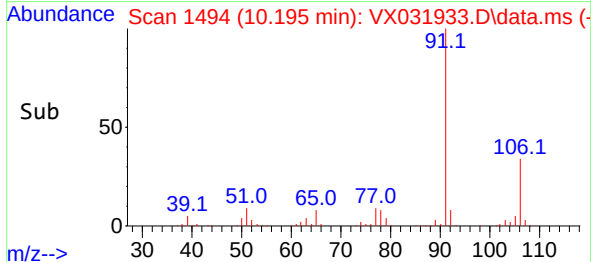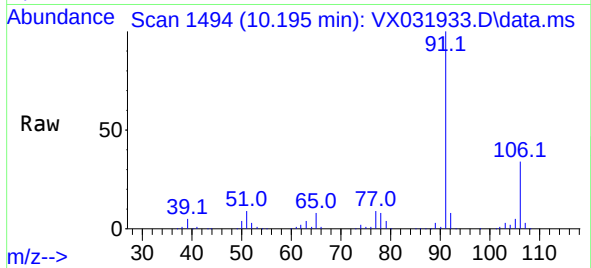

#68
m/p-Xylenes
Concen: 63.935 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 106 Resp: 128320
Ion Ratio Lower Upper
106 100
91 197.4 161.0 241.4

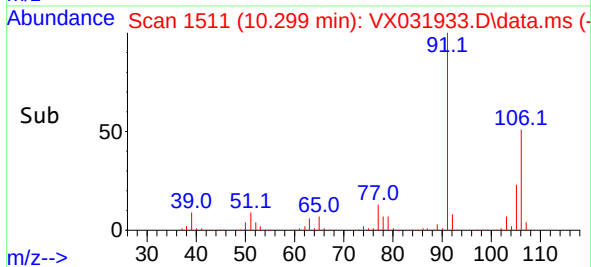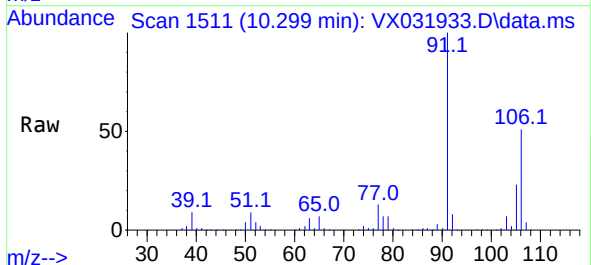



#69

o-Xylene

Concen: 19.230 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. 0.000 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14

Instrument :

MSVOA_X

ClientSampleId :





MW-124

Tgt Ion:106 Resp: 37513

Ion Ratio Lower Upper

106 100

91 213.0 107.2 321.6

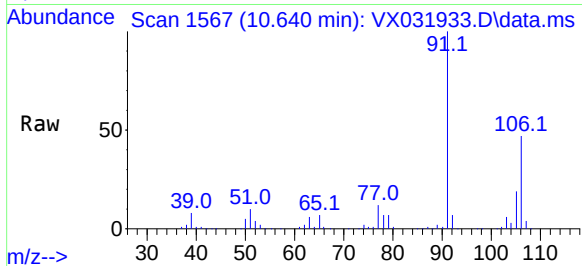

#70

Styrene

Concen: 0.713 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. -0.018 min

Lab File: VX031933.D

Acq: 06 Oct 2022 21:14




Tgt Ion:104 Resp: 2224


Ion Ratio Lower Upper

104 100

78 259.4 41.4 62.2#

103 236.6 43.8 65.8#


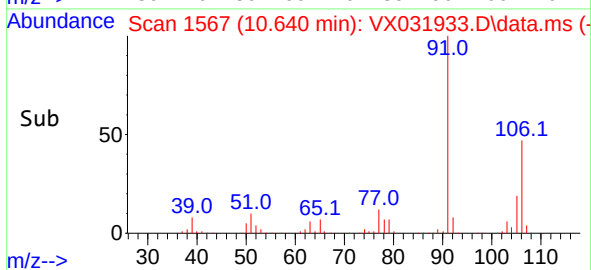

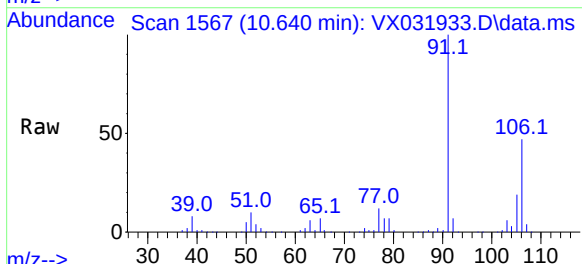




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion:152 Resp: 61963
Ion Ratio Lower Upper
152 100
115 61.5 43.4 130.1
150 162.2 0.0 346.8

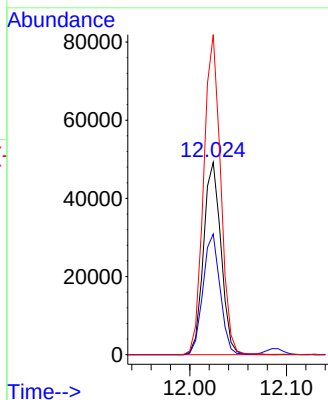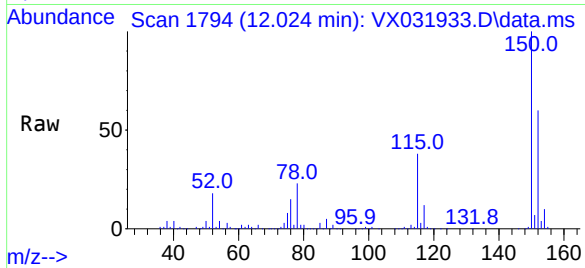

#73
Isopropylbenzene
Concen: 0.720 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion:105 Resp: 3367
Ion Ratio Lower Upper
105 100
120 29.8 13.7 41.0


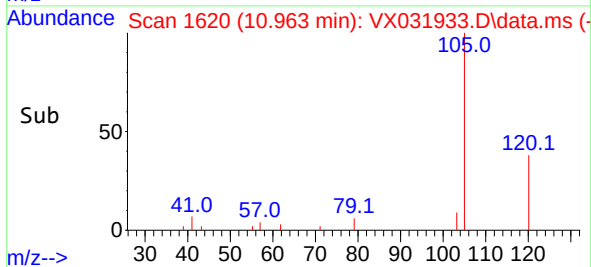
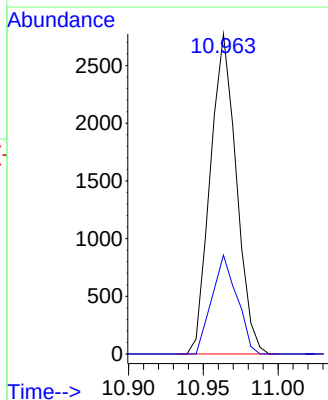
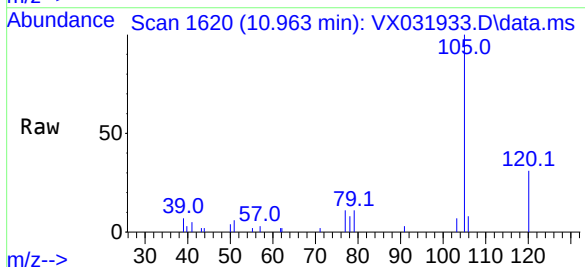




#74
N-amy1 acetate
Concen: 0.872 ug/l
RT: 10.896 min Scan# 1609
Delta R.T. 0.049 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion:	43	Resp:	1244
Ion	Ratio	Lower	Upper
43	100		
70	5.0	33.4	50.2#
55	5.0	18.2	27.2#
61	0.0	19.3	28.9#

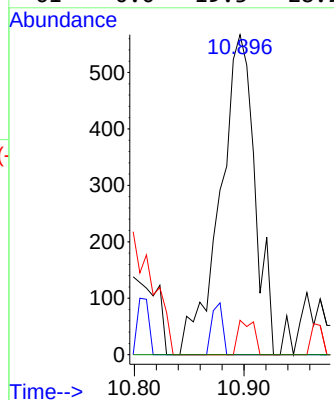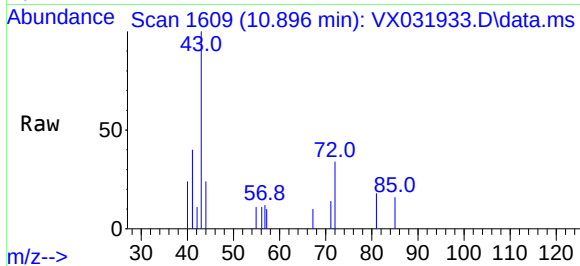

#76
1,2,3-Trichloropropane
Concen: 26.509 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion:	75	Resp:	33664
Ion	Ratio	Lower	Upper
75	100		
77	1.6	20.3	60.9#


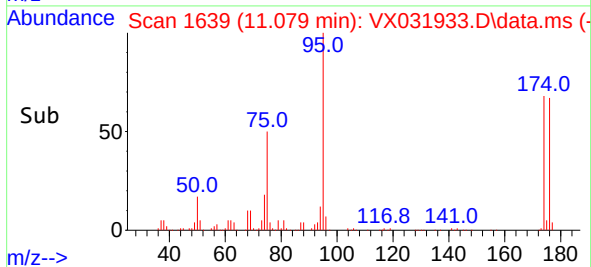
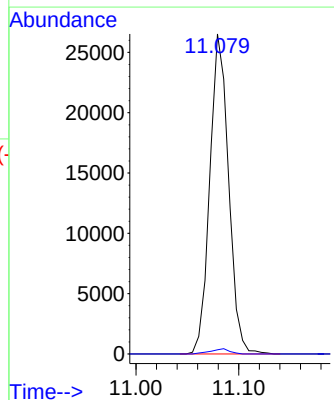
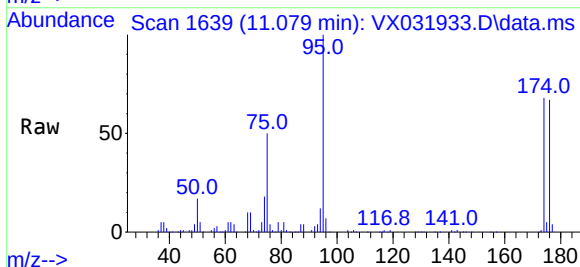




#78
n-propylbenzene
Concen: 2.236 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 91 Resp: 11887
Ion Ratio Lower Upper
91 100
120 25.5 11.8 35.4

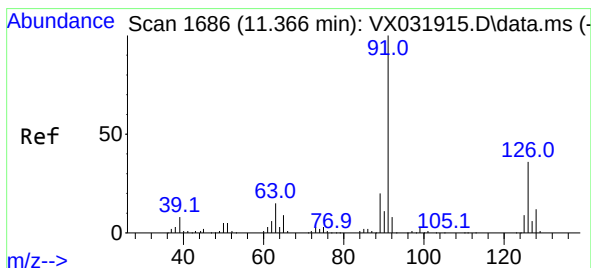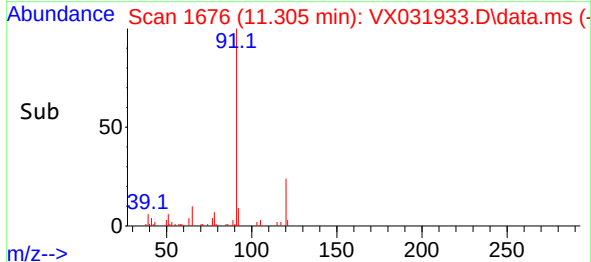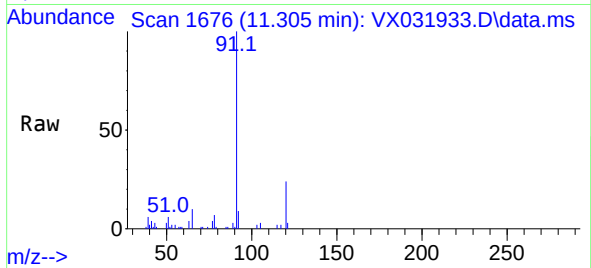

#79
2-Chlorotoluene
Concen: 2.303 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 91 Resp: 7366
Ion Ratio Lower Upper
91 100
126 0.8 17.4 52.3#


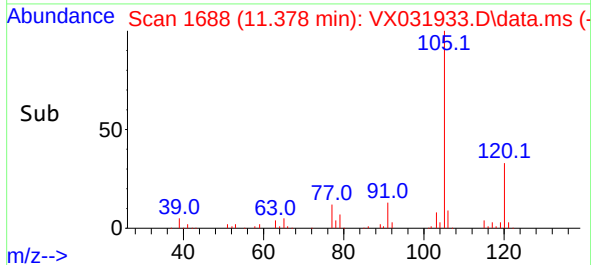

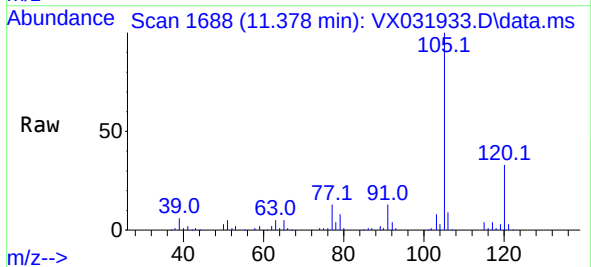




#80
1,3,5-Trimethylbenzene
Concen: 11.720 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion:105 Resp: 45428
Ion Ratio Lower Upper
105 100
120 50.5 24.5 73.5

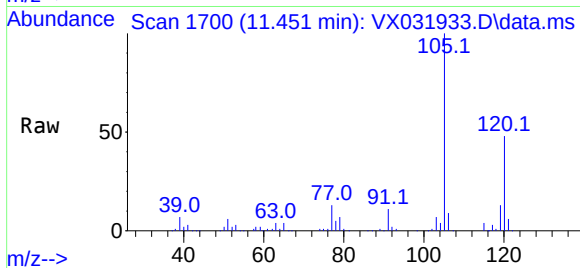

#81
trans-1,4-Dichloro-2-butene
Concen: 90.898 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 75 Resp: 33664
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#


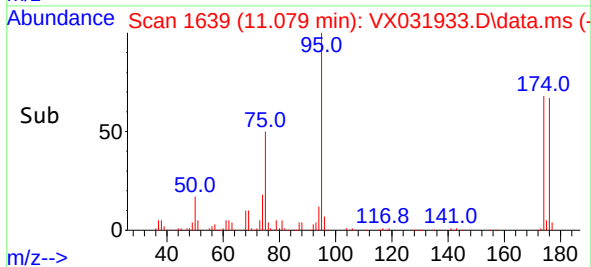

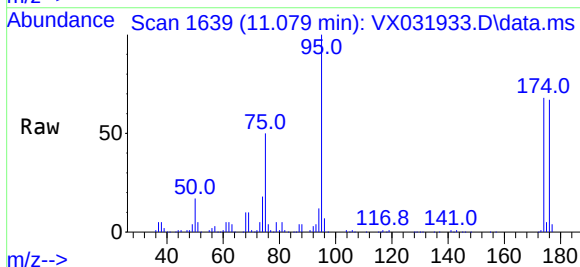




#82
4-Chlorotoluene
Concen: 1.443 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 91 Resp: 5286
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

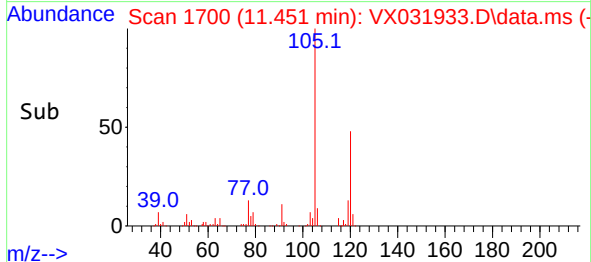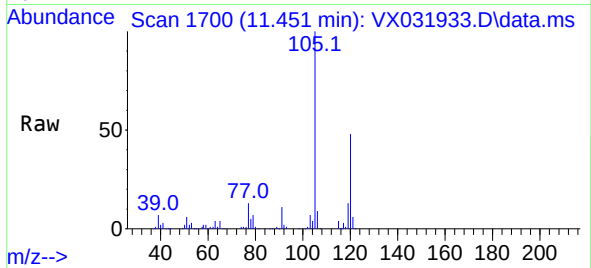

#83
tert-Butylbenzene
Concen: 0.630 ug/l
RT: 11.713 min Scan# 1743
Delta R.T. 0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 119 Resp: 2418
Ion Ratio Lower Upper
119 100
91 72.6 29.2 87.6
134 26.0 11.6 34.8


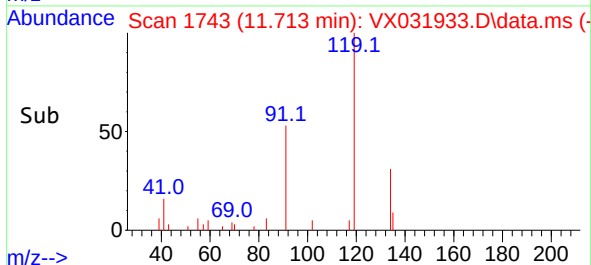
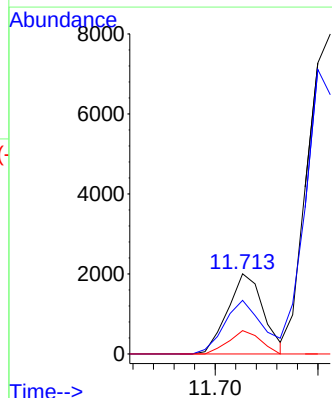
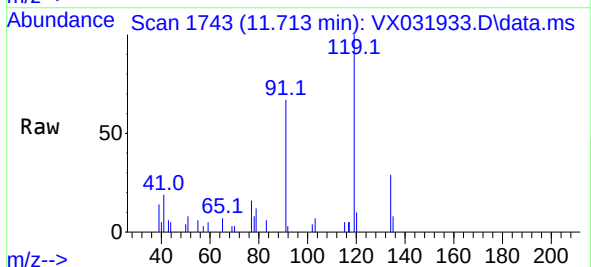




#84
1,2,4-Trimethylbenzene
Concen: 20.275 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion:105 Resp: 79832
Ion Ratio Lower Upper
105 100
120 46.5 22.6 67.8



#85
sec-Butylbenzene
Concen: 16.809 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion:105 Resp: 79832
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#


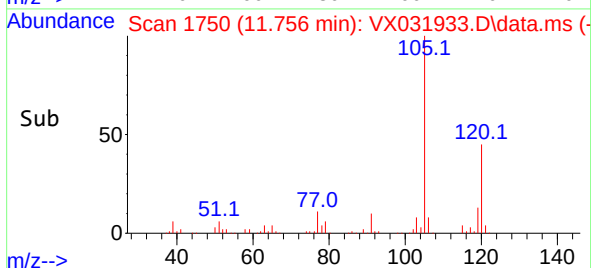
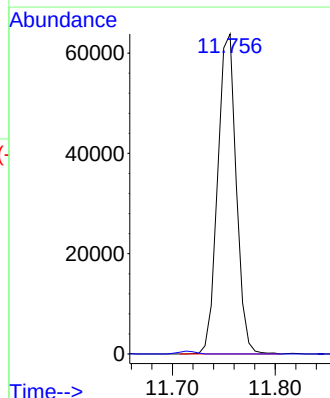





#89
n-Butylbenzene
Concen: 0.813 ug/l
RT: 12.317 min Scan# 119
Delta R.T. -0.018 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14




Instrument :
MSVOA_X
ClientSampleId :
MW-124


Tgt Ion: 91 Resp: 2723
Ion Ratio Lower Upper
91 100
92 22.9 27.0 81.0#
134 133.1 13.3 39.9#

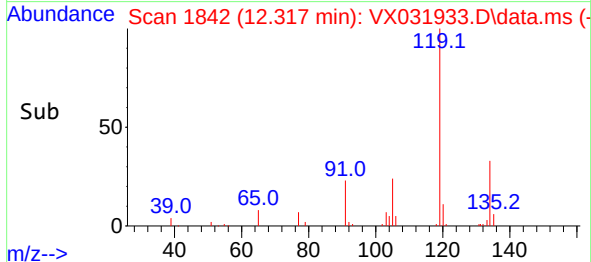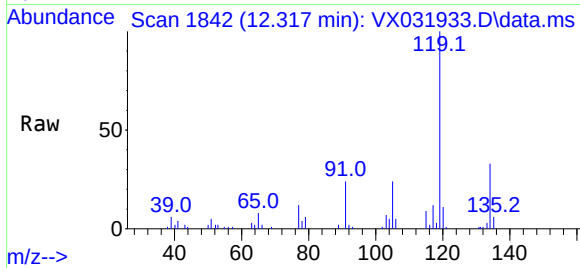

#90
Hexachloroethane
Concen: 2.123 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Tgt Ion: 117 Resp: 532
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

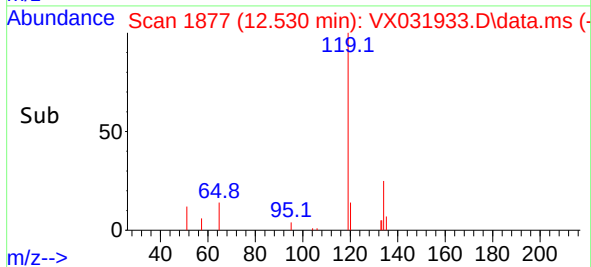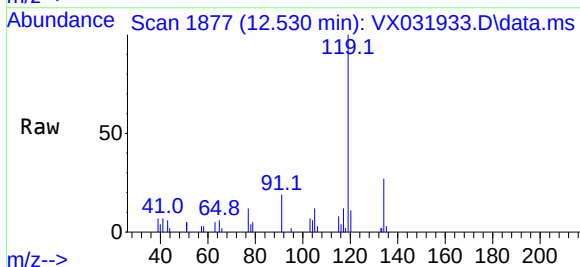

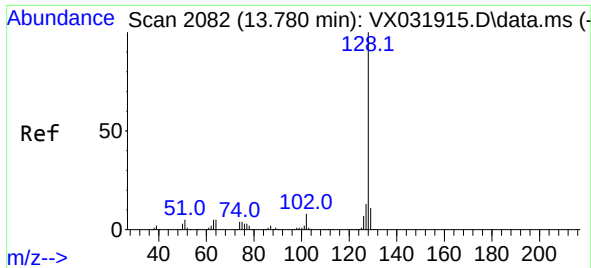

#95
Naphthalene
Concen: 8.366 ug/l
RT: 13.774 min Scan# 20
Delta R.T. -0.006 min
Lab File: VX031933.D
Acq: 06 Oct 2022 21:14

Instrument :
MSVOA_X
ClientSampleId :
MW-124

Tgt Ion:	128	Resp:	37918
Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.4	15.6
129	11.3	8.8	13.2

