

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
 Data File : VX031927.D
 Acq On : 06 Oct 2022 18:55
 Operator : JC/MD
 Sample : N5029-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-100522

Quant Time: Oct 07 08:08:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	63481	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	103544	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	110445	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	68521	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	69519	53.027	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 106.060%	
35) Dibromofluoromethane	5.385	113	57134	48.747	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.500%	
50) Toluene-d8	8.653	98	211835	50.228	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.460%	
62) 4-Bromofluorobenzene	11.079	95	72307	48.496	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 97.000%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031927.D
Acq On : 06 Oct 2022 18:55
Operator : JC/MD
Sample : N5029-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-100522

Quant Time: Oct 07 08:08:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




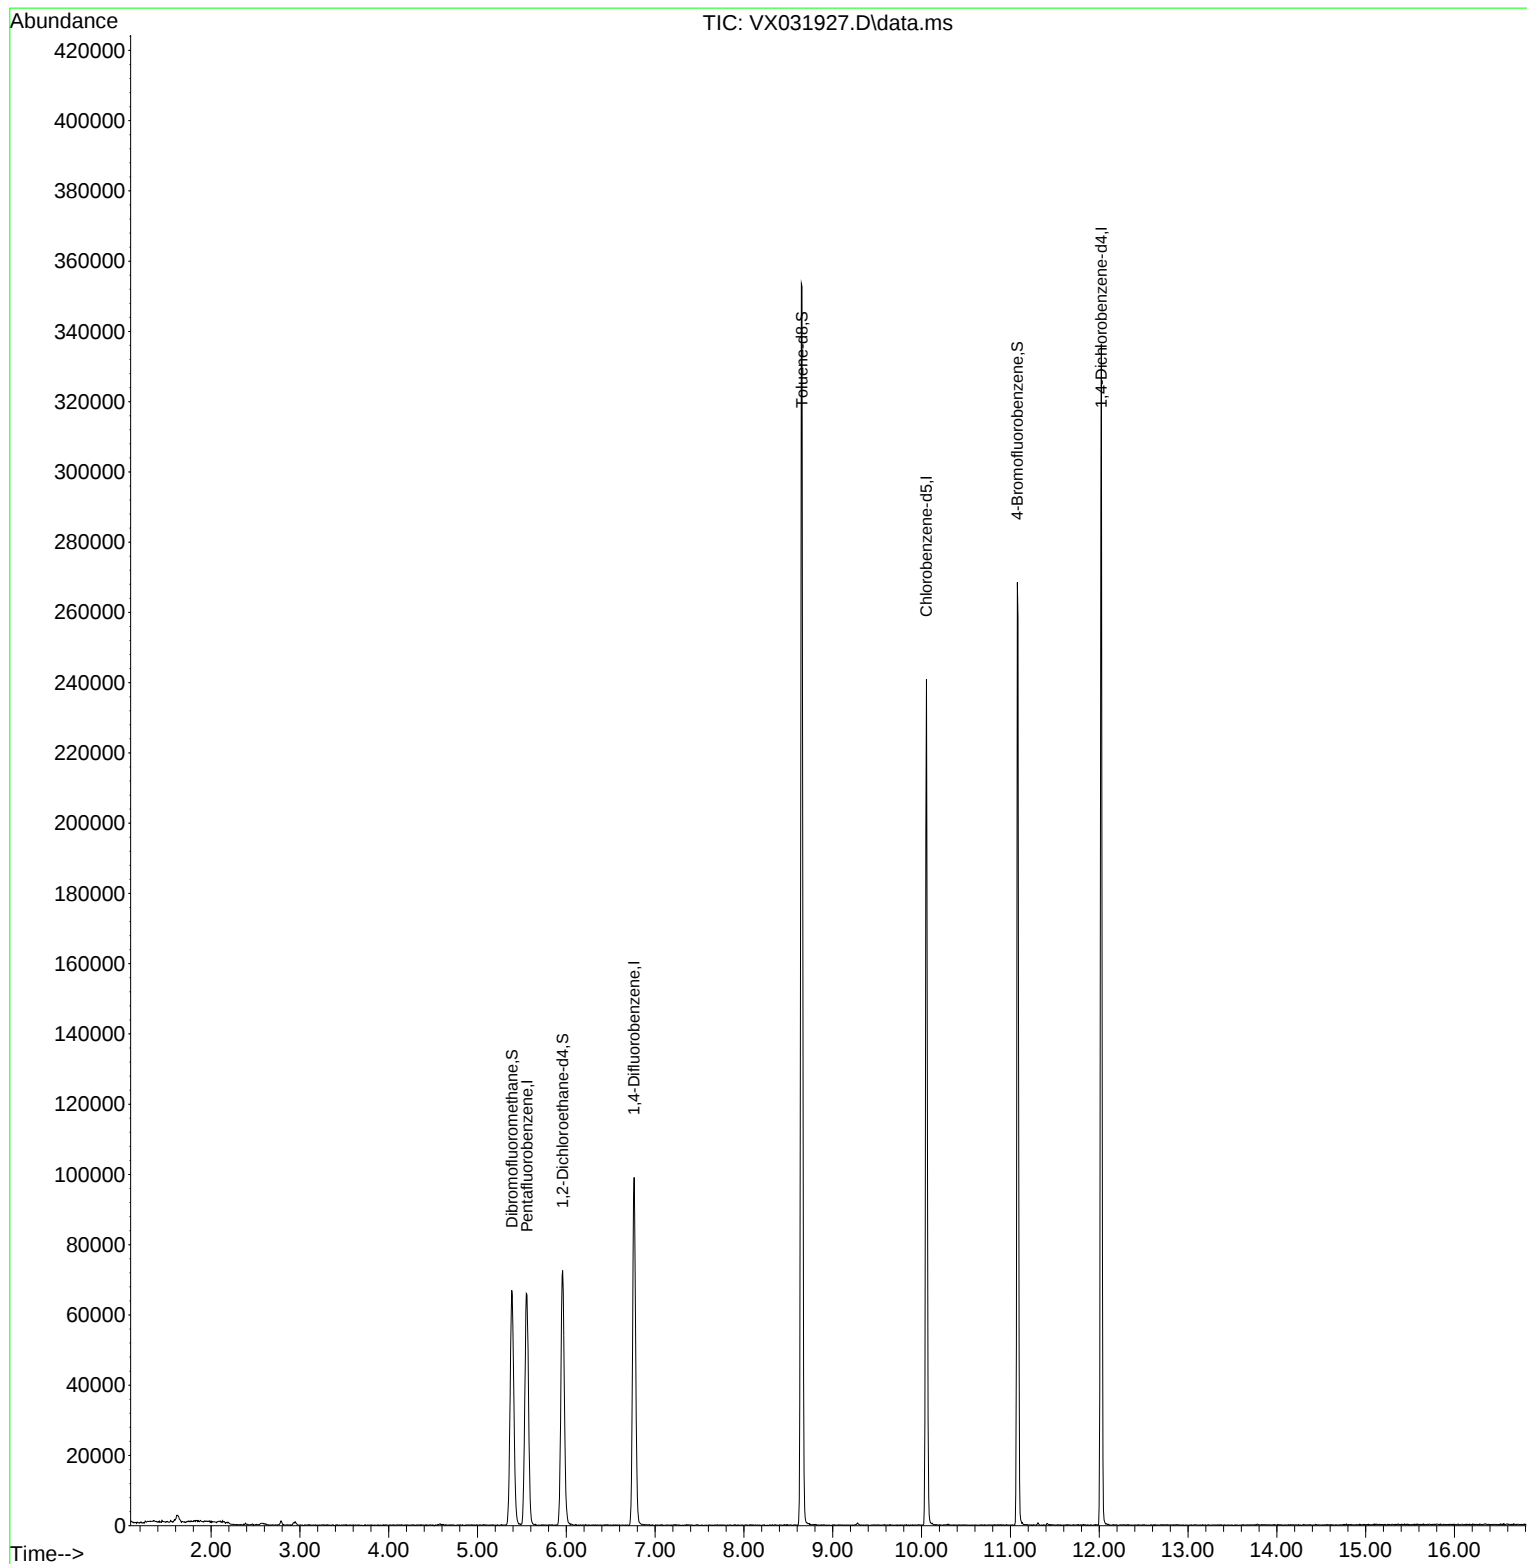




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55




Instrument :
MSVOA_X
ClientSampleId :
TB-01-100522


Tgt Ion:168 Resp: 63481
Ion Ratio Lower Upper
168 100
99 60.0 48.8 73.2

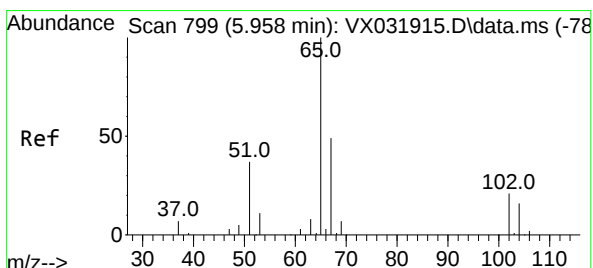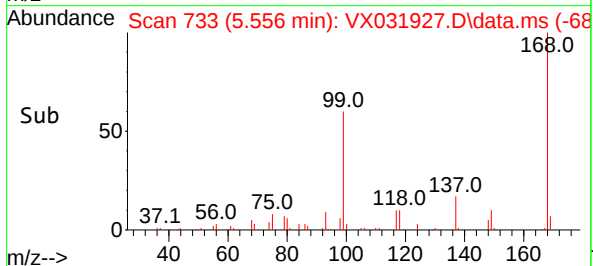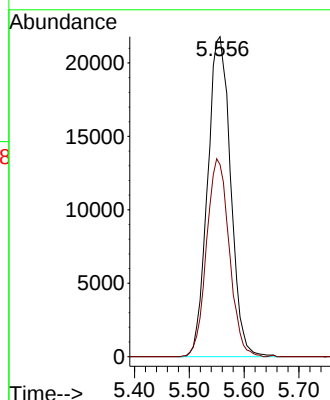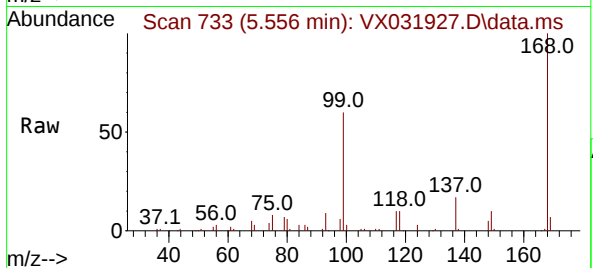

#33
1,2-Dichloroethane-d4
Concen: 53.027 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55

Tgt Ion: 65 Resp: 69519
Ion Ratio Lower Upper
65 100
67 51.1 0.0 102.4


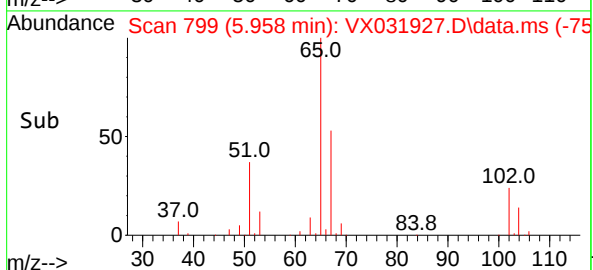
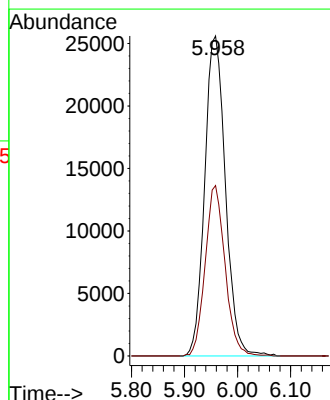
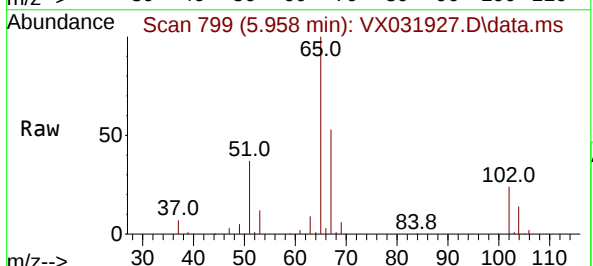


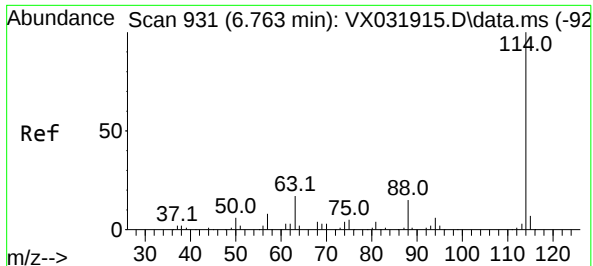

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55




Instrument :
MSVOA_X
ClientSampleId :
TB-01-100522


Tgt Ion:114 Resp: 103544
Ion Ratio Lower Upper
114 100
63 18.5 0.0 42.6
88 14.9 0.0 33.0

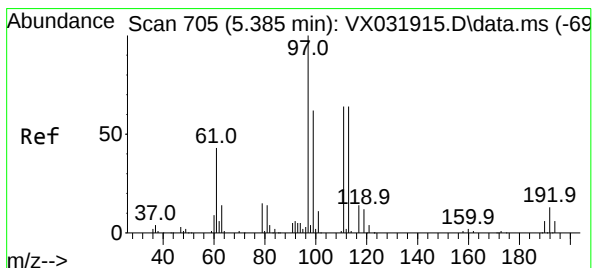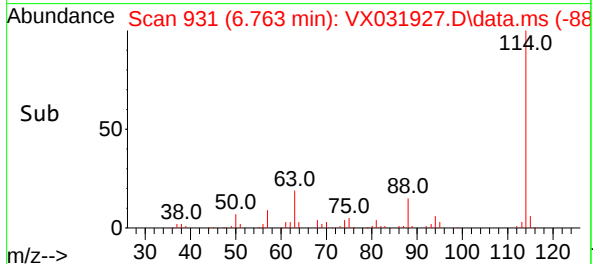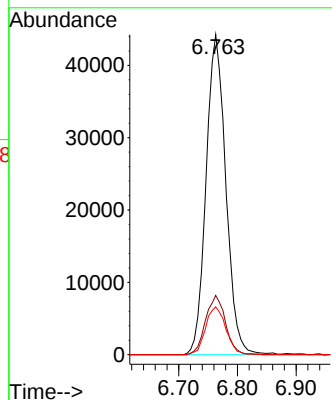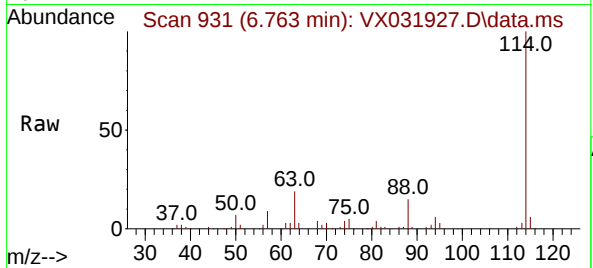

#35
Dibromofluoromethane
Concen: 48.747 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55

Tgt Ion:113 Resp: 57134
Ion Ratio Lower Upper
113 100
111 102.1 82.4 123.6
192 18.3 14.1 21.1


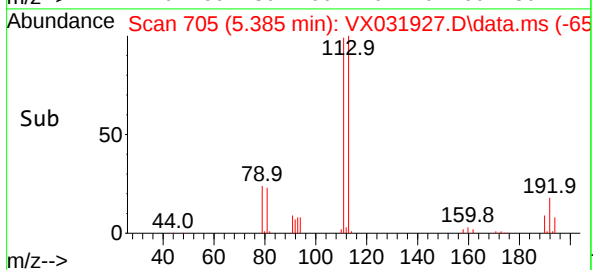
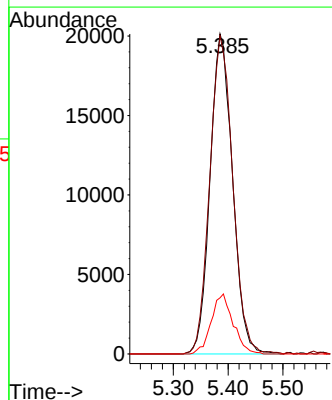
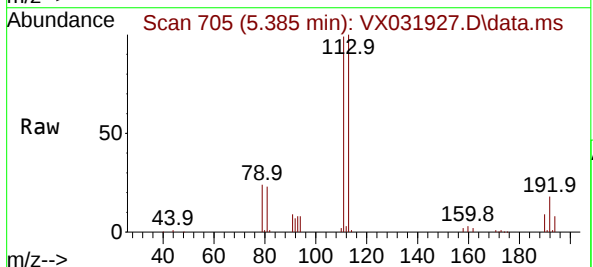


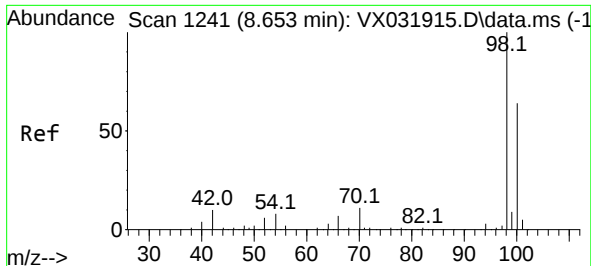

#50
Toluene-d8
Concen: 50.228 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55




Instrument :
MSVOA_X
ClientSampleId :
TB-01-100522


Tgt Ion: 98 Resp: 211835
Ion Ratio Lower Upper
98 100
100 66.2 52.5 78.7

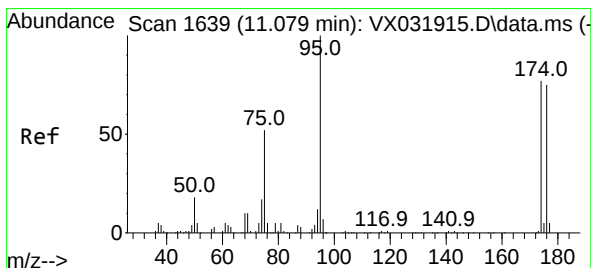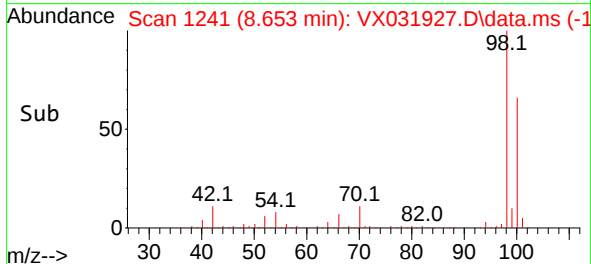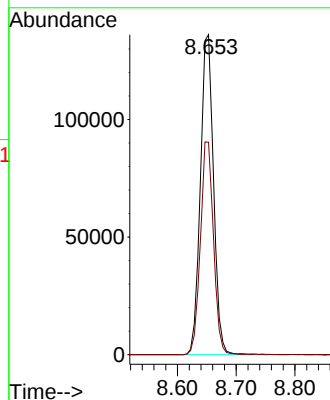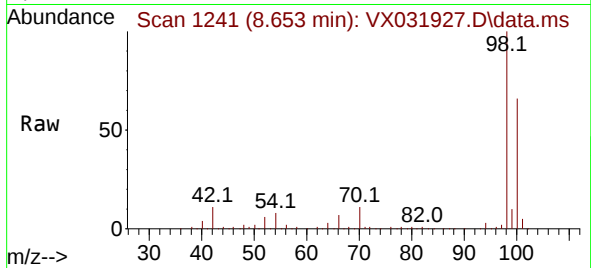

#62
4-Bromofluorobenzene
Concen: 48.496 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55

Tgt Ion: 95 Resp: 72307
Ion Ratio Lower Upper
95 100
174 79.4 0.0 153.2
176 75.9 0.0 144.0


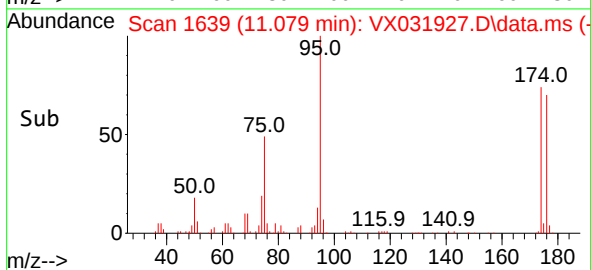
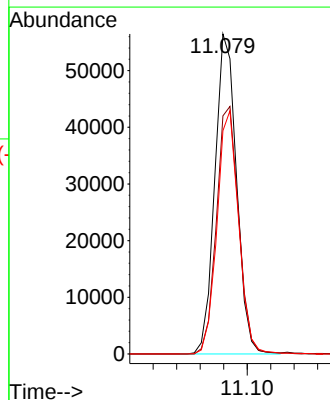
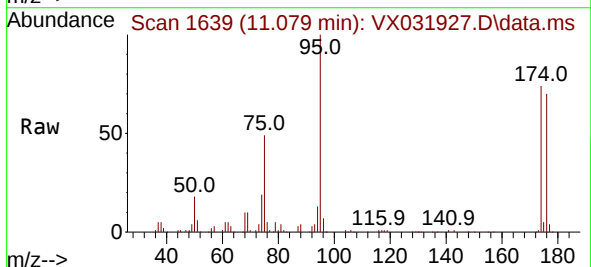


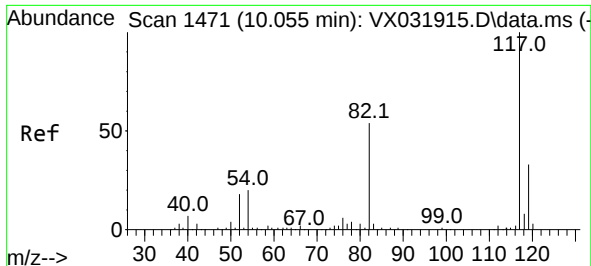

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55

Instrument :
MSVOA_X
ClientSampleId :
TB-01-100522

Tgt Ion:117 Resp: 110445
Ion Ratio Lower Upper
117 100
82 53.6 46.8 70.2
119 32.3 26.4 39.6

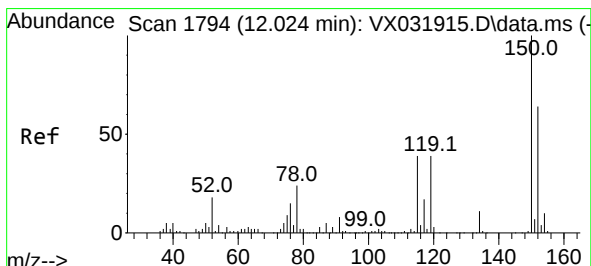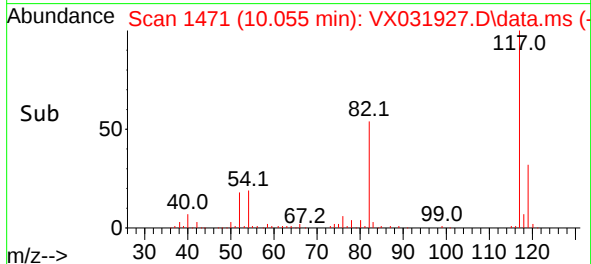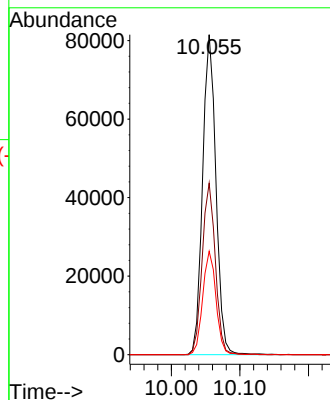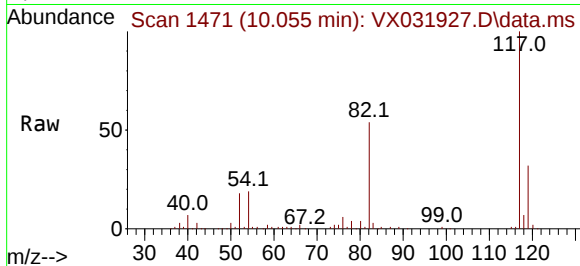

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031927.D
Acq: 06 Oct 2022 18:55

Tgt Ion:152 Resp: 68521
Ion Ratio Lower Upper
152 100
115 59.4 43.4 130.1
150 153.9 0.0 346.8

