

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
 Data File : VX031937.D
 Acq On : 06 Oct 2022 22:47
 Operator : JC/MD
 Sample : N4883-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-133

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX031937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.977	299	310	323	rBV	468051	1274258	21.82%	13.476%
2	3.111	323	332	350	rVB	2580537	5840677	100.00%	61.768%
3	5.385	693	705	719	rBV	60932	176244	3.02%	1.864%
4	5.550	721	732	747	rVB	60145	168552	2.89%	1.783%
5	5.958	789	799	812	rBV	68155	179100	3.07%	1.894%
6	6.324	852	859	870	rVB2	41999	120773	2.07%	1.277%
7	6.763	921	931	947	rBV	90360	214720	3.68%	2.271%
8	8.647	1234	1240	1256	rBV	323095	502734	8.61%	5.317%
9	10.055	1465	1471	1479	rBV	217372	295897	5.07%	3.129%
10	11.079	1634	1639	1648	rBV	237177	315786	5.41%	3.340%
11	12.024	1789	1794	1805	rVB	297612	367145	6.29%	3.883%




Sum of corrected areas: 9455886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031937.D
Acq On : 06 Oct 2022 22:47
Operator : JC/MD
Sample : N4883-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

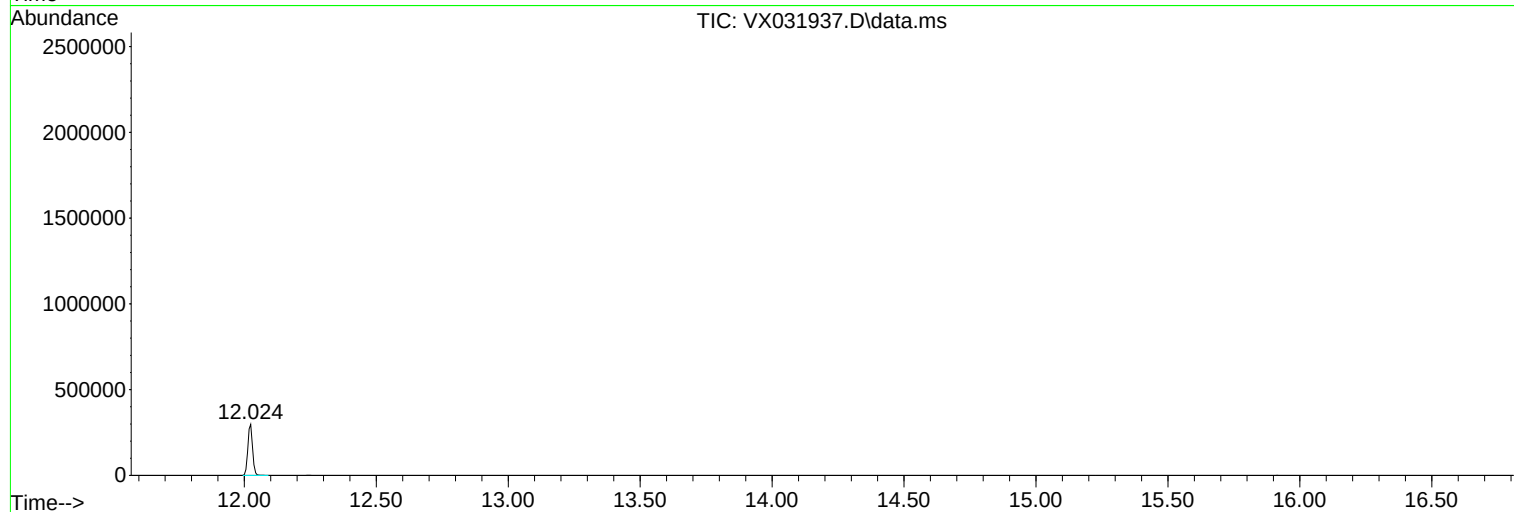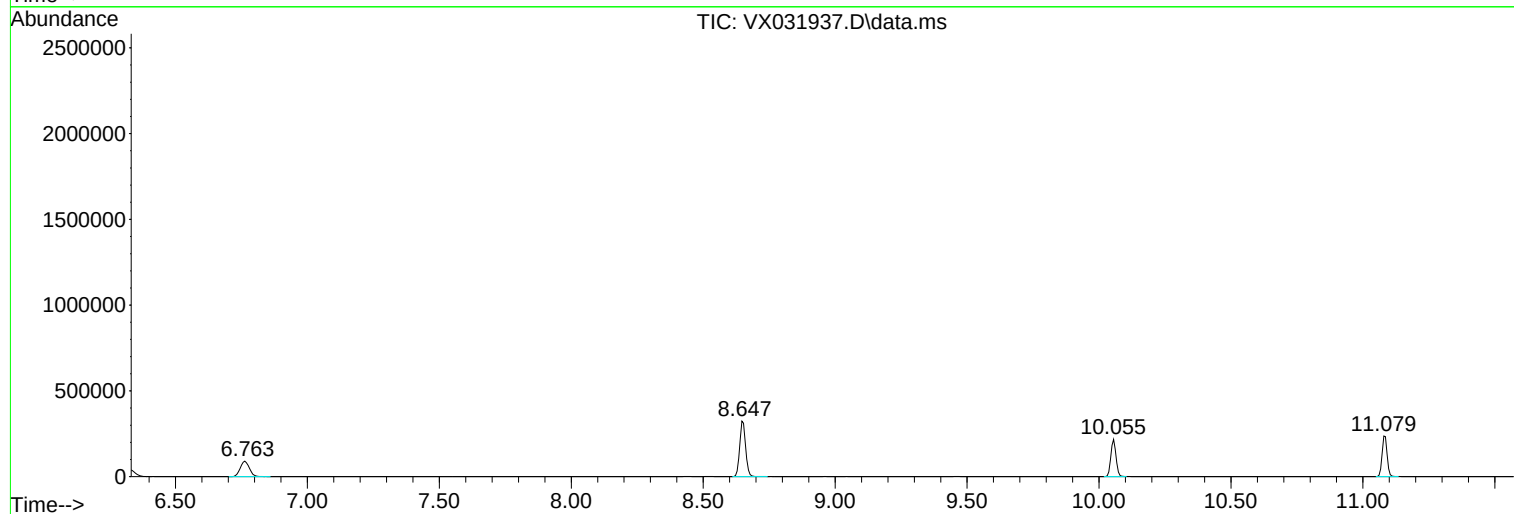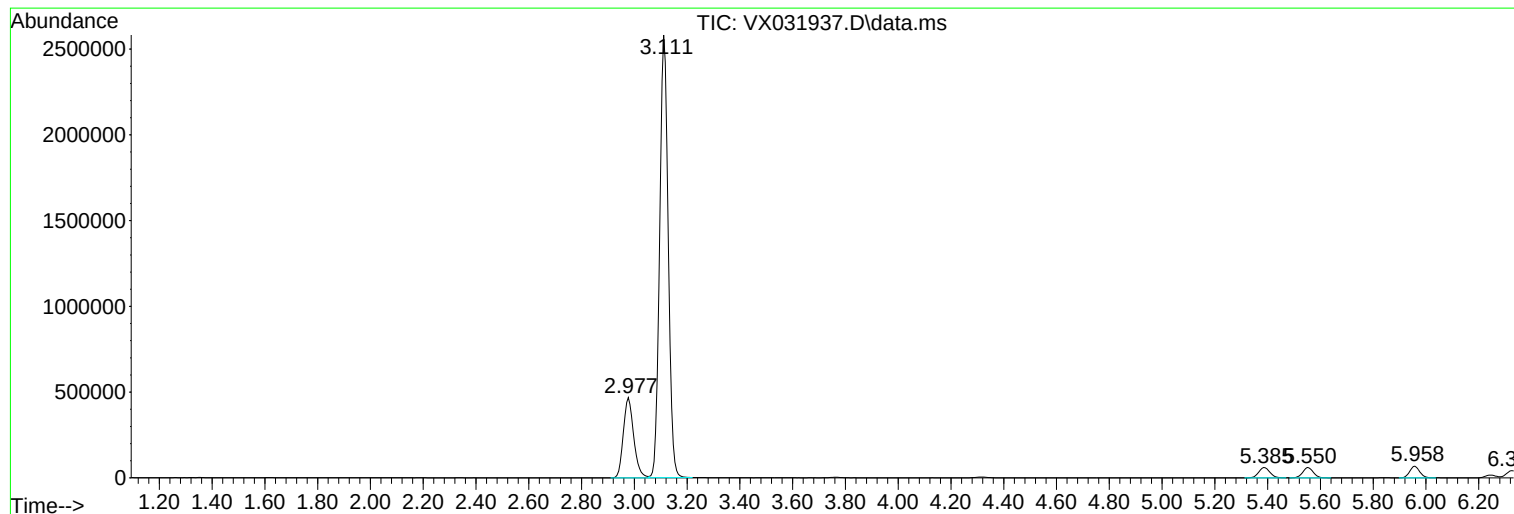

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031937.D
Acq On : 06 Oct 2022 22:47
Operator : JC/MD
Sample : N4883-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-133










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.324	28.12 ug/l	120773	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	74
2			1,4-Butanediamine	88	C4H12N2	000110-60-1	9
3			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
4			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	9
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	9

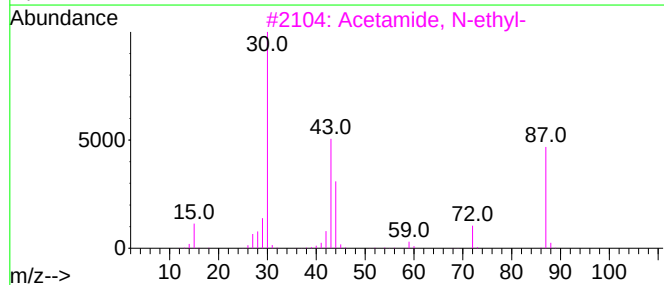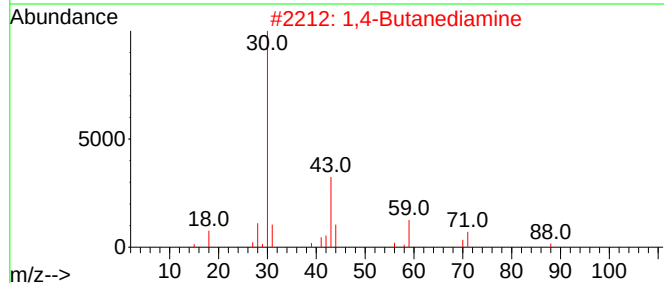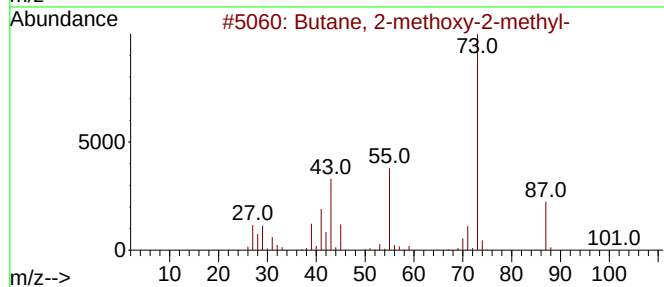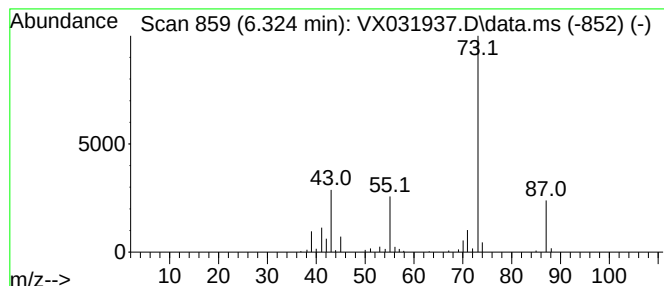

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031937.D
Acq On : 06 Oct 2022 22:47
Operator : JC/MD
Sample : N4883-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-133

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	6.324	28.1	ug/l	120773	2	6.763	214720	50.0