

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
 Data File : VX031938.D
 Acq On : 06 Oct 2022 23:11
 Operator : JC/MD
 Sample : N4883-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-134

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Title : SW846 8260

Signal : TIC: VX031938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.983	301	311	323	rBV	54880	167043	6.63%	3.395%
2	3.111	323	332	352	rVB	1116964	2520351	100.00%	51.225%
3	5.385	695	705	717	rBV	60632	172066	6.83%	3.497%
4	5.556	722	733	748	rVB2	56820	159998	6.35%	3.252%
5	5.958	788	799	812	rBV	66854	175010	6.94%	3.557%
6	6.324	849	859	874	rVB2	23965	69344	2.75%	1.409%
7	6.763	921	931	946	rBV	86344	206431	8.19%	4.196%
8	8.653	1234	1241	1251	rBV	303305	489182	19.41%	9.942%
9	10.055	1465	1471	1483	rBV	218748	294085	11.67%	5.977%
10	11.079	1634	1639	1654	rVB	240455	307736	12.21%	6.255%
11	12.024	1788	1794	1804	rBV	287443	358869	14.24%	7.294%




Sum of corrected areas: 4920115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031938.D
Acq On : 06 Oct 2022 23:11
Operator : JC/MD
Sample : N4883-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-134

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

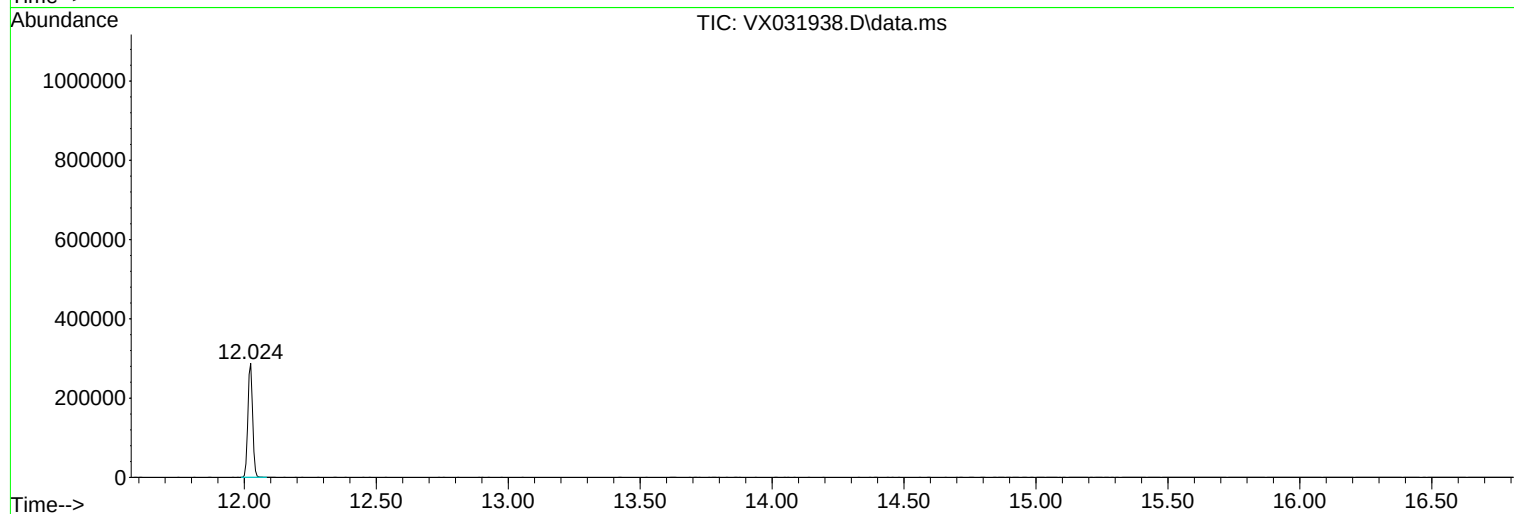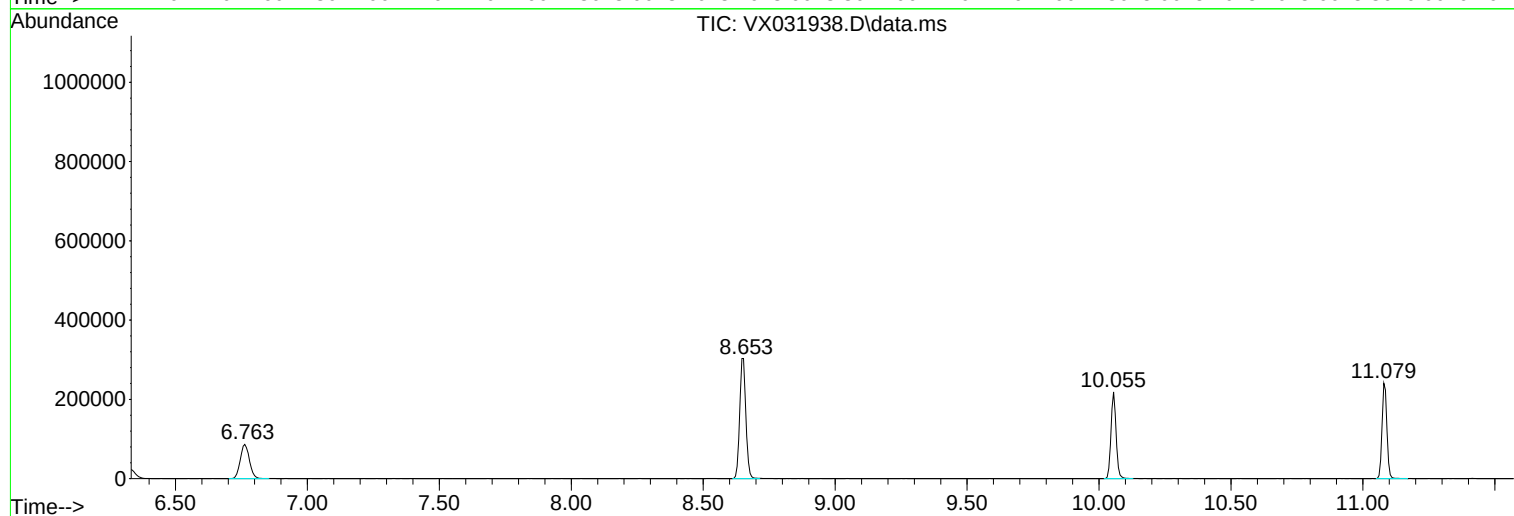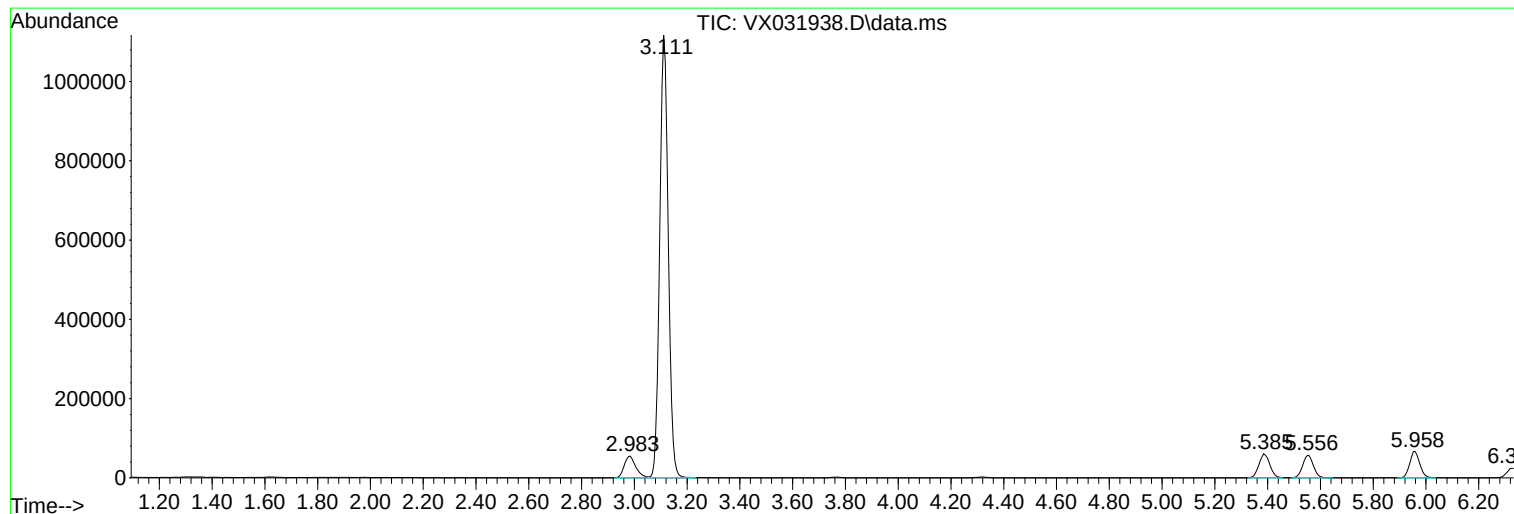

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031938.D
Acq On : 06 Oct 2022 23:11
Operator : JC/MD
Sample : N4883-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-134










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.324	16.80 ug/l	69344	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	56
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
3			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	17
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

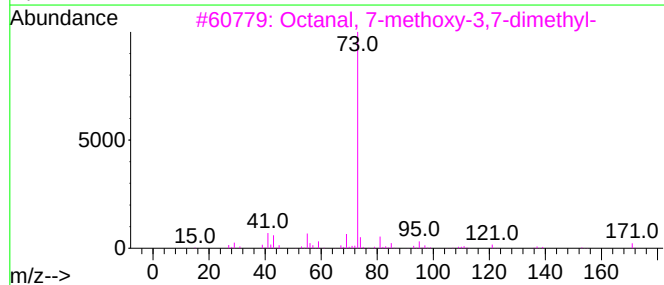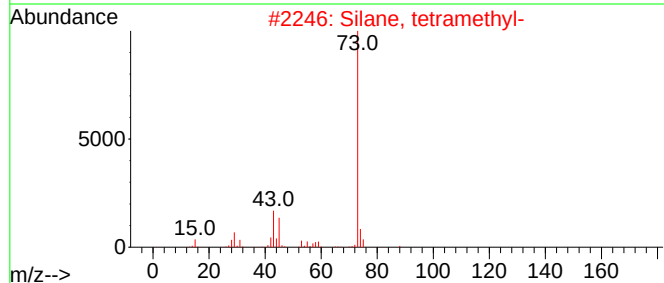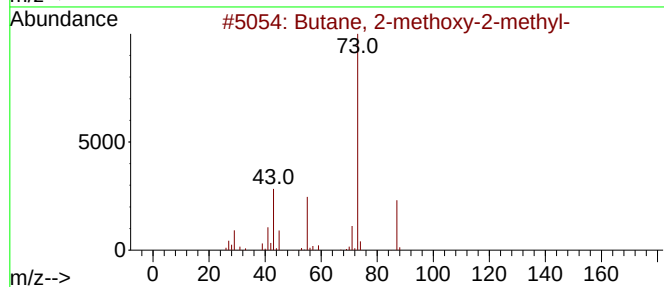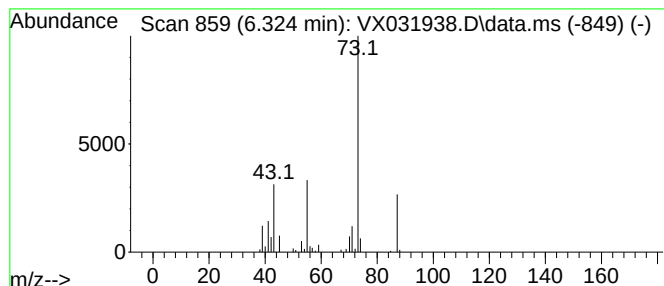

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100622\
Data File : VX031938.D
Acq On : 06 Oct 2022 23:11
Operator : JC/MD
Sample : N4883-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-134

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	6.324	16.8	ug/l	69344	2	6.763	206431	50.0