

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
 Data File : VX038124.D
 Acq On : 06 Oct 2023 12:38
 Operator : JC/MD
 Sample : 04723-03 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6A

Quant Time: Oct 07 04:18:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 05 15:27:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	106953	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	192921	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	189246	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	98355	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	77735	45.188	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	90.380%		
35) Dibromofluoromethane	5.391	113	59663	42.919	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	85.840%		
50) Toluene-d8	8.653	98	242326	45.619	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	91.240%#		
62) 4-Bromofluorobenzene	11.079	95	89788	44.586	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	89.180%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.611	94	106	Below Cal	#	3
6) Chloroethane	1.715	64	188	Below Cal	#	43
11) Tert butyl alcohol	2.953	59	699	Below Cal	#	78
13) Acrolein	2.215	56	1069	4.371	ug/l #	1
14) Allyl chloride	2.745	41	1645	0.940	ug/l #	1
16) Acetone	2.379	43	835	1.163	ug/l	90
20) Methylene Chloride	2.788	84	689	0.510	ug/l #	76
26) 2,2-Dichloropropane	4.562	77	596	0.343	ug/l #	54
31) Cyclohexane	5.483	56	2416	1.296	ug/l #	89
36) 1,1-Dichloropropene	5.556	75	9341	4.873	ug/l #	51
38) Carbon Tetrachloride	5.550	117	11104	5.888	ug/l #	17
39) Methylcyclohexane	7.372	83	1064	0.474	ug/l #	80
40) Benzene	6.043	78	87935	16.401	ug/l	99
51) 4-Methyl-2-Pentanone	8.653	43	1144	0.488	ug/l #	1
52) Toluene	8.720	92	303995	87.040	ug/l	93
53) t-1,3-Dichloropropene	8.720	75	3813	1.855	ug/l #	1
55) 1,1,2-Trichloroethane	9.019	97	893	0.598	ug/l #	17
67) Ethyl Benzene	10.195	91	61402	8.687	ug/l	98
68) m/p-Xylenes	10.299	106	57983	21.214	ug/l	98
69) o-Xylene	10.640	106	17847	6.690	ug/l	97
70) Styrene	10.646	104	1127	0.259	ug/l #	1
73) Isopropylbenzene	10.963	105	1644	0.249	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	50268	22.481	ug/l #	39
78) n-propylbenzene	11.305	91	5356	0.664	ug/l	99
79) 2-Chlorotoluene	11.384	91	3016	0.631	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	5386	0.946	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	50268	64.382	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.750	105	26921	4.745	ug/l	98
85) sec-Butylbenzene	11.750	105	26921	3.738	ug/l #	57
95) Naphthalene	13.780	128	13562	1.868	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038124.D
Acq On : 06 Oct 2023 12:38
Operator : JC/MD
Sample : 04723-03 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6A

Quant Time: Oct 07 04:18:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 05 15:27:13 2023
Response via : Initial Calibration




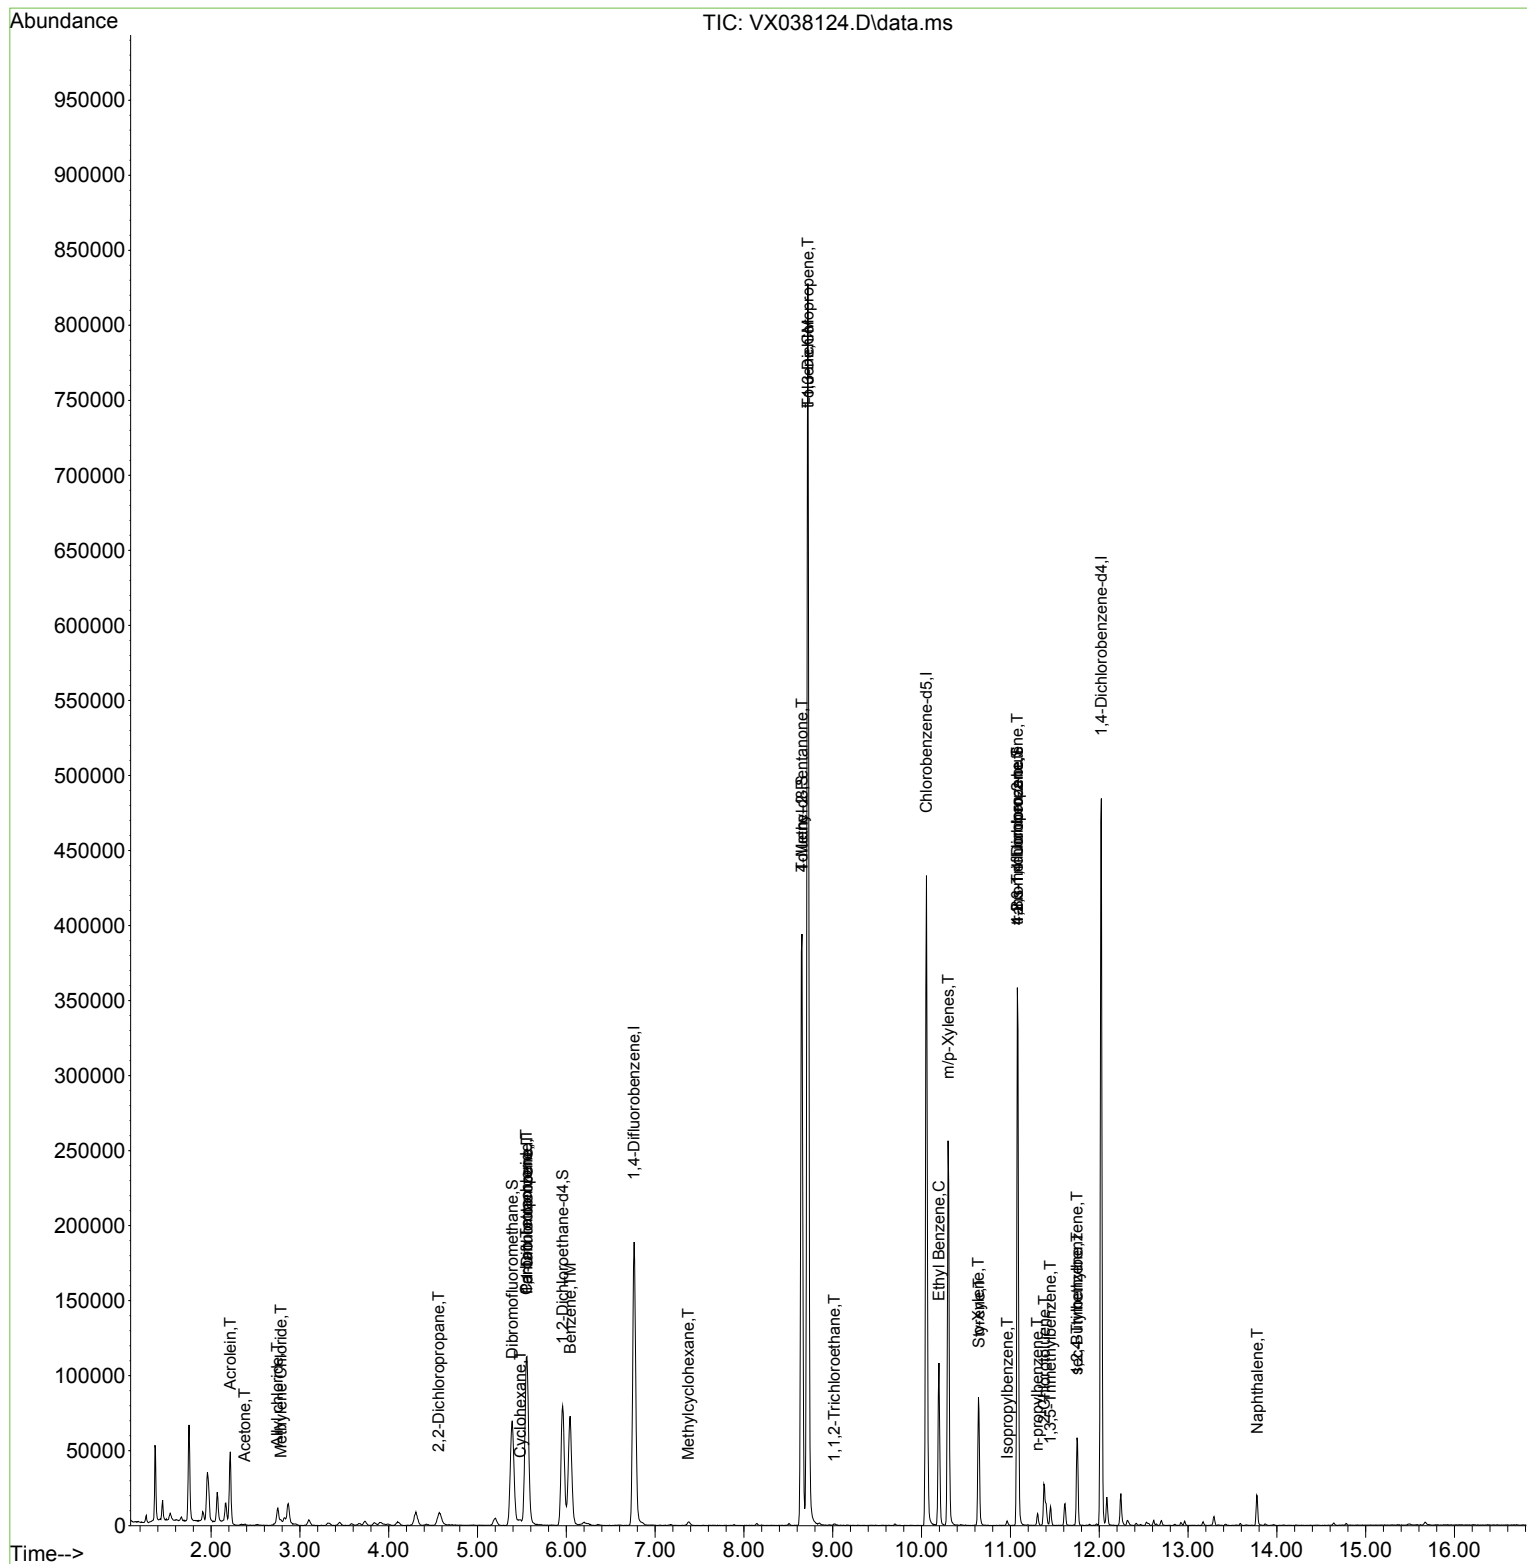




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion:168 Resp: 106953
Ion Ratio Lower Upper
168 100
99 59.2 56.6 85.0

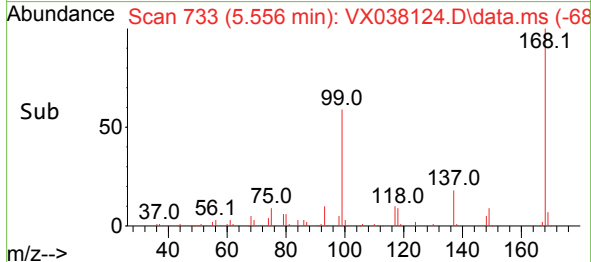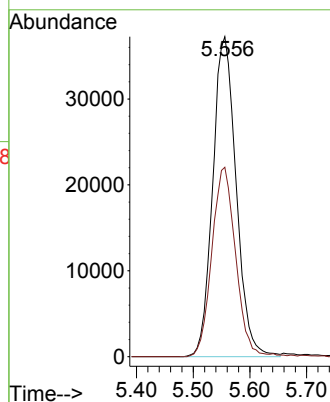

#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 94 Resp: 106
Ion Ratio Lower Upper
94 100
96 0.0 74.6 111.8#

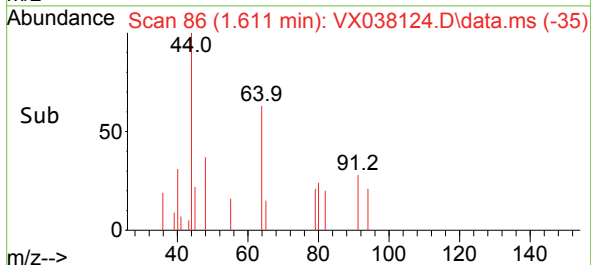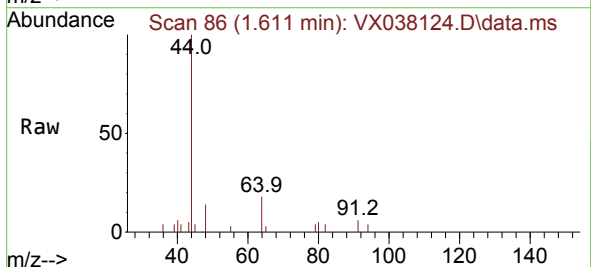

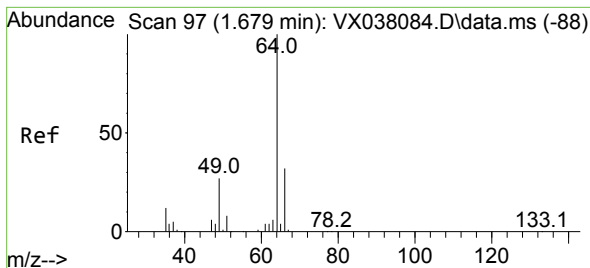

#6

Chloroethane

Concen: Below Cal

RT: 1.715 min Scan# 103

Delta R.T. 0.036 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion: 64 Resp: 188

Ion Ratio Lower Upper

64 100

66 0.0 25.1 37.7#

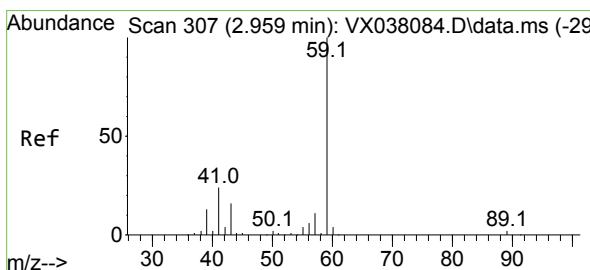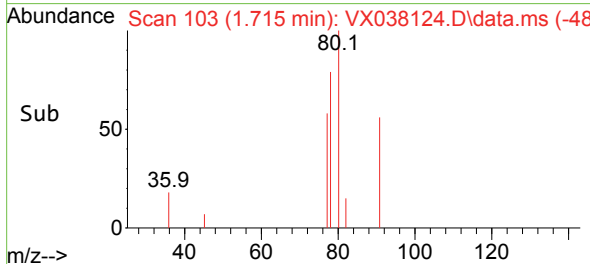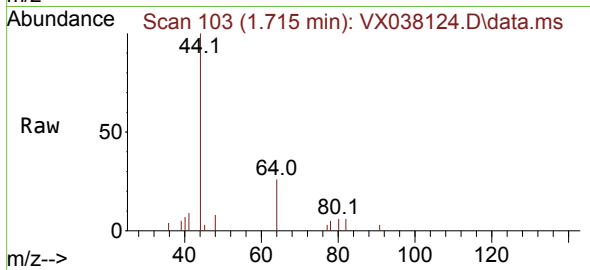

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.953 min Scan# 306

Delta R.T. -0.006 min

Lab File: VX038124.D




Acq: 06 Oct 2023 12:38


Tgt Ion: 59 Resp: 699

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

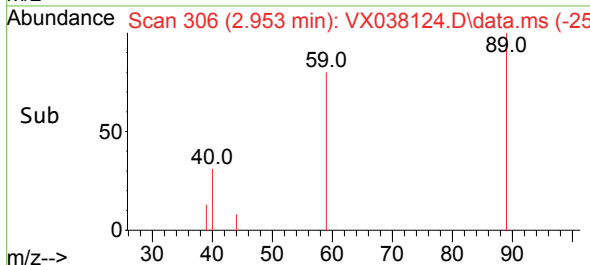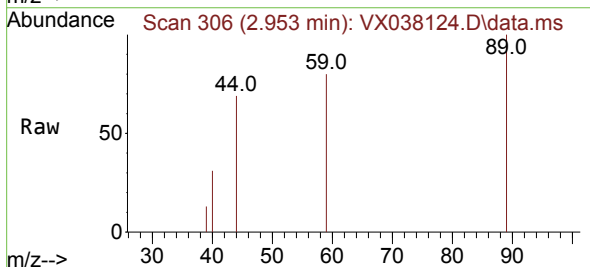



#13

Acrolein

Concen: 4.371 ug/l

RT: 2.215 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion: 56 Resp: 1069

Ion Ratio Lower Upper

56 100

55 2034.5 57.1 85.7#

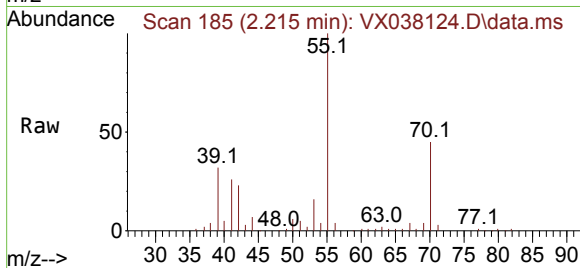

#14

Allyl chloride

Concen: 0.940 ug/l

RT: 2.745 min Scan# 272

Delta R.T. 0.085 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38




Tgt Ion: 41 Resp: 1645


Ion Ratio Lower Upper

41 100

39 174.5 55.8 83.6#

76 0.0 24.3 36.5#

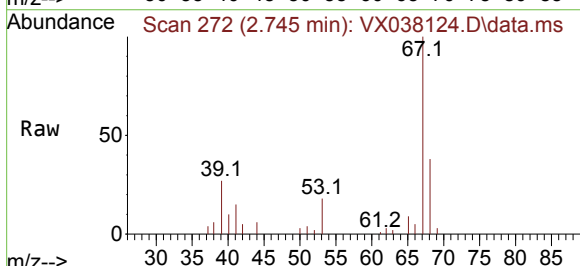



#16

Acetone

Concen: 1.163 ug/l

RT: 2.379 min Scan# 212

Delta R.T. -0.001 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion: 43 Resp: 835

Ion Ratio Lower Upper

43 100

58 22.3 21.9 32.9

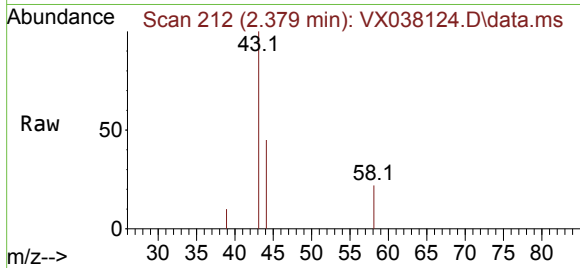

#20

Methylene Chloride

Concen: 0.510 ug/l

RT: 2.788 min Scan# 279

Delta R.T. -0.000 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Tgt Ion: 84 Resp: 689




Ion Ratio Lower Upper


84 100

49 166.6 103.6 155.4#

51 64.4 33.8 50.6#

86 61.9 49.4 74.0


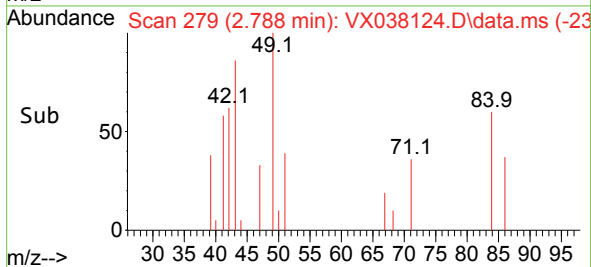
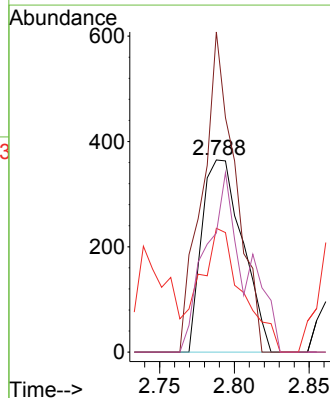
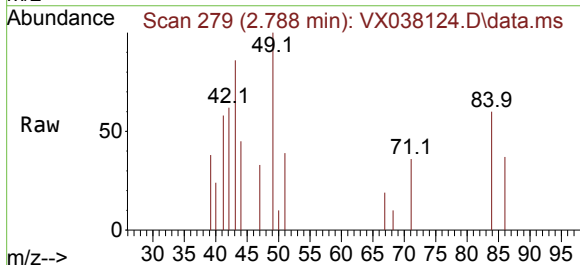




#26
2,2-Dichloropropane
Concen: 0.343 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.085 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 77 Resp: 596
Ion Ratio Lower Upper
77 100
97 0.0 10.8 32.3#



#31
Cyclohexane
Concen: 1.296 ug/l
RT: 5.483 min Scan# 721
Delta R.T. 0.012 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 56 Resp: 2416
Ion Ratio Lower Upper
56 100
69 22.5 23.4 35.2#
84 73.3 65.9 98.9




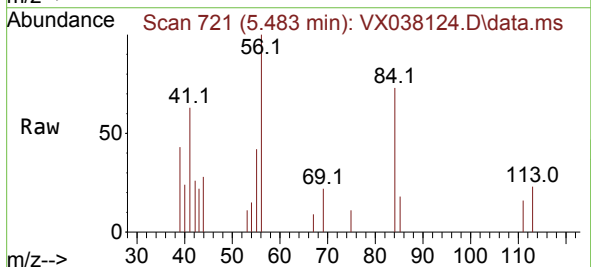




#33
1,2-Dichloroethane-d4
Concen: 45.188 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 65 Resp: 77735
Ion Ratio Lower Upper
65 100
67 52.2 0.0 100.2



#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 114 Resp: 192921
Ion Ratio Lower Upper
114 100
63 19.7 0.0 45.0
88 14.7 0.0 36.6




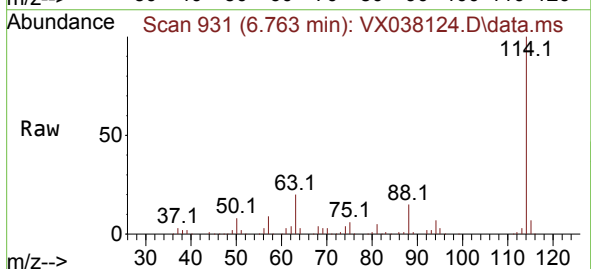


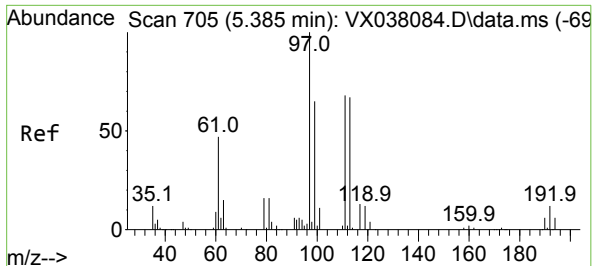

#35
Dibromofluoromethane
Concen: 42.919 ug/l
RT: 5.391 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion:113 Resp: 59663
Ion Ratio Lower Upper
113 100
111 102.1 82.9 124.3
192 18.1 13.3 19.9

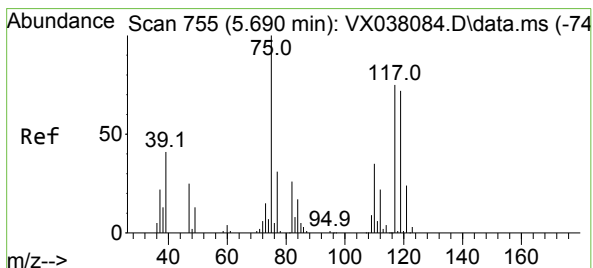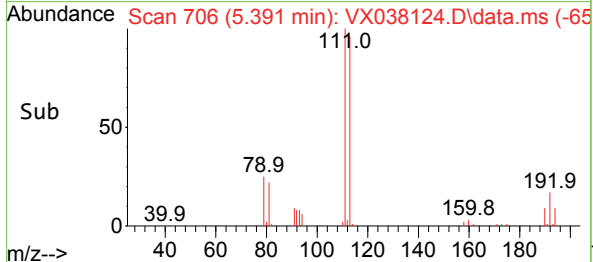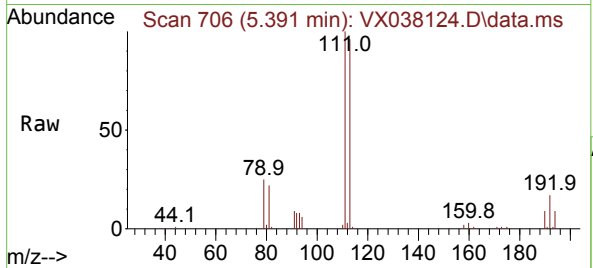

#36
1,1-Dichloropropene
Concen: 4.873 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38


Tgt Ion: 75 Resp: 9341
Ion Ratio Lower Upper
75 100
110 10.0 17.0 50.9#
77 0.0 24.7 37.1#

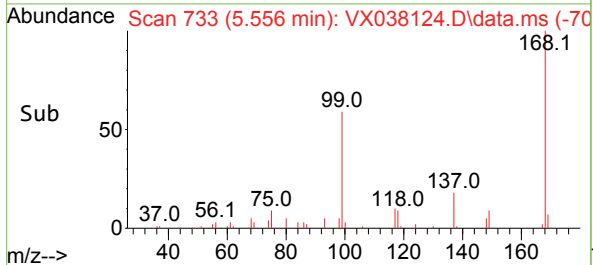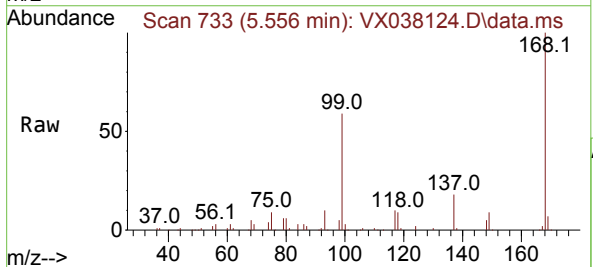






#38
Carbon Tetrachloride
Concen: 5.888 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Instrument :
MSVOA_X
ClientSampleId :
MW-6A







Tgt Ion:117 Resp: 11104
Ion Ratio Lower Upper
117 100
119 8.0 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 0.474 ug/l
RT: 7.372 min Scan# 1031
Delta R.T. -0.013 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 83 Resp: 1064
Ion Ratio Lower Upper
83 100
55 89.7 64.6 97.0
98 20.9 36.7 55.1#




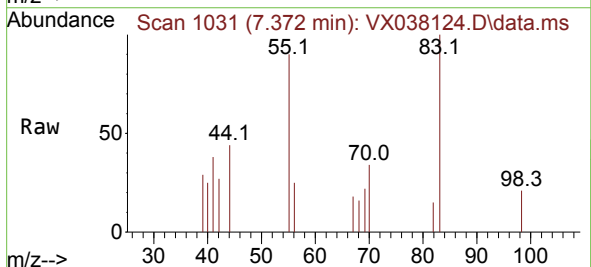




#40
Benzene
Concen: 16.401 ug/l
RT: 6.043 min Scan# 812
Delta R.T. 0.005 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 78 Resp: 87935
Ion Ratio Lower Upper
78 100
77 23.4 19.3 28.9



#50
Toluene-d8
Concen: 45.619 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 98 Resp: 242326
Ion Ratio Lower Upper
98 100
100 63.2 53.1 79.7

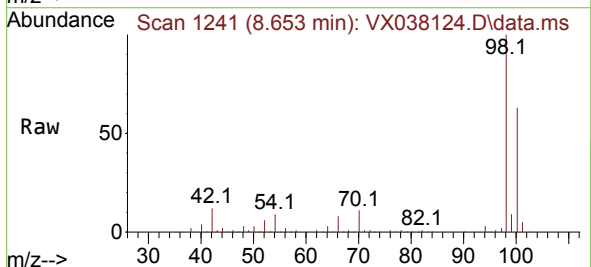



#51

4-Methyl-2-Pentanone

Concen: 0.488 ug/l

RT: 8.653 min Scan# 11

Delta R.T. 0.079 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion: 43 Resp: 1144

Ion Ratio Lower Upper

43 100

58 173.5 30.4 45.6#



#52

Toluene

Concen: 87.040 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX038124.D




Acq: 06 Oct 2023 12:38


Tgt Ion: 92 Resp: 303995

Ion Ratio Lower Upper

92 100

91 177.4 134.2 201.2









#53
t-1,3-Dichloropropene
Concen: 1.855 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.256 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 75 Resp: 3813
Ion Ratio Lower Upper
75 100
77 139.2 25.7 38.5#

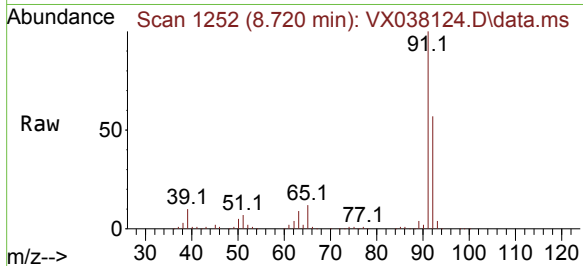

#55
1,1,2-Trichloroethane
Concen: 0.598 ug/l
RT: 9.019 min Scan# 1301
Delta R.T. -0.134 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 97 Resp: 893
Ion Ratio Lower Upper
97 100
83 0.0 65.8 98.8#
85 0.0 41.6 62.4#
99 0.0 47.8 71.8#



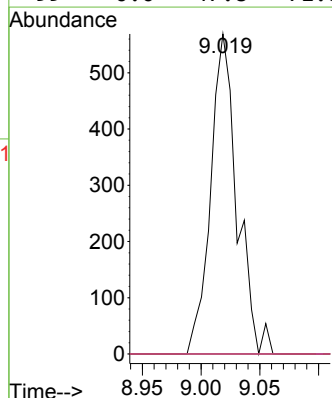
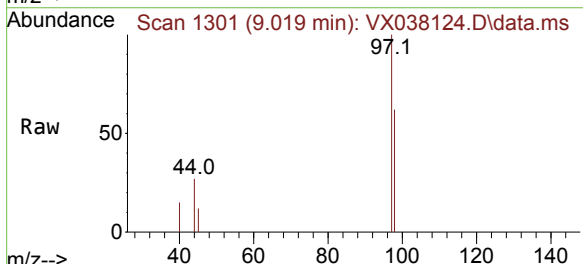




#62
4-Bromofluorobenzene
Concen: 44.586 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 95 Resp: 89788
Ion Ratio Lower Upper
95 100
174 80.8 0.0 135.6
176 77.6 0.0 131.0

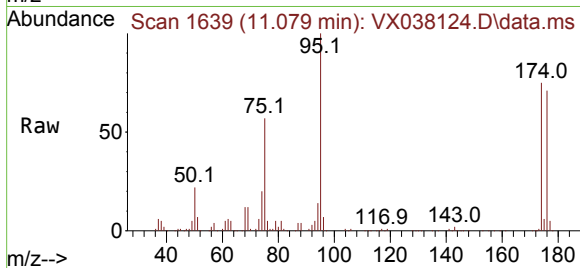

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 117 Resp: 189246
Ion Ratio Lower Upper
117 100
82 55.2 46.2 69.4
119 31.6 25.5 38.3

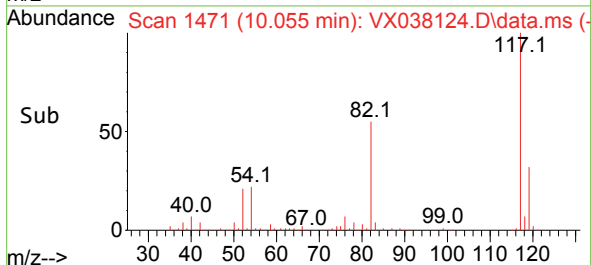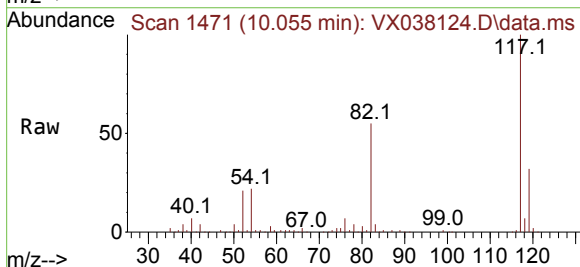



#67

Ethyl Benzene

Concen: 8.687 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion: 91 Resp: 61402

Ion Ratio Lower Upper

91 100

106 32.4 24.9 37.3



#68

m/p-Xylenes

Concen: 21.214 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.006 min

Lab File: VX038124.D




Acq: 06 Oct 2023 12:38


Tgt Ion: 106 Resp: 57983

Ion Ratio Lower Upper

106 100

91 209.6 165.5 248.3

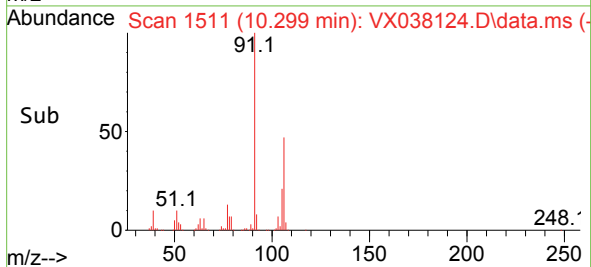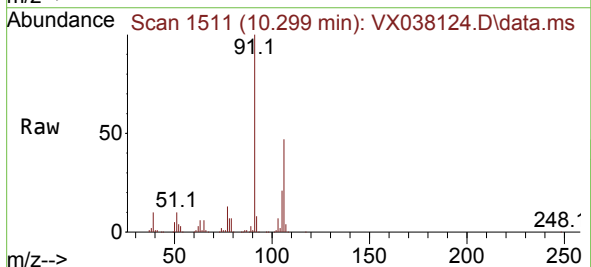



#69

o-Xylene

Concen: 6.690 ug/l

RT: 10.640 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion:106 Resp: 17847

Ion Ratio Lower Upper

106 100

91 223.3 108.9 326.8

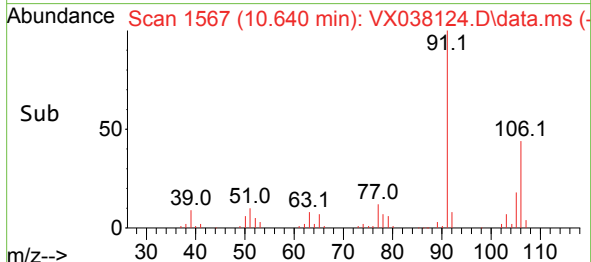

#70

Styrene

Concen: 0.259 ug/l

RT: 10.646 min Scan# 1568

Delta R.T. -0.013 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38




Tgt Ion:104 Resp: 1127


Ion Ratio Lower Upper

104 100

78 255.1 43.6 65.4#

103 256.2 43.6 65.4#


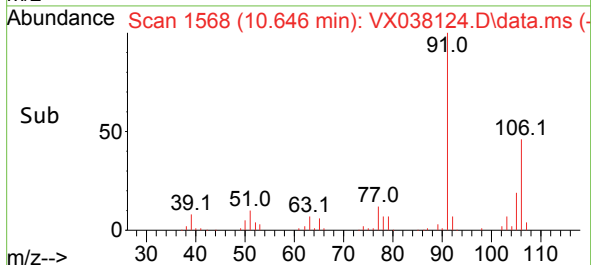

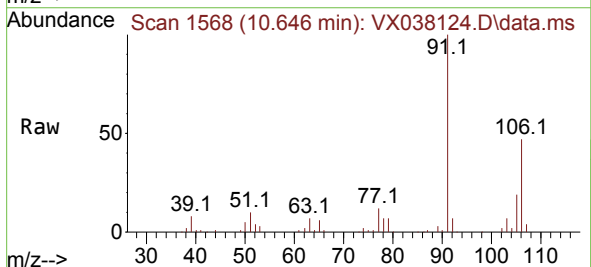




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX038124.D
 Acq: 06 Oct 2023 12:38




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6A


Tgt Ion:152 Resp: 98355
 Ion Ratio Lower Upper
 152 100
 115 60.7 43.3 129.9
 150 156.1 0.0 345.0

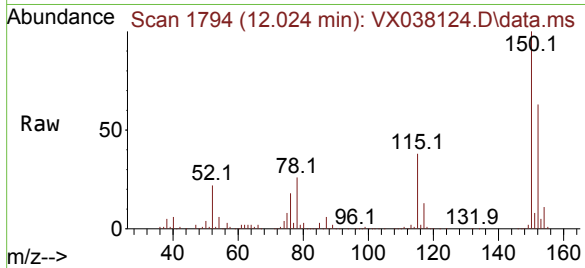

#73
 Isopropylbenzene
 Concen: 0.249 ug/l
 RT: 10.963 min Scan# 1620
 Delta R.T. 0.000 min
 Lab File: VX038124.D
 Acq: 06 Oct 2023 12:38

Tgt Ion:105 Resp: 1644
 Ion Ratio Lower Upper
 105 100
 120 26.2 12.9 38.6

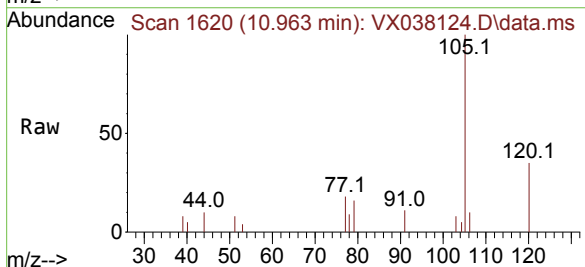



#76

1,2,3-Trichloropropane

Concen: 22.481 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX038124.D

Acq: 06 Oct 2023 12:38

Instrument :

MSVOA_X

ClientSampleId :





MW-6A

Tgt Ion: 75 Resp: 50268

Ion Ratio Lower Upper

75 100

77 1.1 19.1 57.5#



#78

n-propylbenzene

Concen: 0.664 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX038124.D




Acq: 06 Oct 2023 12:38


Tgt Ion: 91 Resp: 5356

Ion Ratio Lower Upper

91 100

120 22.2 11.5 34.4









#79
2-Chlorotoluene
Concen: 0.631 ug/l
RT: 11.384 min Scan# 1
Delta R.T. 0.018 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 91 Resp: 3016
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

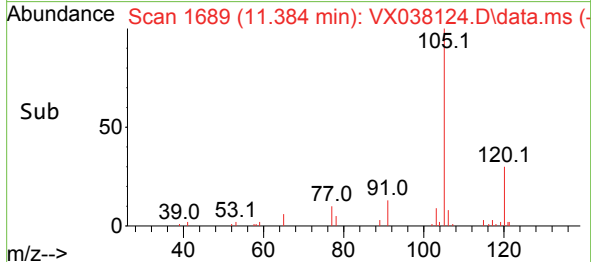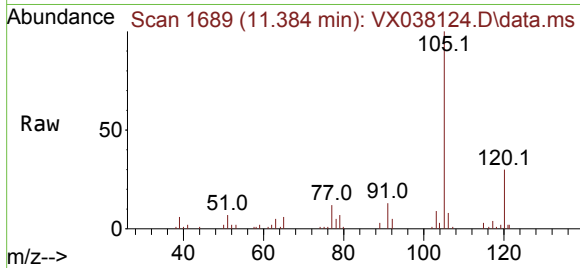

#80
1,3,5-Trimethylbenzene
Concen: 0.946 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 105 Resp: 5386
Ion Ratio Lower Upper
105 100
120 48.5 24.1 72.3


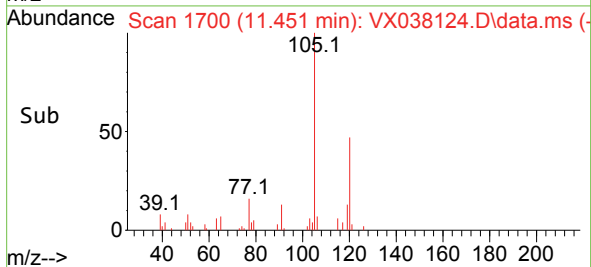

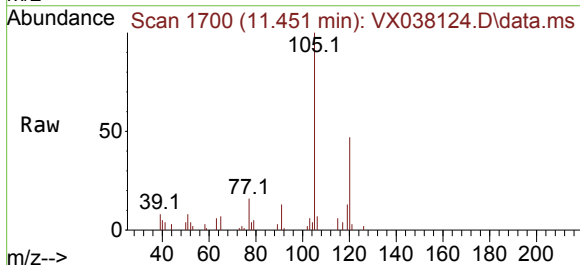




#81
trans-1,4-Dichloro-2-butene
Concen: 64.382 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38




Instrument :
MSVOA_X
ClientSampleId :
MW-6A


Tgt Ion: 75 Resp: 50268
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

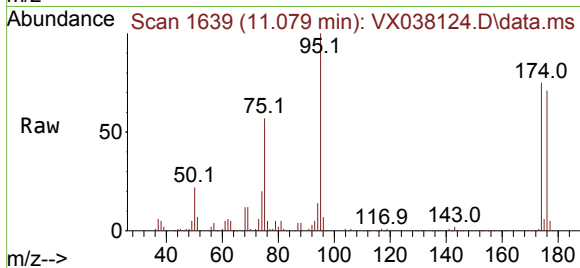

#84
1,2,4-Trimethylbenzene
Concen: 4.745 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX038124.D
Acq: 06 Oct 2023 12:38

Tgt Ion: 105 Resp: 26921
Ion Ratio Lower Upper
105 100
120 43.6 21.2 63.6




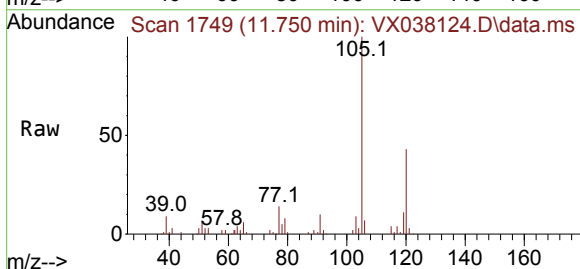




#85
 sec-Butylbenzene
 Concen: 3.738 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.140 min
 Lab File: VX038124.D
 Acq: 06 Oct 2023 12:38

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6A

Tgt Ion:105 Resp: 26921
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4#



#95
 Naphthalene
 Concen: 1.868 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.006 min
 Lab File: VX038124.D
 Acq: 06 Oct 2023 12:38

Tgt Ion:128 Resp: 13562
 Ion Ratio Lower Upper
 128 100
 127 12.0 10.3 15.5
 129 11.8 8.8 13.2

