

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038135.D
Acq On : 06 Oct 2023 16:54
Operator : JC/MD
Sample : 04794-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-C-20231005

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260

Signal : TIC: VX038135.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.337	197	205	209	rBV2	4551	8726	1.45%	0.263%
2	4.574	563	572	582	rBV3	1932	6755	1.12%	0.204%
3	5.391	693	706	722	rBV2	65899	195325	32.45%	5.896%
4	5.556	722	733	747	rBV	104663	302425	50.24%	9.129%
5	5.958	789	799	812	rBV	76563	206431	34.29%	6.232%
6	6.763	921	931	944	rBV	176374	422270	70.15%	12.747%
7	8.653	1234	1241	1257	rBV	365886	601943	100.00%	18.171%
8	10.055	1465	1471	1485	rBV	414543	560552	93.12%	16.921%
9	11.079	1634	1639	1649	rBV	326070	432366	71.83%	13.052%
10	12.024	1788	1794	1802	rBV	447540	575890	95.67%	17.384%




Sum of corrected areas: 3312683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038135.D
Acq On : 06 Oct 2023 16:54
Operator : JC/MD
Sample : 04794-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-C-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

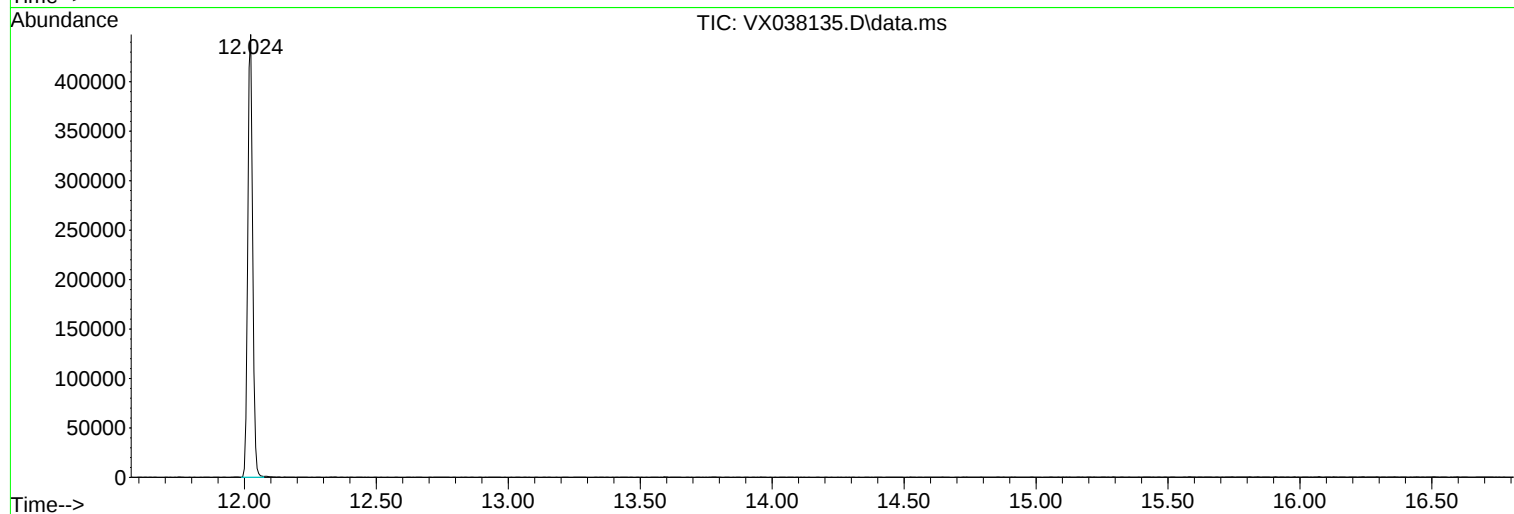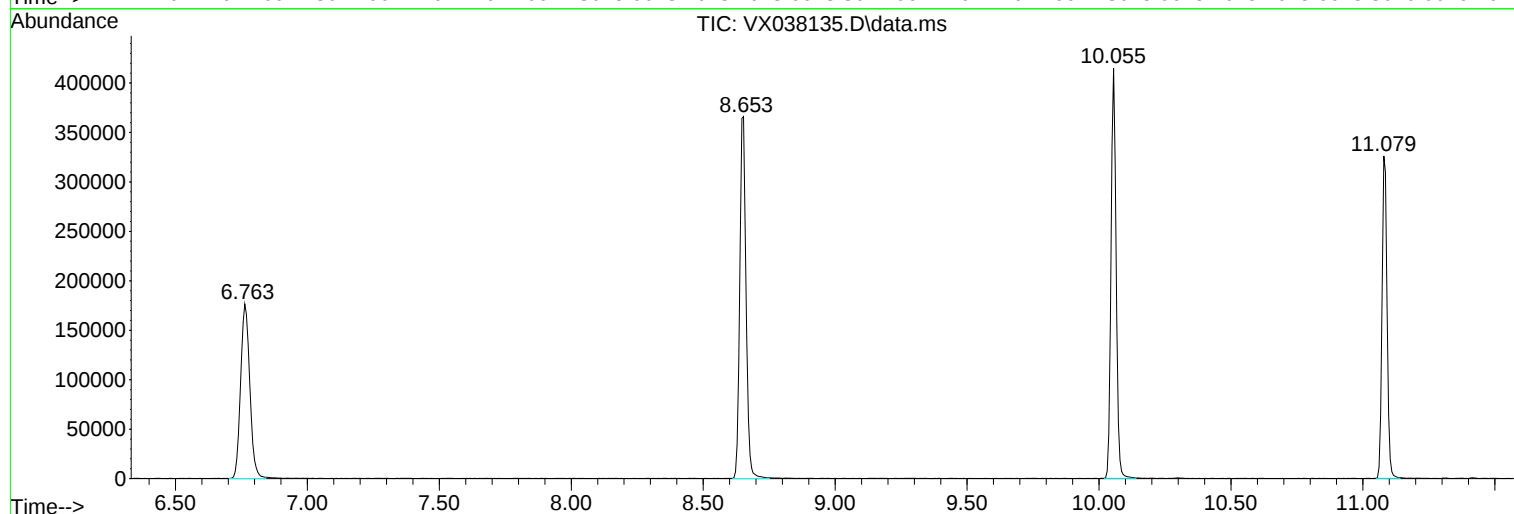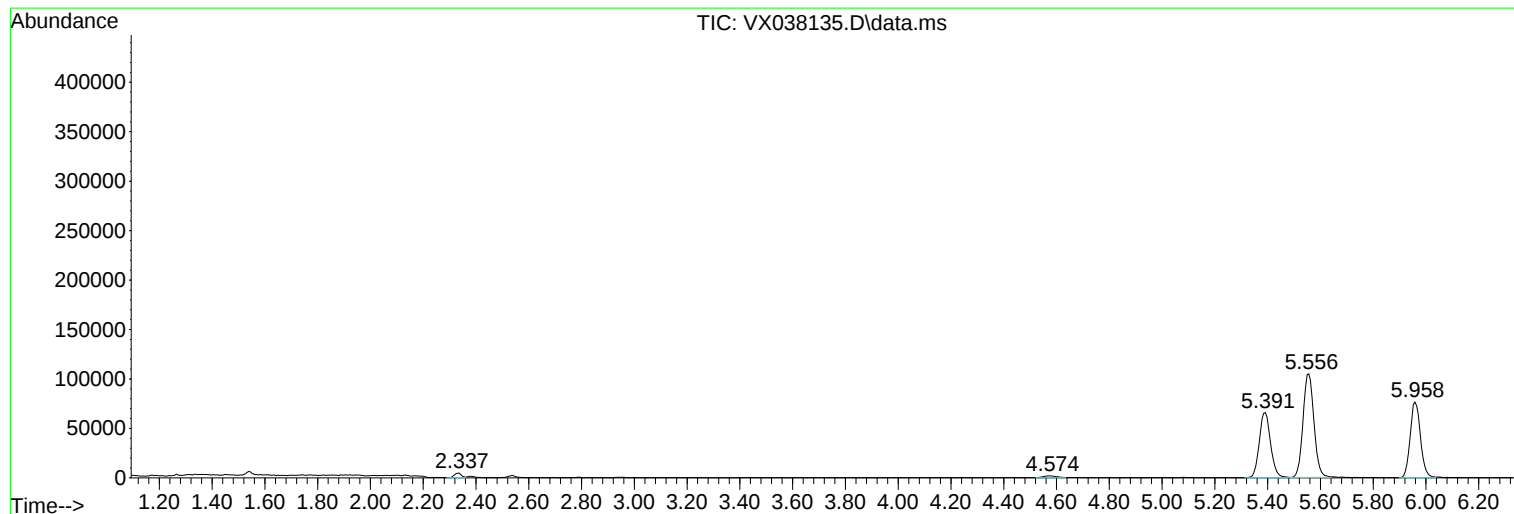

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038135.D
Acq On : 06 Oct 2023 16:54
Operator : JC/MD
Sample : 04794-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-C-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038135.D
Acq On : 06 Oct 2023 16:54
Operator : JC/MD
Sample : 04794-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-C-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------