

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038137.D
Acq On : 06 Oct 2023 17:41
Operator : JC/MD
Sample : 04794-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-A-20231005

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.538	69	74	78	rBV2	3816	6502	1.10%	0.197%
2	2.331	199	204	209	rBV2	5222	9403	1.59%	0.285%
3	2.538	231	238	245	rBV	4085	8048	1.36%	0.244%
4	4.574	561	572	582	rBV2	5059	16860	2.85%	0.511%
5	5.391	692	706	721	rBV	65080	191262	32.32%	5.791%
6	5.556	721	733	748	rBV	104941	294454	49.76%	8.916%
7	5.958	788	799	812	rBV2	73415	199623	33.73%	6.045%
8	6.763	920	931	946	rBV	173731	415122	70.15%	12.570%
9	8.647	1234	1240	1256	rBV	358851	585177	98.89%	17.719%
10	10.055	1465	1471	1489	rBV	404088	551509	93.20%	16.700%
11	11.079	1634	1639	1651	rBV	330772	432833	73.14%	13.106%
12	12.024	1788	1794	1810	rVB	446153	591754	100.00%	17.918%




Sum of corrected areas: 3302547

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038137.D
Acq On : 06 Oct 2023 17:41
Operator : JC/MD
Sample : 04794-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-A-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

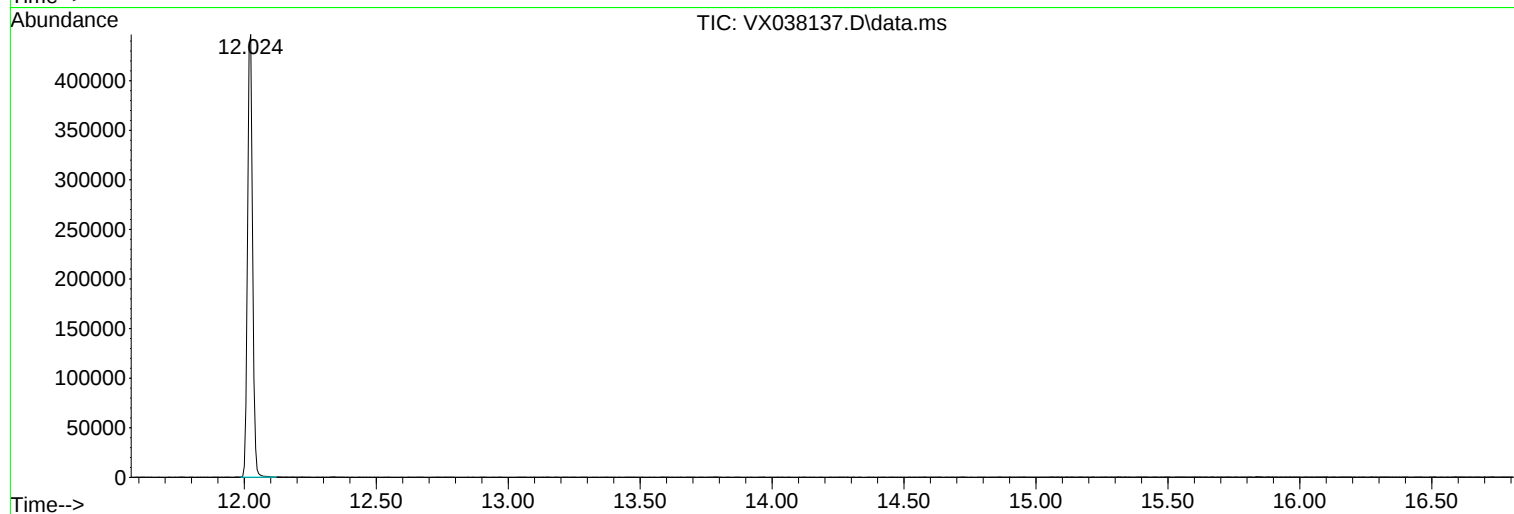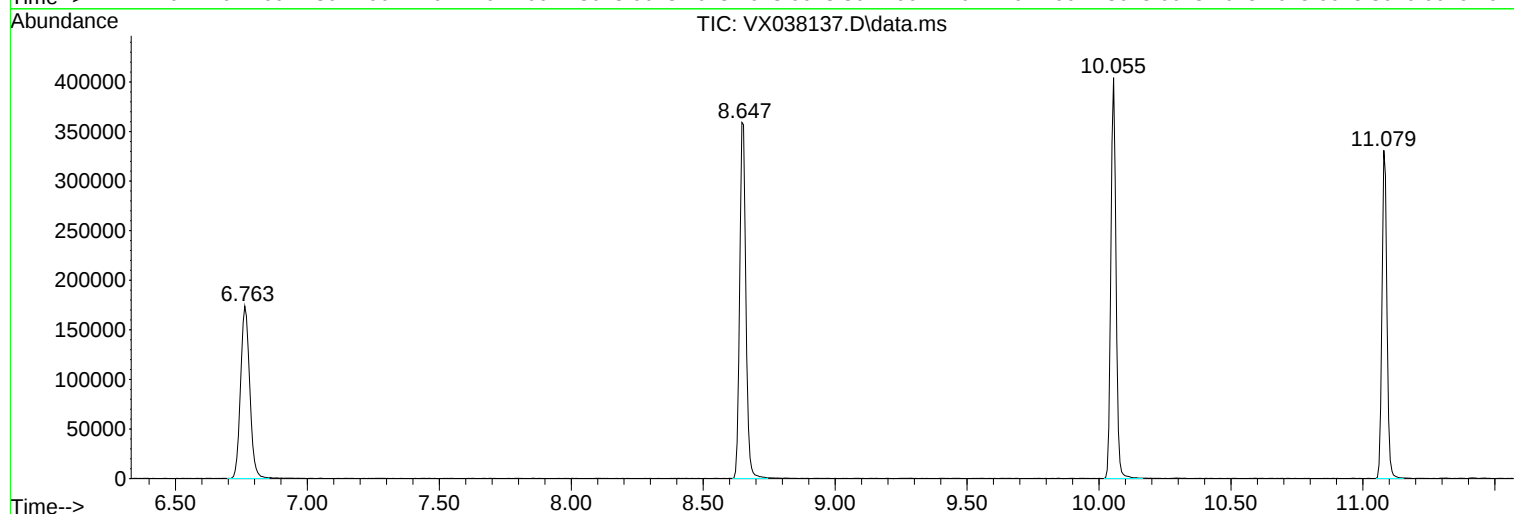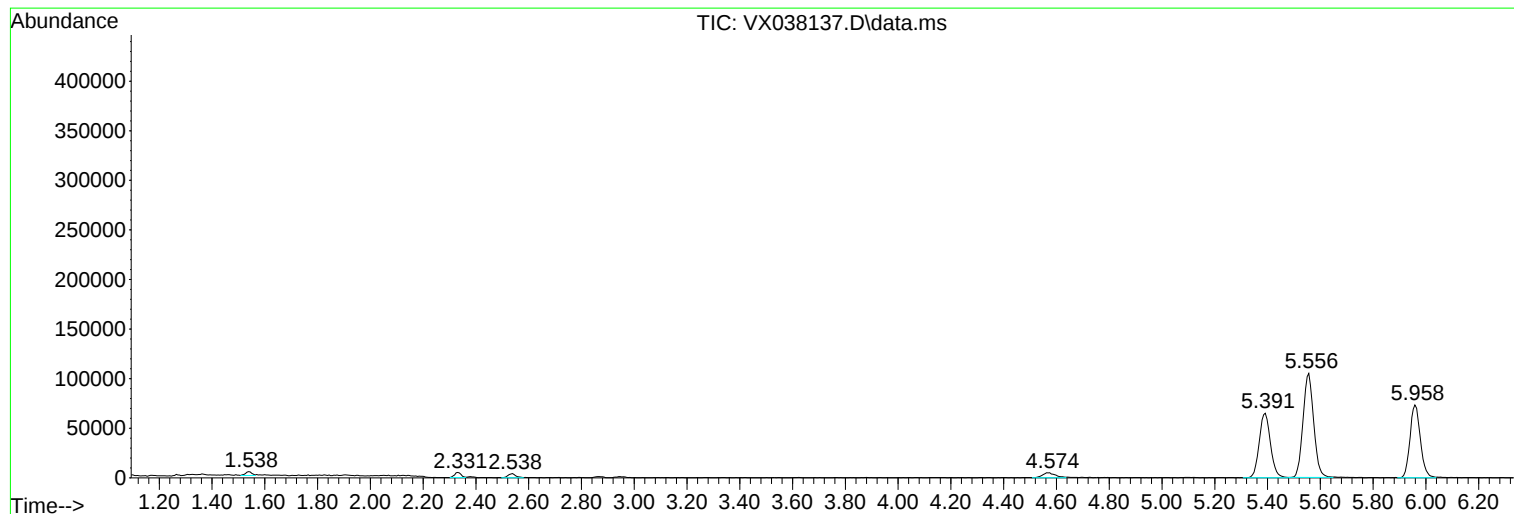

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038137.D
Acq On : 06 Oct 2023 17:41
Operator : JC/MD
Sample : 04794-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-A-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038137.D
Acq On : 06 Oct 2023 17:41
Operator : JC/MD
Sample : 04794-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-BASIN-A-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------