

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
 Data File : VX038138.D
 Acq On : 06 Oct 2023 18:04
 Operator : JC/MD
 Sample : 04794-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE137-SP-303-20231005

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M

Title : SW846 8260

Signal : TIC: VX038138.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.538	69	74	81	rVB2	3980	6977	1.24%	0.219%
2	2.331	198	204	211	rBV2	8745	16532	2.93%	0.519%
3	2.532	230	237	247	rBV	5143	10850	1.92%	0.340%
4	4.574	559	572	583	rBV2	5523	19481	3.45%	0.611%
5	5.391	695	706	720	rBV	63060	182954	32.43%	5.741%
6	5.556	722	733	750	rVV	99677	286017	50.70%	8.976%
7	5.958	790	799	816	rBV	75172	193990	34.39%	6.088%
8	6.763	922	931	945	rBV2	163885	399264	70.77%	12.530%
9	8.653	1234	1241	1256	rBV	344912	564133	100.00%	17.703%
10	10.055	1465	1471	1485	rBV	397366	529354	93.83%	16.612%
11	11.079	1634	1639	1650	rBV	318448	413897	73.37%	12.989%
12	12.024	1788	1794	1803	rBV	429626	563121	99.82%	17.672%


Sum of corrected areas: 3186570

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038138.D
Acq On : 06 Oct 2023 18:04
Operator : JC/MD
Sample : 04794-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-SP-303-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

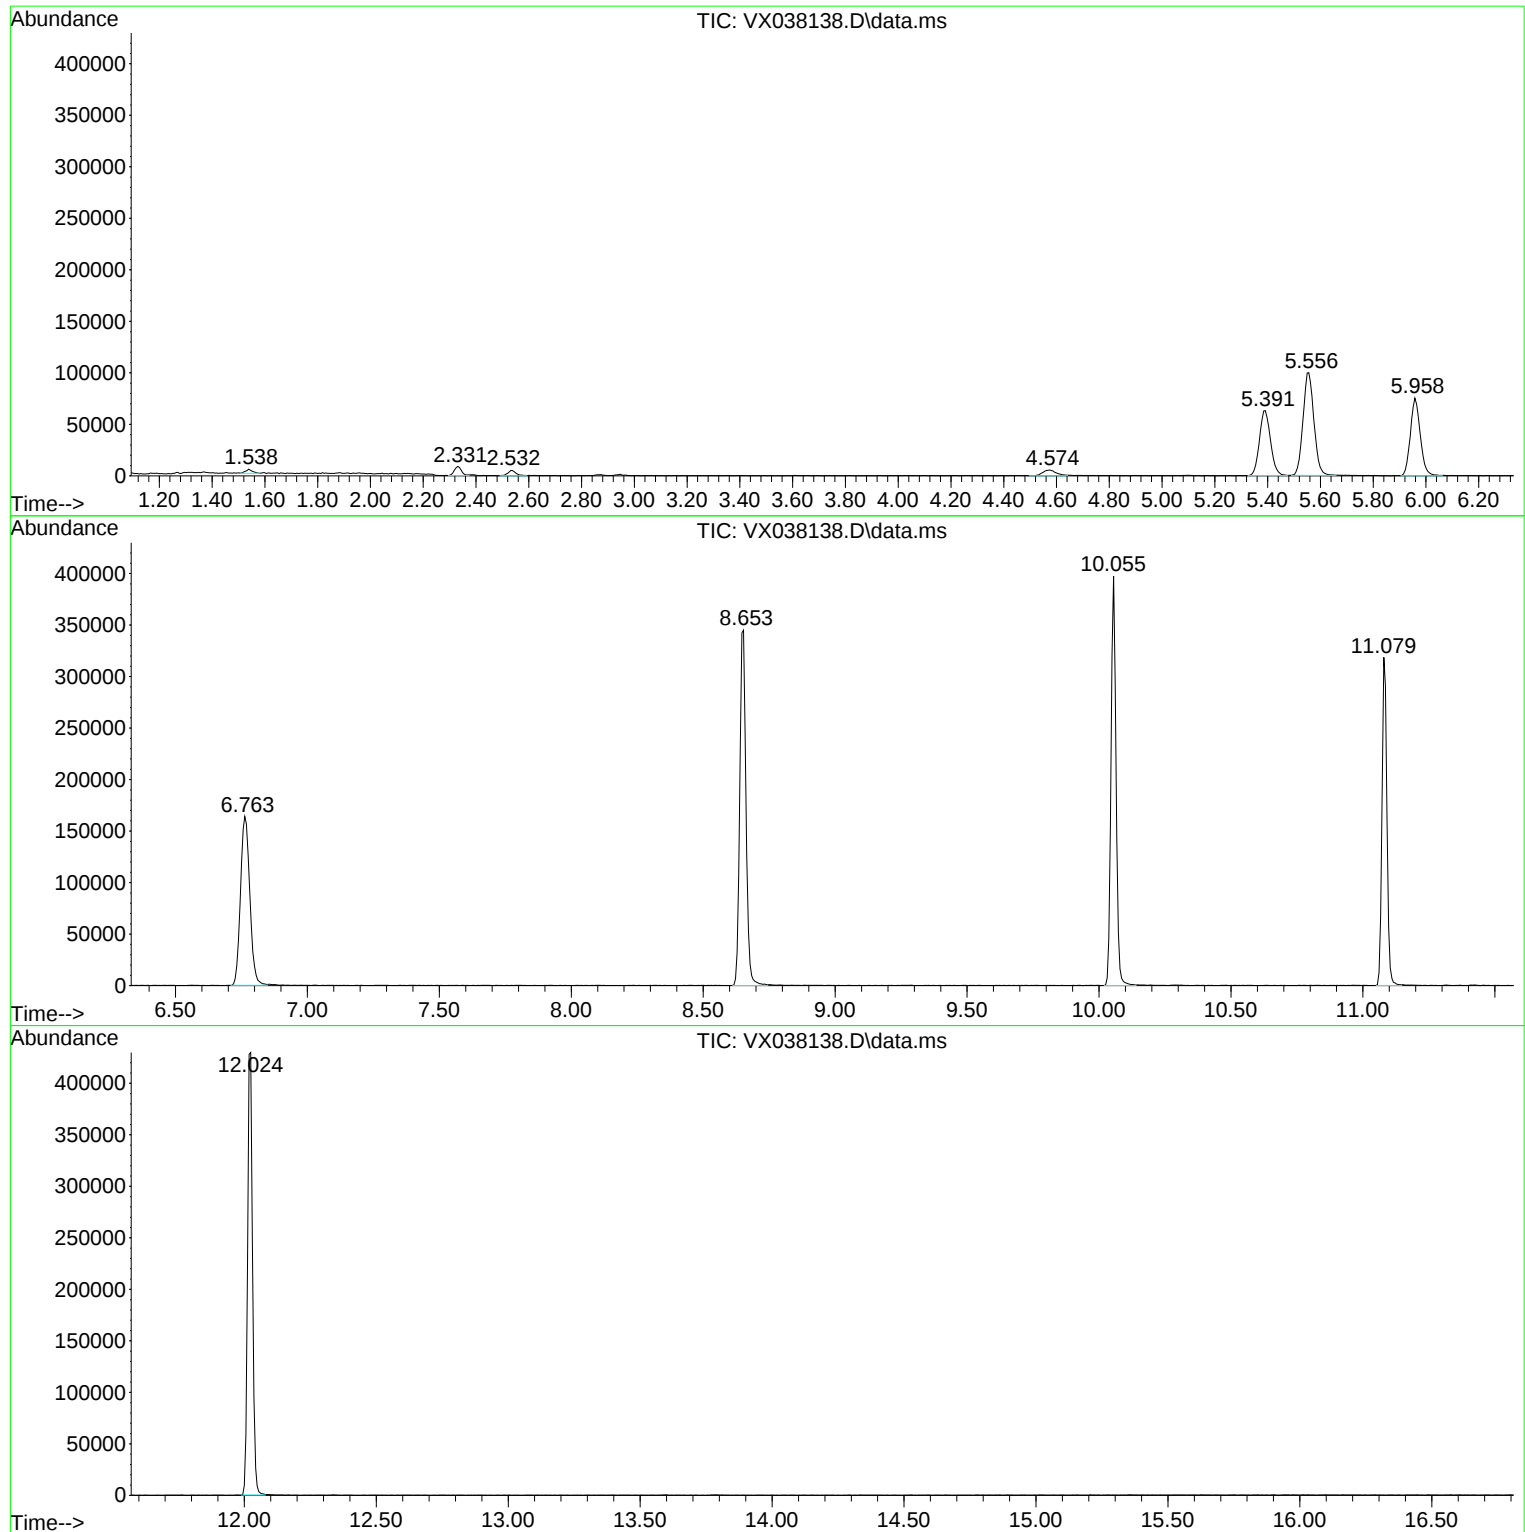

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038138.D
Acq On : 06 Oct 2023 18:04
Operator : JC/MD
Sample : 04794-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-SP-303-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038138.D
Acq On : 06 Oct 2023 18:04
Operator : JC/MD
Sample : 04794-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE137-SP-303-20231005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------