

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
 Data File : VX038154.D
 Acq On : 07 Oct 2023 03:19
 Operator : JC/MD
 Sample : 04783-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 231003027-03RE

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X100623W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX038154.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.544	70	75	84	rVB2	5130	8769	3.09%	0.698%
2	2.379	206	212	217	rBV	12080	19494	6.87%	1.551%
3	2.526	229	236	246	rBV4	2288	5271	1.86%	0.419%
4	4.903	616	626	638	rBV2	22738	67374	23.73%	5.361%
5	5.958	790	799	812	rBV	41838	115472	40.68%	9.188%
6	6.763	922	931	942	rBV	71041	173803	61.23%	13.829%
7	8.653	1234	1241	1249	rBV	161019	266286	93.80%	21.188%
8	8.720	1249	1252	1261	rVB2	3945	6870	2.42%	0.547%
9	10.055	1465	1471	1480	rBV	208514	283875	100.00%	22.588%
10	11.079	1634	1639	1648	rBV	213708	280803	98.92%	22.343%
11	12.024	1789	1794	1802	rVB4	3434	6631	2.34%	0.528%
12	13.383	2010	2017	2022	rBV4	1793	2979	1.05%	0.237%
13	13.585	2042	2050	2056	rBV4	3848	5937	2.09%	0.472%
14	14.590	2211	2215	2222	rBV2	10255	13205	4.65%	1.051%




Sum of corrected areas: 1256769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038154.D
Acq On : 07 Oct 2023 03:19
Operator : JC/MD
Sample : 04783-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
231003027-03RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X100623W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

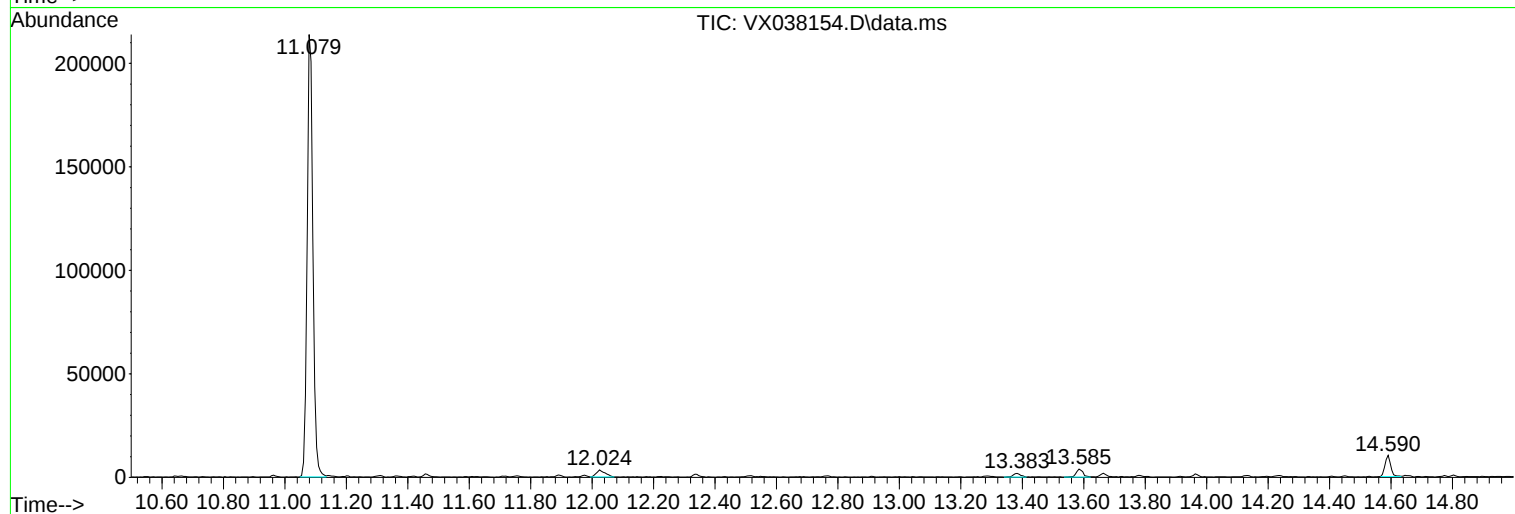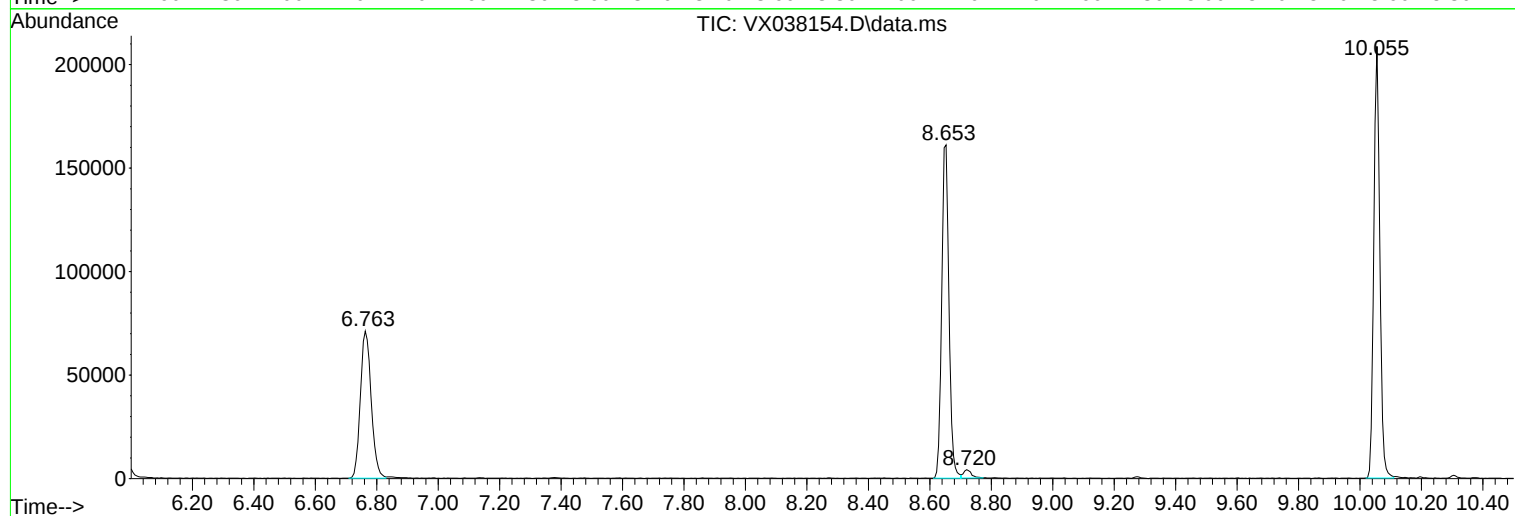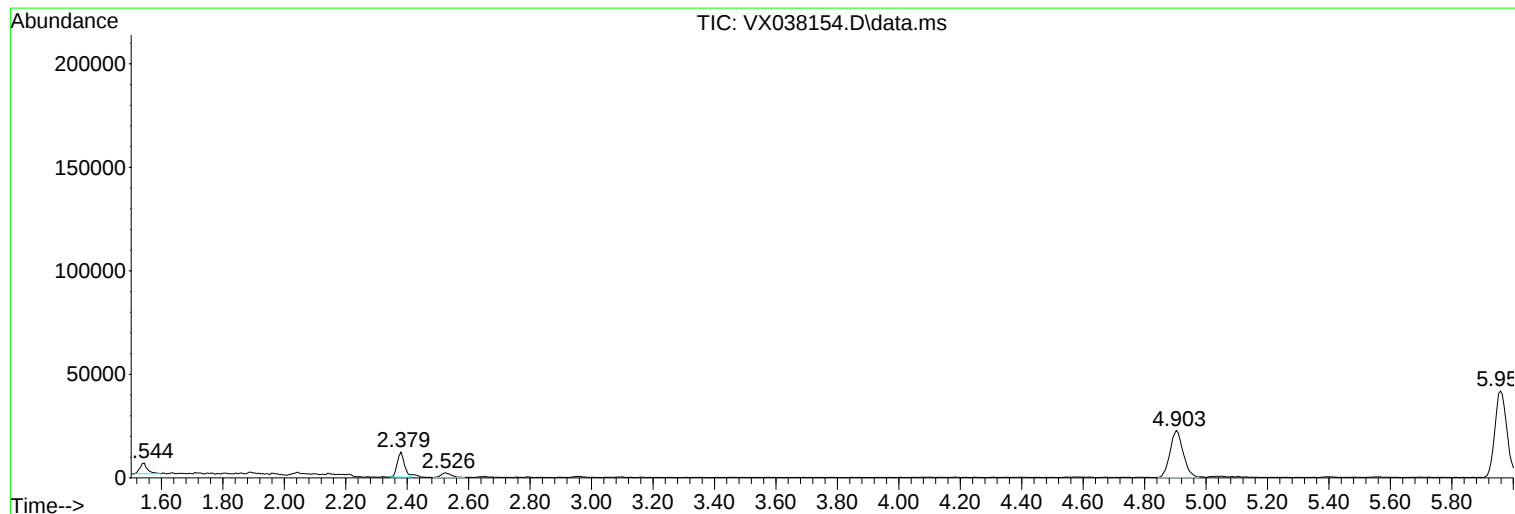

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038154.D
Acq On : 07 Oct 2023 03:19
Operator : JC/MD
Sample : 04783-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
231003027-03RE










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X100623W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown1.544 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.544	3.90 ug/l	8769	Bromochloromethane	4.909

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Thiophene-3-ol, tetrahydro-, 1,1...	136	C4H8O3S	013031-76-0	42
2			Benzeneethanamine, 2-fluoro-.bet...	185	C9H12FN02	103439-04-9	40
3			Amphetamine-3-methyl	149	C10H15N	000588-06-7	9
4			Ethanesulfonamide	109	C2H7N02S	001520-70-3	9
5			1-Adamantanemethylamine, .alpha....	179	C12H21N	013392-28-4	9

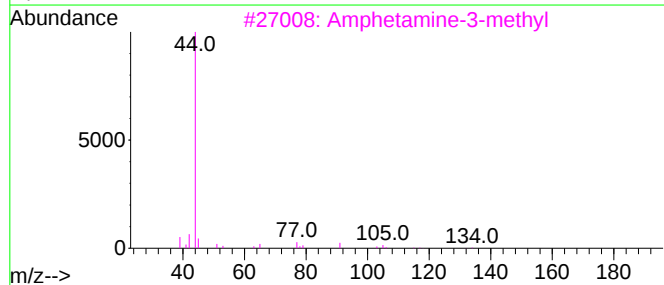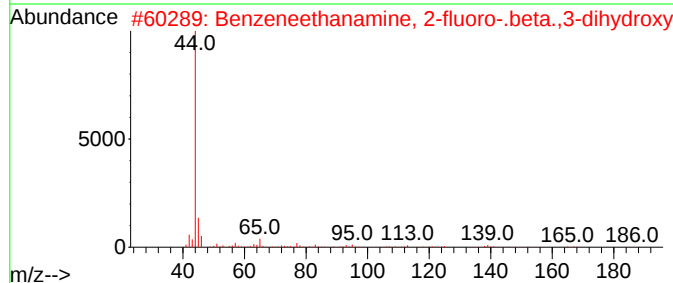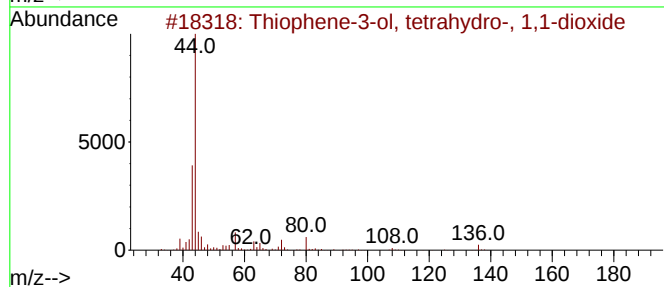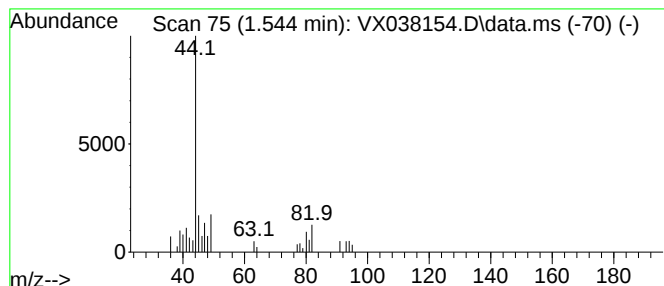

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038154.D
Acq On : 07 Oct 2023 03:19
Operator : JC/MD
Sample : 04783-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
231003027-03RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X100623W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown1.544	1.544	3.9	ug/l	8769	1	4.909	67374	30.0