


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100623\
Data File : VX038115.D
Acq On : 06 Oct 2023 08:56
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100523W.M
Title : SW846 8260
Last Update : Thu Oct 05 15:27:13 2023

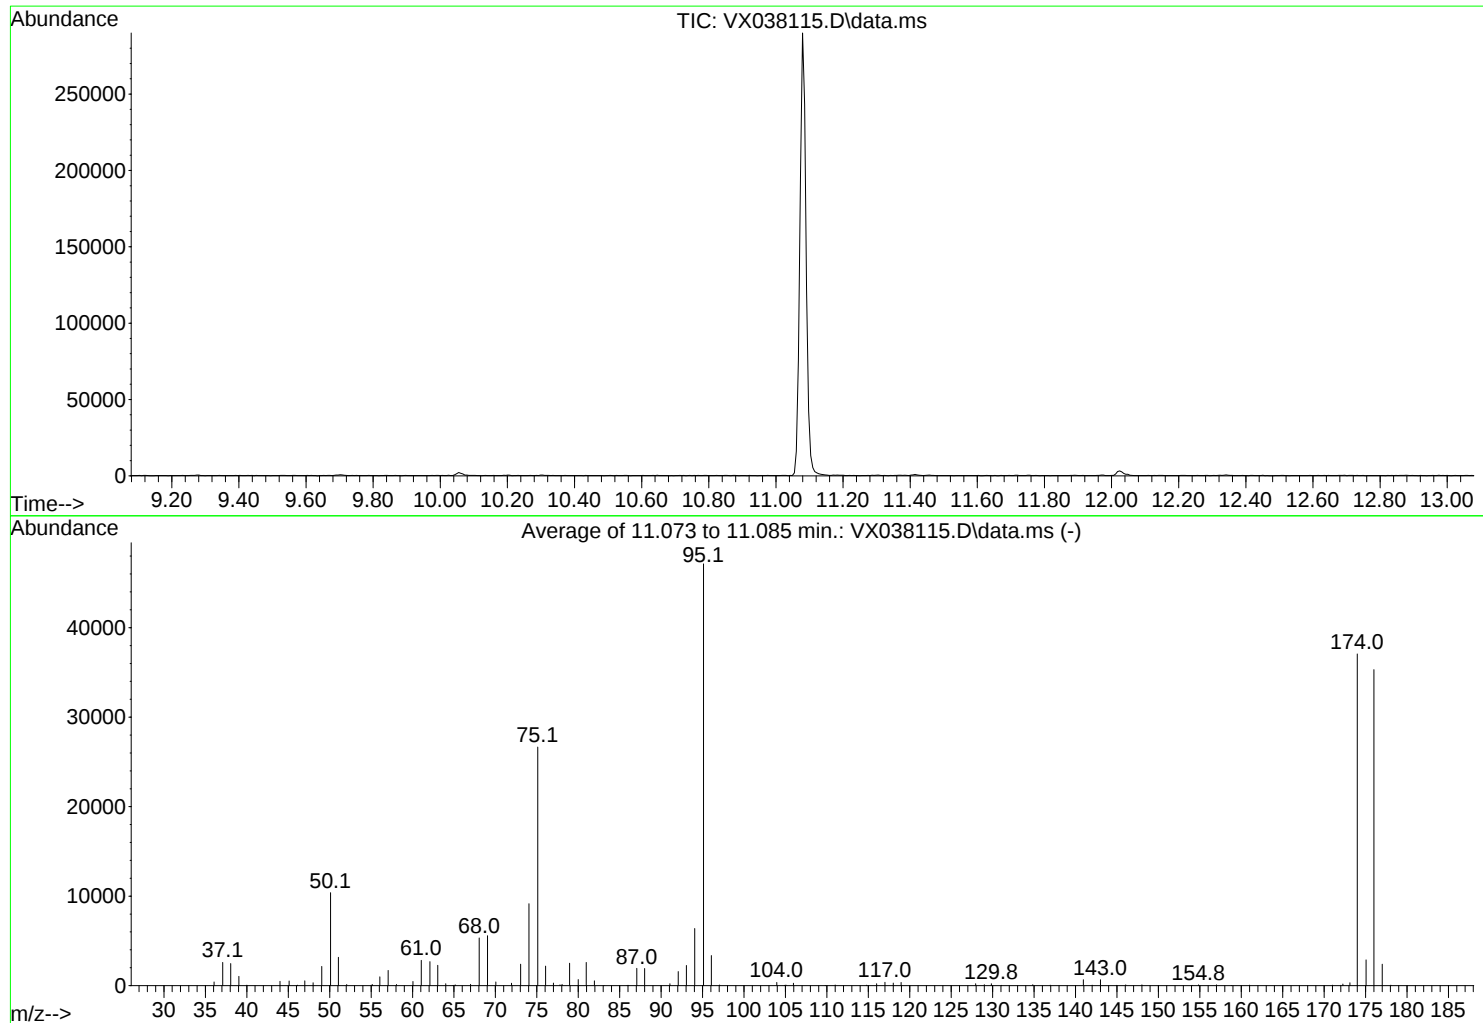

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	10385	PASS
75	95	30	60	56.6	26659	PASS
95	95	100	100	100.0	47136	PASS
96	95	5	9	7.1	3356	PASS
173	174	0.00	2	0.9	330	PASS
174	95	50	100	78.6	37061	PASS
175	174	5	9	7.7	2872	PASS
176	174	95	101	95.3	35312	PASS
177	176	5	9	6.8	2403	PASS