

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100625\
 Data File : VX048022.D
 Acq On : 06 Oct 2025 14:28
 Operator : JC/MD
 Sample : Q3201-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW10

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Title : SW846 8260

Signal : TIC: VX048022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.379	692	704	721	rBV	94874	308016	32.06%	5.903%
2	5.538	721	730	753	rVB	135617	427094	44.45%	8.186%
3	5.946	786	797	819	rBV2	109052	317760	33.07%	6.090%
4	6.239	837	845	858	rVB3	5479	16477	1.72%	0.316%
5	6.751	920	929	949	rBV	257015	668069	69.54%	12.804%
6	7.970	1121	1129	1141	rVB4	6559	14534	1.51%	0.279%
7	8.092	1141	1149	1160	rBV2	18861	43025	4.48%	0.825%
8	8.635	1229	1238	1252	rBV	524291	865525	90.09%	16.589%
9	10.037	1462	1468	1488	rVB	633830	909762	94.69%	17.437%
10	11.067	1631	1637	1651	rBV	490059	675802	70.34%	12.952%
11	12.006	1785	1791	1802	rVV	723330	960758	100.00%	18.414%
12	12.110	1802	1808	1810	rVV4	5947	10746	1.12%	0.206%




Sum of corrected areas: 5217568

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100625\
Data File : VX048022.D
Acq On : 06 Oct 2025 14:28
Operator : JC/MD
Sample : Q3201-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

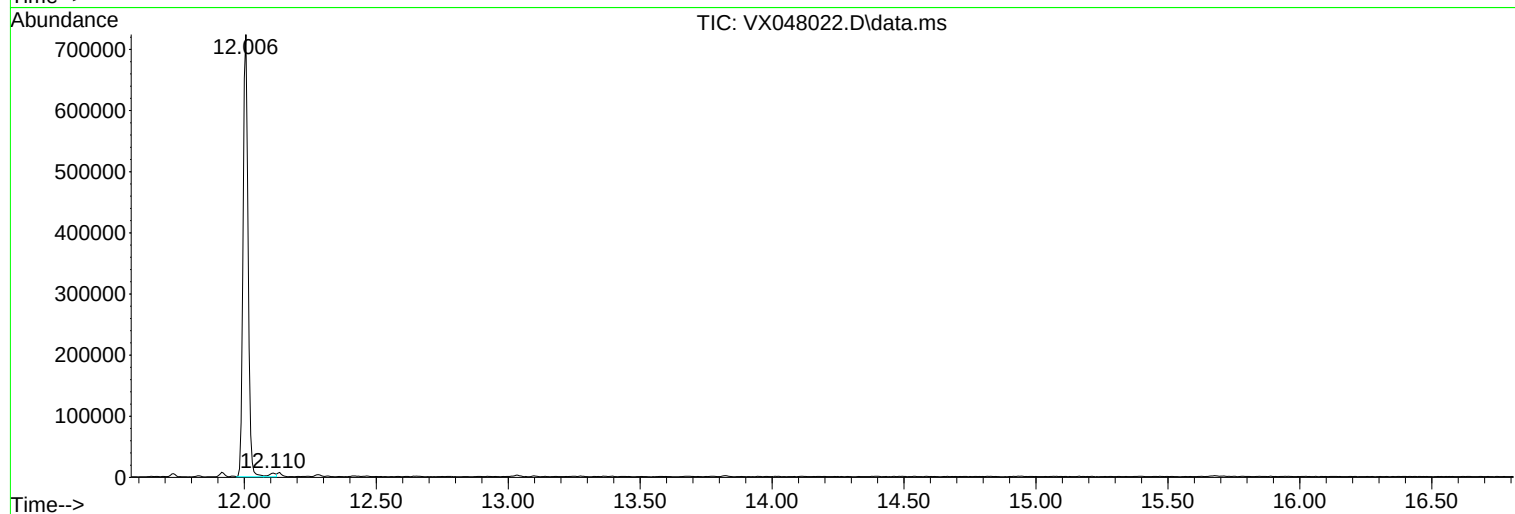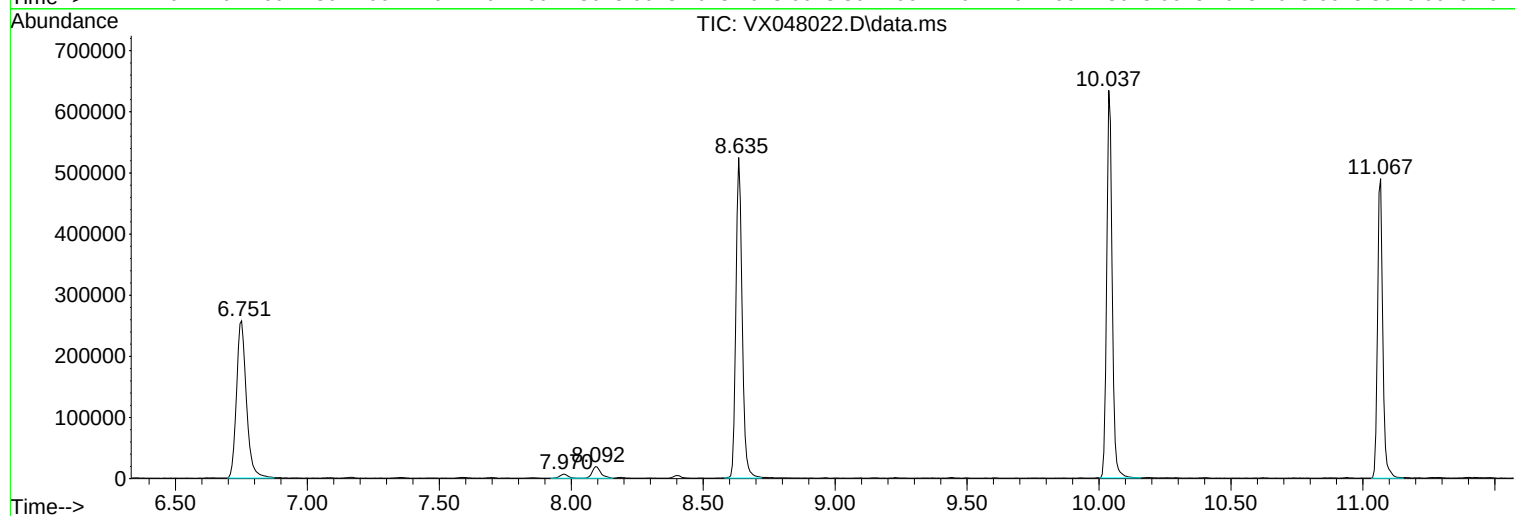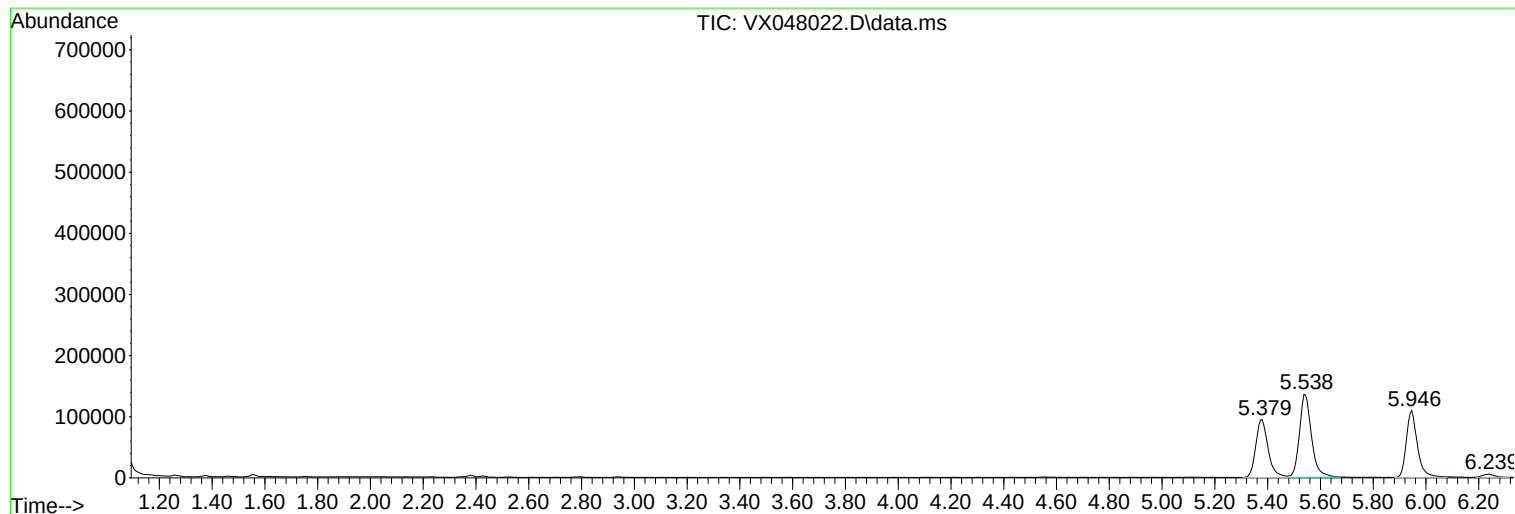

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100625\
Data File : VX048022.D
Acq On : 06 Oct 2025 14:28
Operator : JC/MD
Sample : Q3201-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100625\
Data File : VX048022.D
Acq On : 06 Oct 2025 14:28
Operator : JC/MD
Sample : Q3201-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc