

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100625\  
Data File : VX048027.D  
Acq On : 06 Oct 2025 16:12  
Operator : JC/MD  
Sample : Q3202-07  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SY-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091625W.M

Title : SW846 8260

Signal : TIC: VX048027.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.373       | 691           | 703         | 719          | rBV4     | 81702          | 266048        | 32.16%          | 5.971%        |
| 2         | 5.538       | 720           | 730         | 754          | rVB      | 118117         | 374924        | 45.32%          | 8.415%        |
| 3         | 5.946       | 786           | 797         | 817          | rBV      | 92439          | 270571        | 32.71%          | 6.073%        |
| 4         | 6.751       | 919           | 929         | 948          | rBV      | 224288         | 591021        | 71.44%          | 13.265%       |
| 5         | 8.635       | 1231          | 1238        | 1254         | rBV      | 457423         | 740467        | 89.51%          | 16.619%       |
| 6         | 10.037      | 1462          | 1468        | 1487         | rBV      | 555963         | 810266        | 97.94%          | 18.185%       |
| 7         | 11.067      | 1631          | 1637        | 1651         | rBV      | 415354         | 575034        | 69.51%          | 12.906%       |
| 8         | 12.006      | 1785          | 1791        | 1803         | rBV      | 614364         | 827289        | 100.00%         | 18.567%       |




Sum of corrected areas: 4455620

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100625\  
Data File : VX048027.D  
Acq On : 06 Oct 2025 16:12  
Operator : JC/MD  
Sample : Q3202-07  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SY-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091625W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

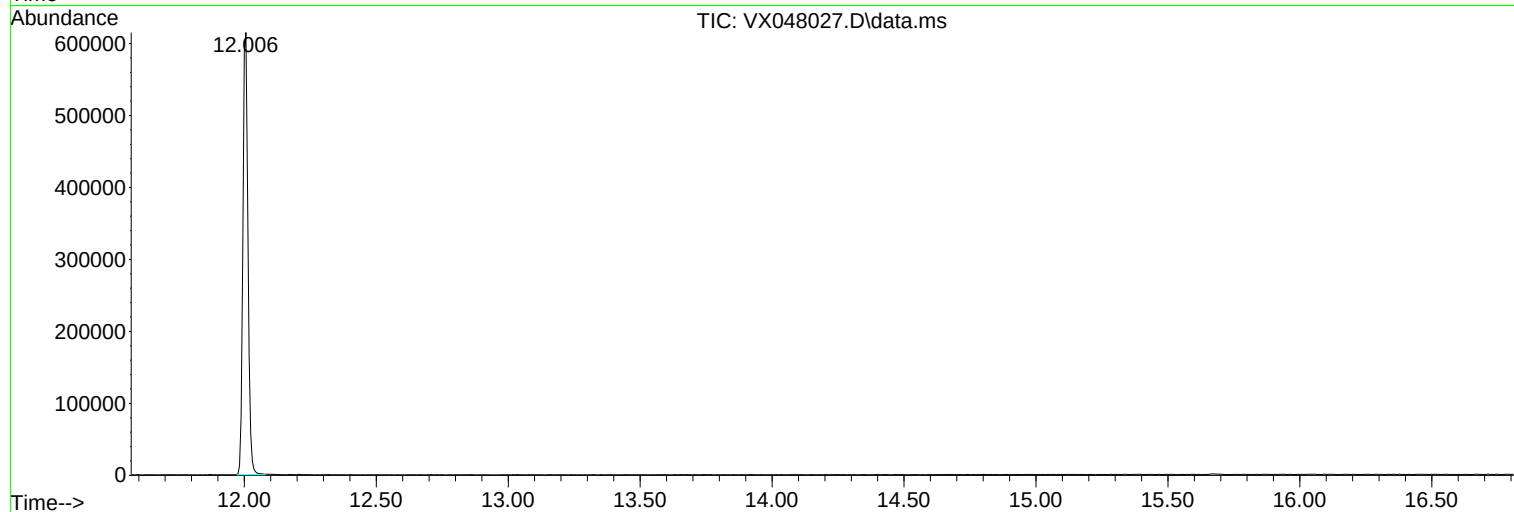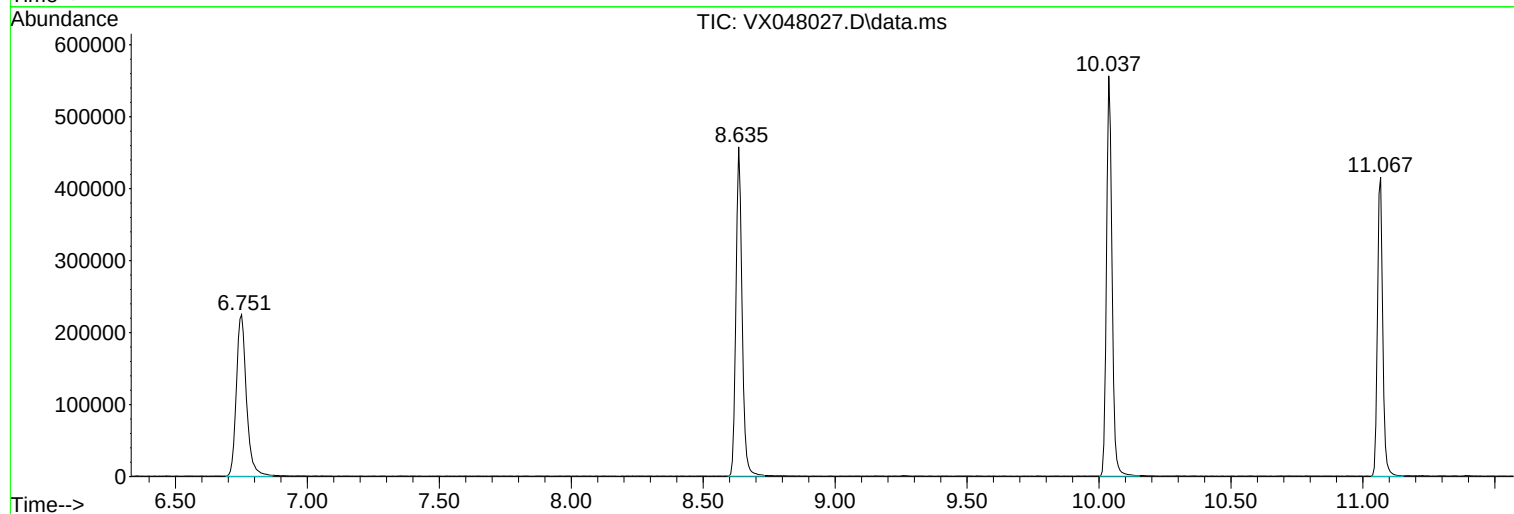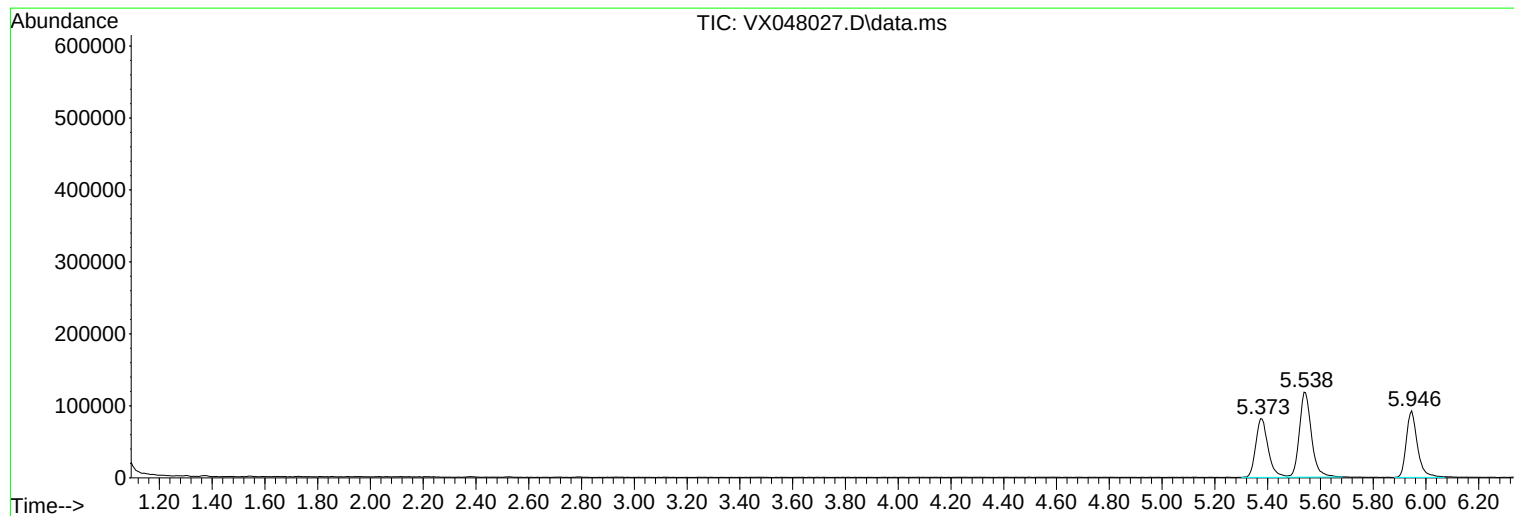

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100625\  
Data File : VX048027.D  
Acq On : 06 Oct 2025 16:12  
Operator : JC/MD  
Sample : Q3202-07  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SY-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091625W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100625\  
Data File : VX048027.D  
Acq On : 06 Oct 2025 16:12  
Operator : JC/MD  
Sample : Q3202-07  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SY-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091625W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |