

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100719\
Data File : VX012868.D
Acq On : 08 Oct 2019 04:03
Operator : JC/SP
Sample : K5216-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S49-0541

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	921371	1095637	1.26%	1.056%
2	1.399	80	84	93	rBV	894929	906301	1.04%	0.874%
3	4.588	592	607	631	rBV	4966881	13689227	15.72%	13.194%
4	7.234	1023	1041	1065	rBV	32232306	87100065	100.00%	83.952%
5	8.709	1276	1283	1290	rBV	625407	958482	1.10%	0.924%


Sum of corrected areas: 103749712

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100719\
Data File : VX012868.D
Acq On : 08 Oct 2019 04:03
Operator : JC/SP
Sample : K5216-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S49-0541

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

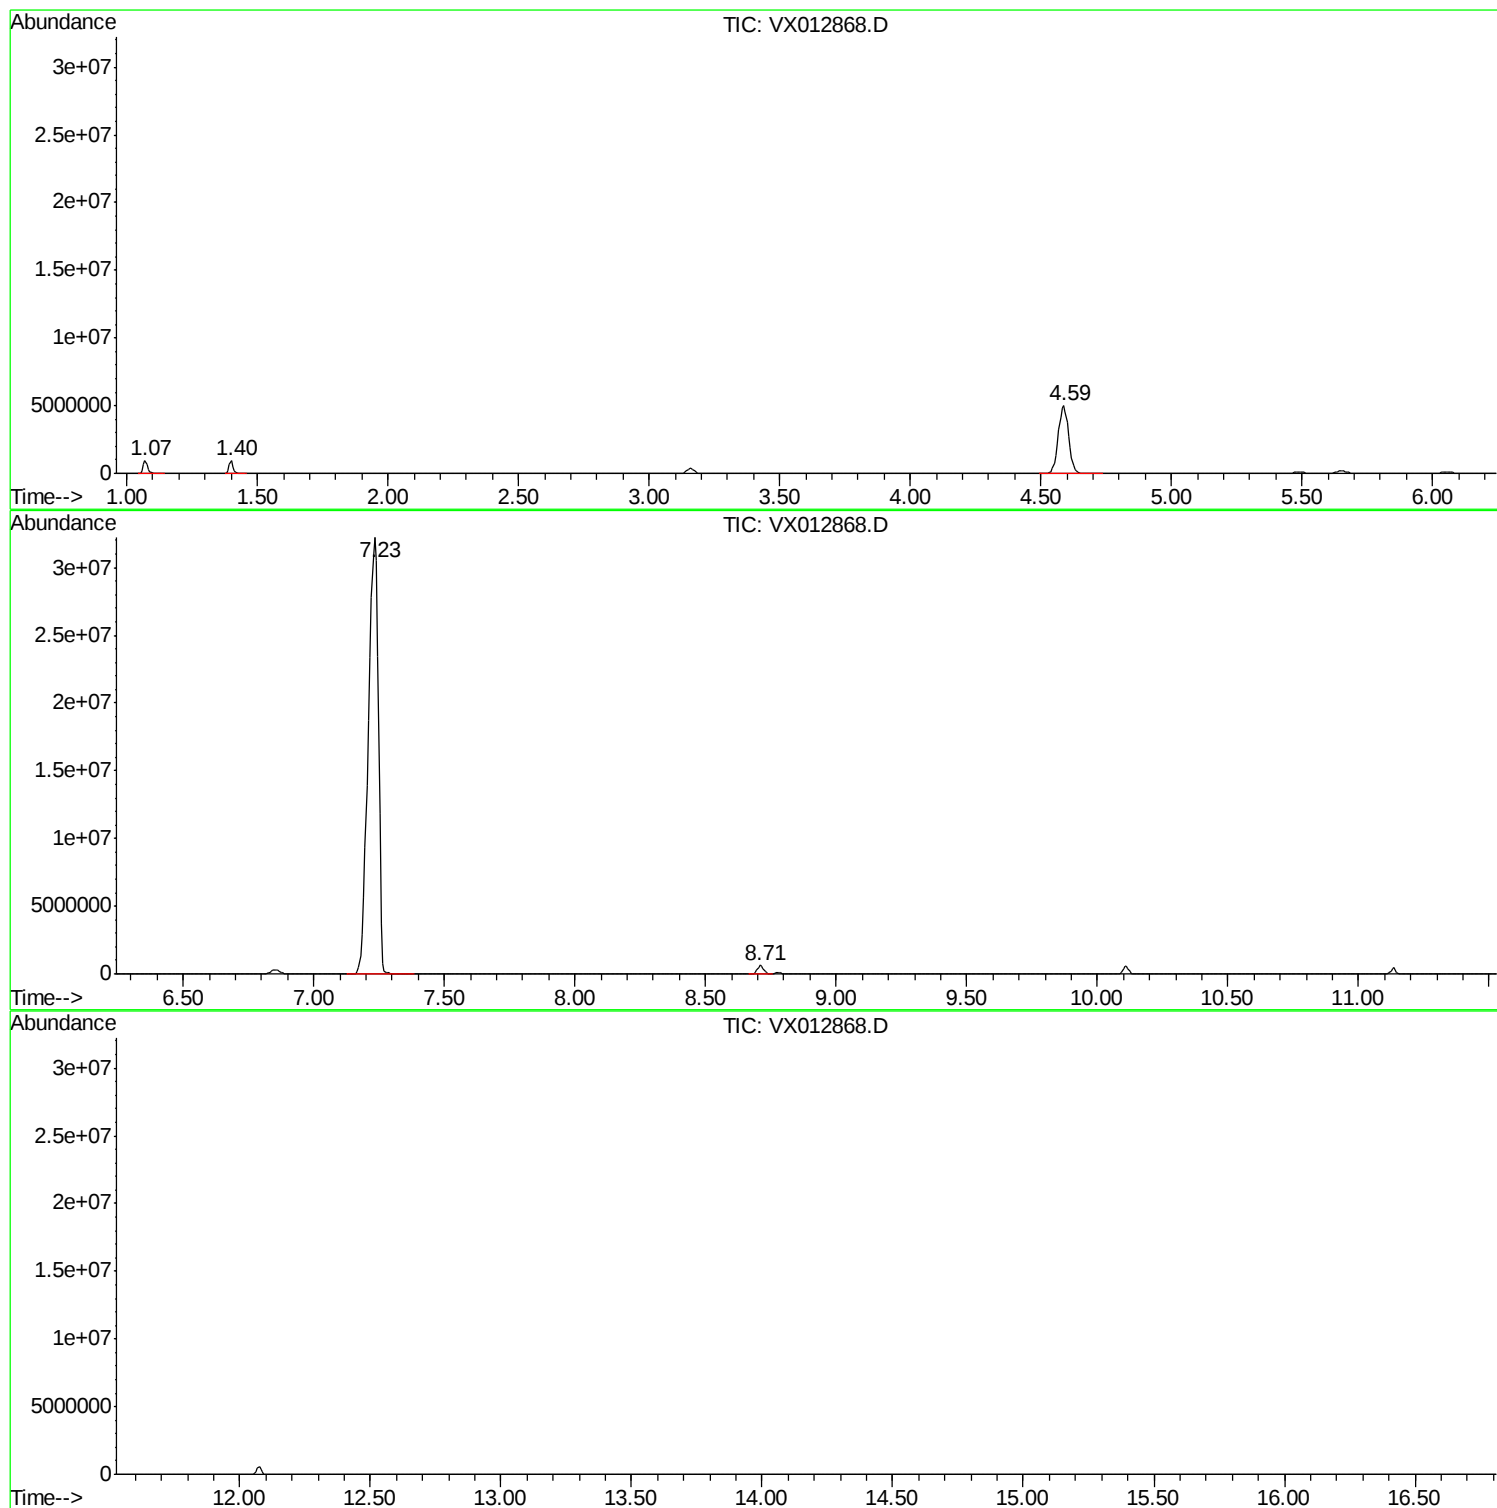

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100719\
Data File : VX012868.D
Acq On : 08 Oct 2019 04:03
Operator : JC/SP
Sample : K5216-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S49-0541

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100719\
Data File : VX012868.D
Acq On : 08 Oct 2019 04:03
Operator : JC/SP
Sample : K5216-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S49-0541

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc