

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100720\
 Data File : VX018818.D
 Acq On : 07 Oct 2020 18:06
 Operator : JC/SP
 Sample : VIBLK69
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK69

Quant Time: Oct 08 02:26:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 08 01:16:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	136540	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	129181	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	58308	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	35649	4.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.40%
7) Chloroethane-d5	1.70	69	33915	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.60%
11) 1,1-Dichloroethene-d2	2.34	63	66644	3.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.00%
20) 2-Butanone-d5	4.56	46	152336	72.82	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	145.64%#
24) Chloroform-d	5.14	84	100683	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.40%
26) 1,2-Dichloroethane-d4	6.03	65	60881	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	6.04	84	176044	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.60%
36) 1,2-Dichloropropane-d6	7.37	67	57385	6.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	123.60%
41) Toluene-d8	8.70	98	154985	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
45) trans-1,3-Dichloropropene-	8.99	79	24756	4.96	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.20%
48) 2-Hexanone-d5	9.43	63	118140	70.60	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	141.20%#
59) 1,1,2,2-Tetrachloroethane-	11.23	84	46957	6.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	124.40%#
65) 1,2-Dichlorobenzene-d4	12.36	152	62926	5.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.00%


Target Compounds					Ovalue
16) Methylene chloride	2.84	84	3904	0.473 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100720\
Data File : VX018818.D
Acq On : 07 Oct 2020 18:06
Operator : JC/SP
Sample : VIBLK69
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK69

Quant Time: Oct 08 02:26:18 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 08 01:16:58 2020
Response via : Initial Calibration

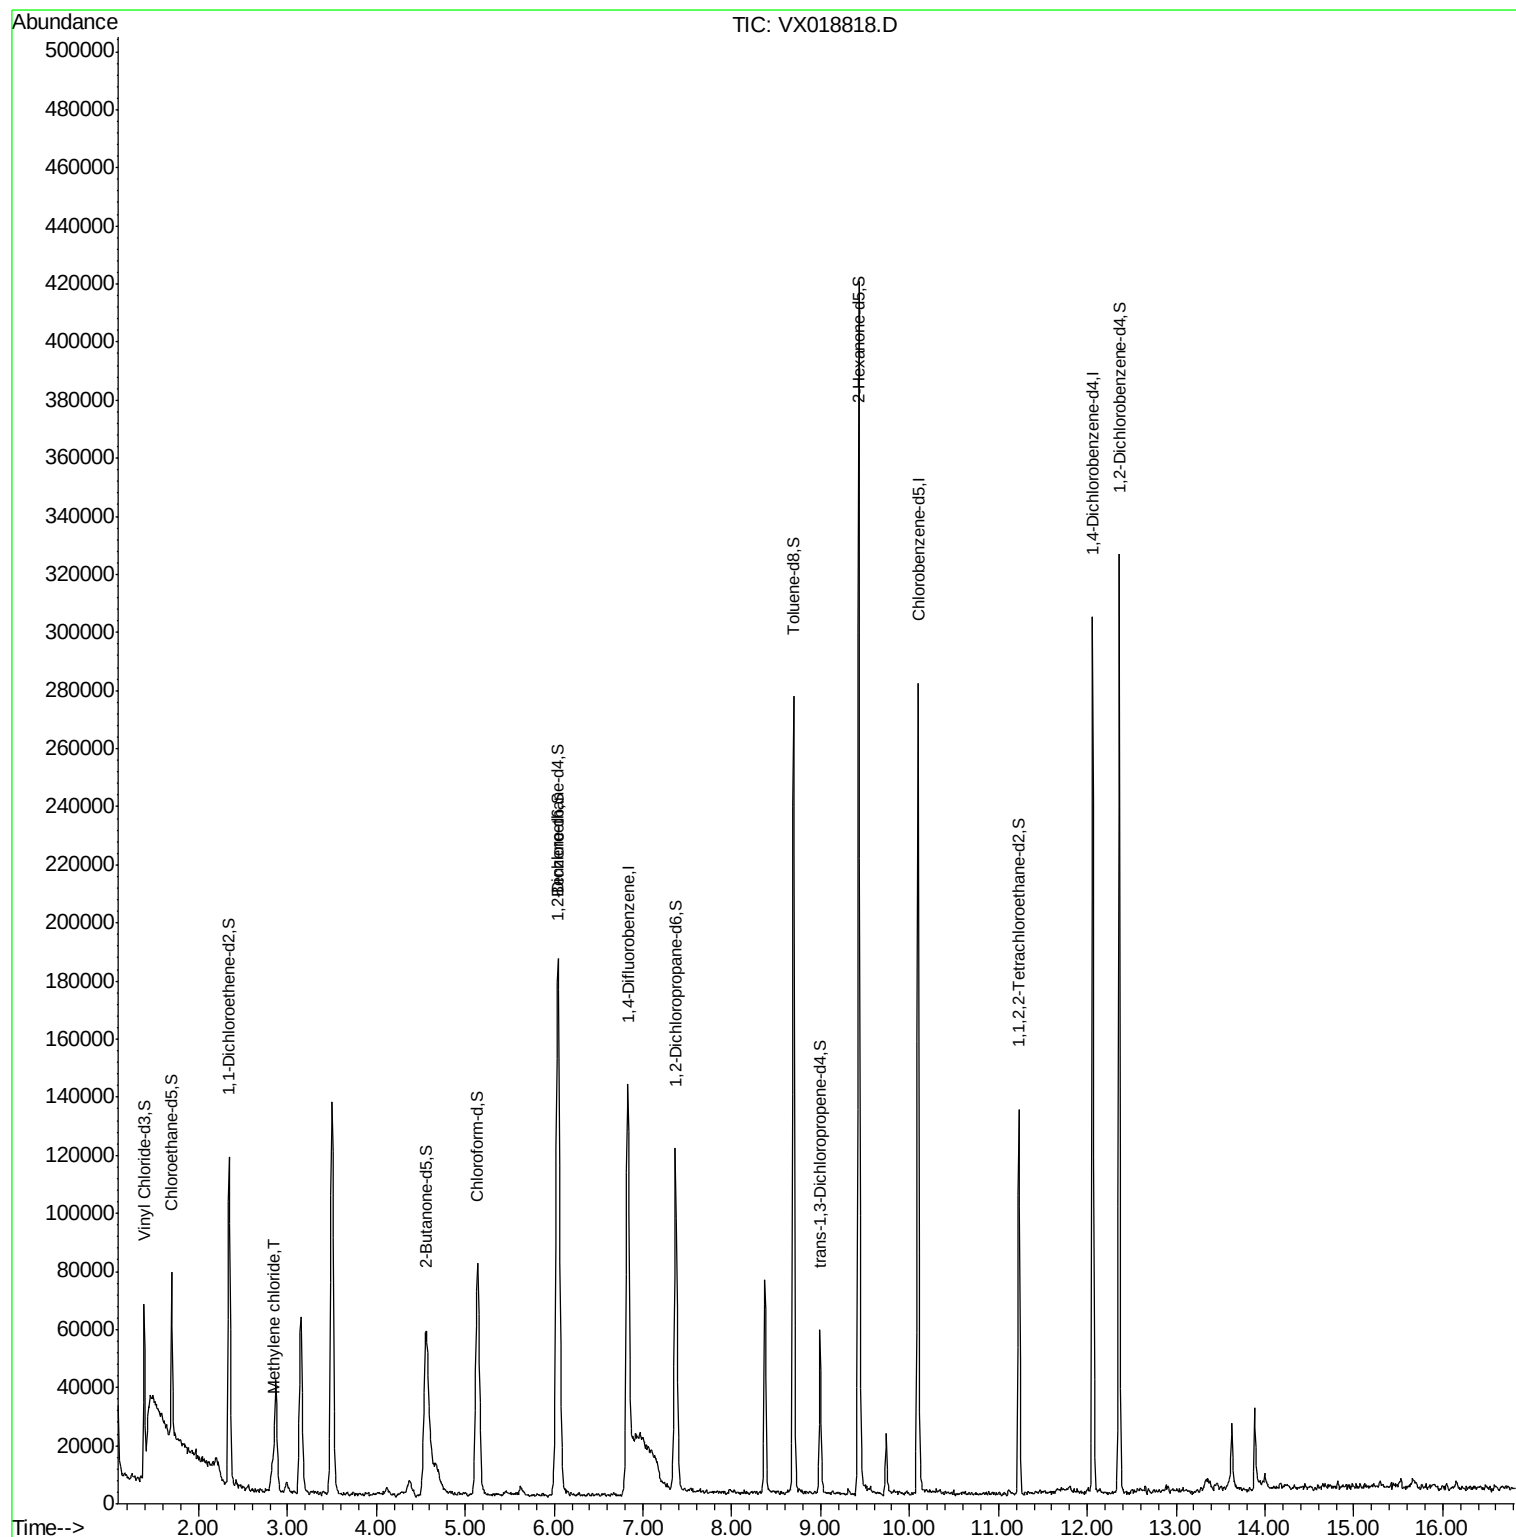

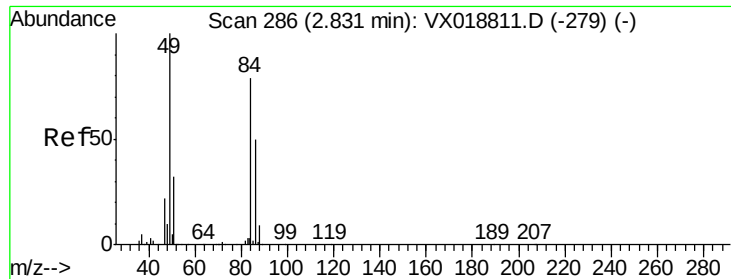

#16
 Methylene chloride
 Concen: 0.473 ug/L
 RT: 2.84 min Scan# 287
 Delta R.T. 0.01 min
 Lab File: VX018818.D
 Acq: 07 Oct 2020 18:06

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK69

Tot Ion: 84 Resp: 3904
 Ion Ratio Lower Upper
 84 100
 86 73.7 45.6 84.8
 49 102.4 85.8 159.3

