

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100720\
 Data File : VX018824.D
 Acq On : 07 Oct 2020 20:39
 Operator : JC/SP
 Sample : L4290-01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 JLWS9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.386	46	49	60	rBV	56968	59283	9.42%	1.240%
2	1.697	95	100	110	rBV	53995	66872	10.63%	1.399%
3	2.221	184	186	195	rVB8	5388	9601	1.53%	0.201%
4	2.343	200	206	213	rBV	109012	172268	27.37%	3.604%
5	2.465	219	226	234	rVB3	4229	12102	1.92%	0.253%
6	3.148	332	338	350	rVB5	6912	18085	2.87%	0.378%
7	3.501	385	396	404	rBV2	19367	45720	7.26%	0.957%
8	4.556	556	569	592	rBV	60149	262623	41.73%	5.494%
9	5.141	653	665	677	rBV	82713	246206	39.12%	5.151%
10	5.635	735	746	752	rVB	2425	6769	1.08%	0.142%
11	6.043	801	813	828	rBV2	183855	550896	87.53%	11.526%
12	6.830	932	942	951	rBV	140603	337328	53.60%	7.057%
13	7.141	984	993	994	rBV8	2786	6556	1.04%	0.137%
14	7.366	1022	1030	1045	rVB	118352	267000	42.42%	5.586%
15	8.372	1188	1195	1203	rBV	77404	124928	19.85%	2.614%
16	8.531	1213	1221	1229	rBV3	13014	26229	4.17%	0.549%
17	8.695	1240	1248	1257	rBV	277727	433812	68.93%	9.076%
18	8.994	1290	1297	1303	rBV	53895	79887	12.69%	1.671%
19	9.427	1362	1368	1380	rBV	434089	629346	100.00%	13.167%
20	10.098	1472	1478	1484	rBV	290081	401676	63.82%	8.404%
21	11.232	1659	1664	1671	rVB	139331	176018	27.97%	3.683%
22	12.061	1795	1800	1806	rBV	289929	358061	56.89%	7.491%
23	12.256	1828	1832	1839	rBV	16437	25614	4.07%	0.536%
24	12.359	1843	1849	1855	rBV	323383	406352	64.57%	8.502%
25	12.798	1915	1921	1926	rBV2	17920	26335	4.18%	0.551%
26	13.890	2094	2100	2105	rBV5	7115	12734	2.02%	0.266%
27	14.164	2141	2145	2154	rVB	12629	17459	2.77%	0.365%


Sum of corrected areas: 4779760

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100720\
Data File : VX018824.D
Acq On : 07 Oct 2020 20:39
Operator : JC/SP
Sample : L4290-01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLWS9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

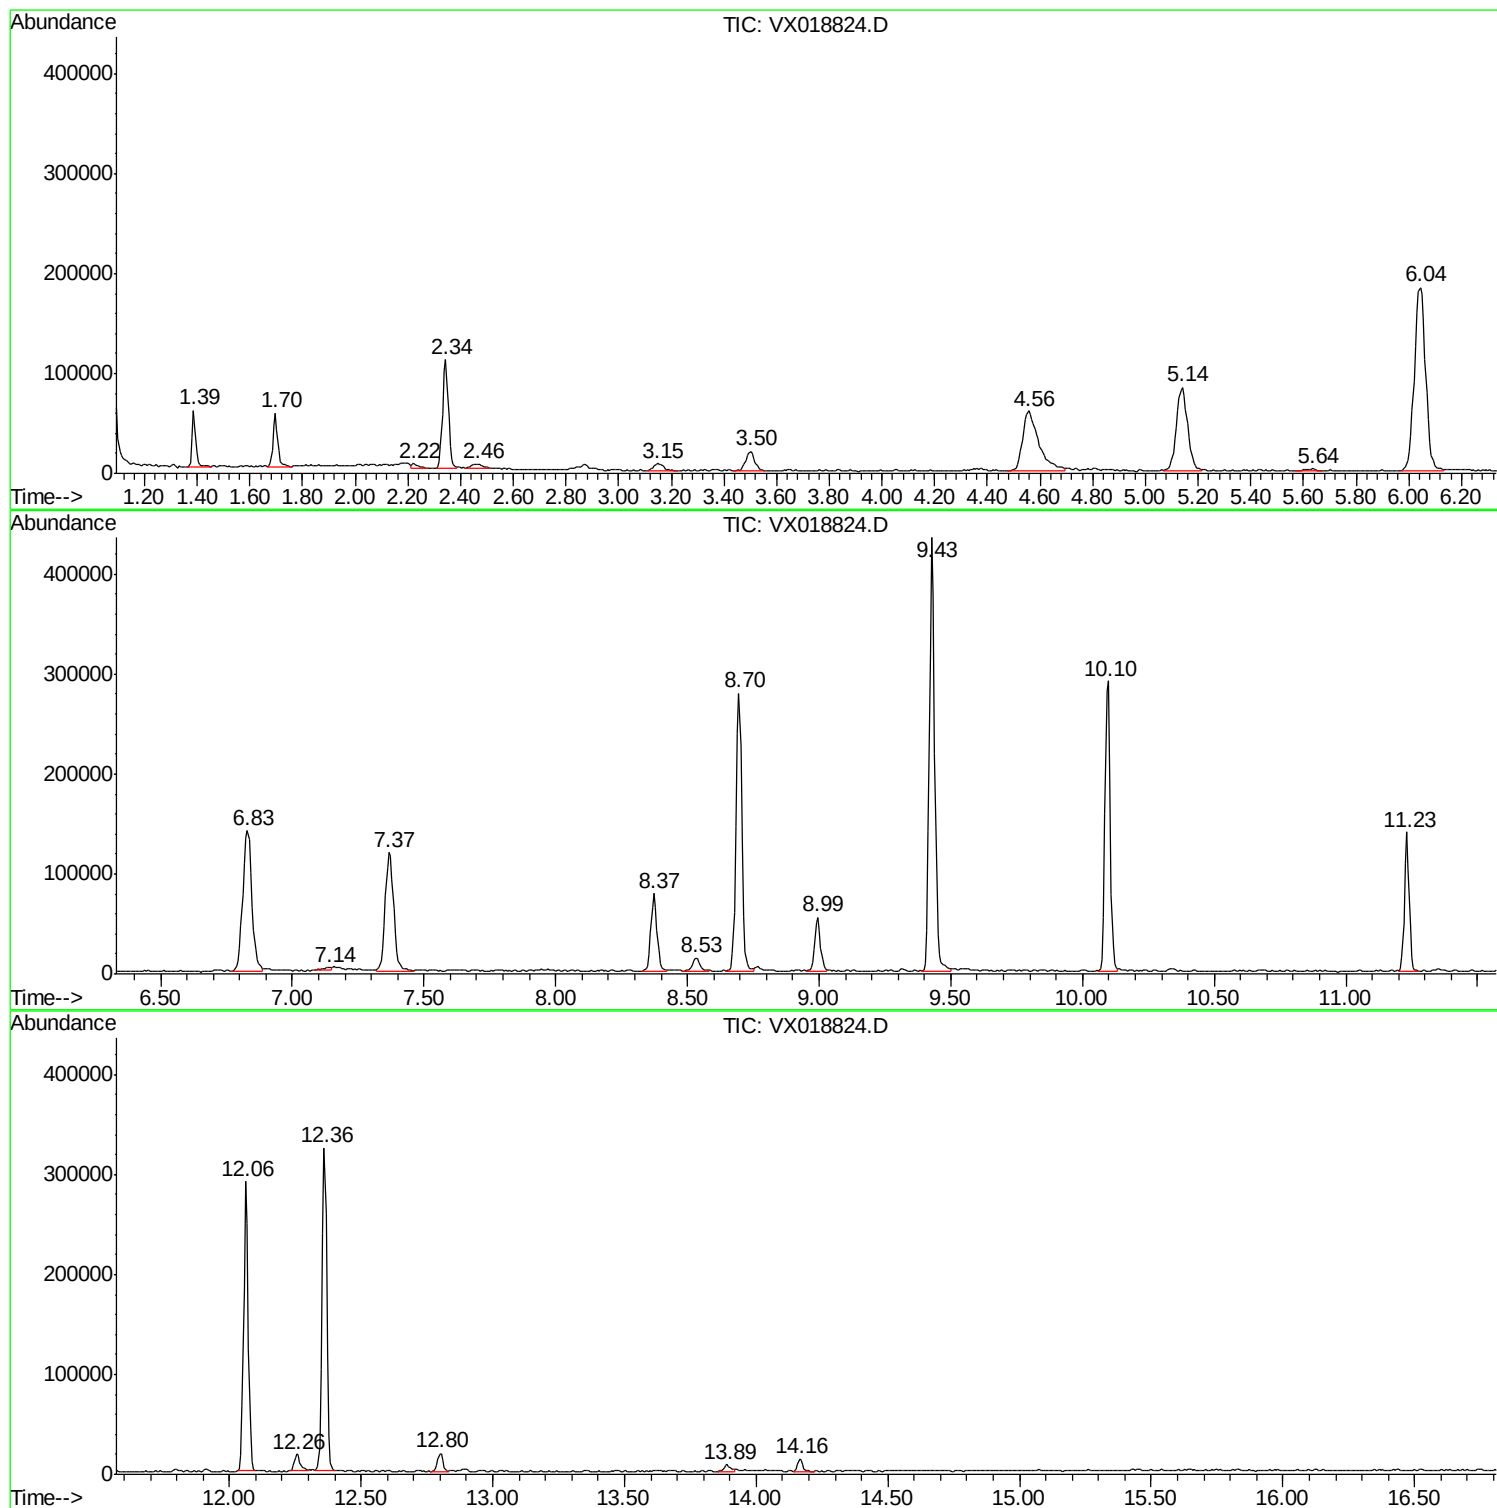

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100720\
Data File : VX018824.D
Acq On : 07 Oct 2020 20:39
Operator : JC/SP
Sample : L4290-01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLWS9










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.50	0.68 ug/L	45720	1,4-Difluorobenzene	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	n-Hexane	86	C6H14	000110-54-3	80
2		n-Hexane	86	C6H14	000110-54-3	72
3		n-Hexane	86	C6H14	000110-54-3	56
4		.alpha.-Amino-.gamma.-butyrolactone	101	C4H7NO2	001192-20-7	50
5		Hydroperoxide, hexyl	118	C6H14O2	004312-76-9	40

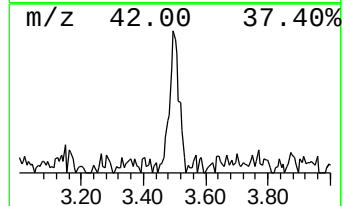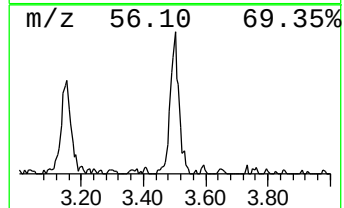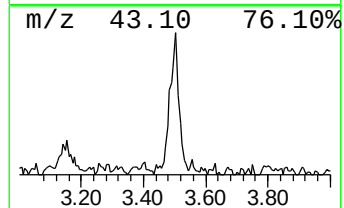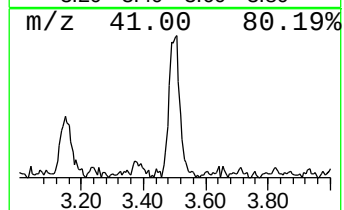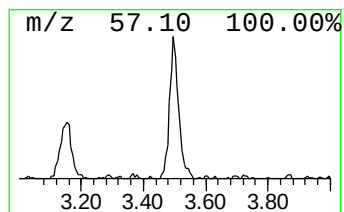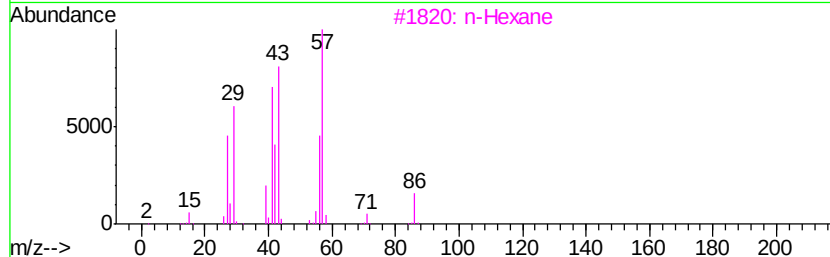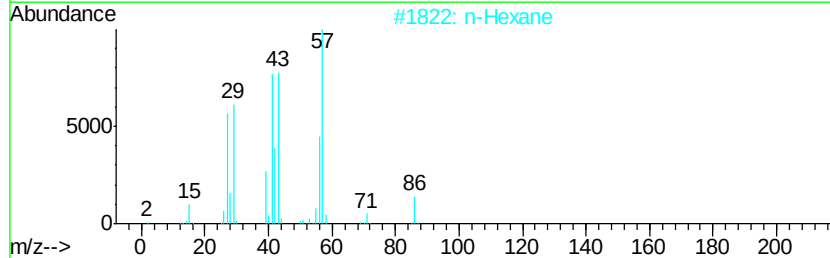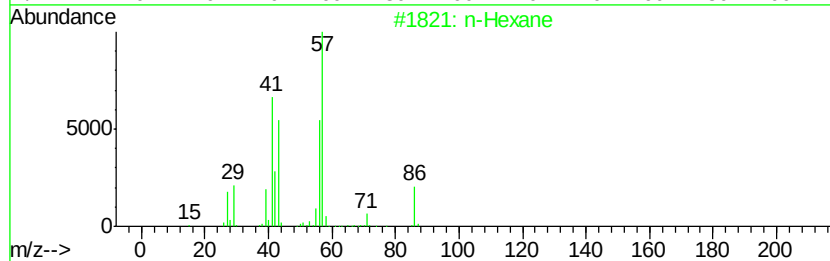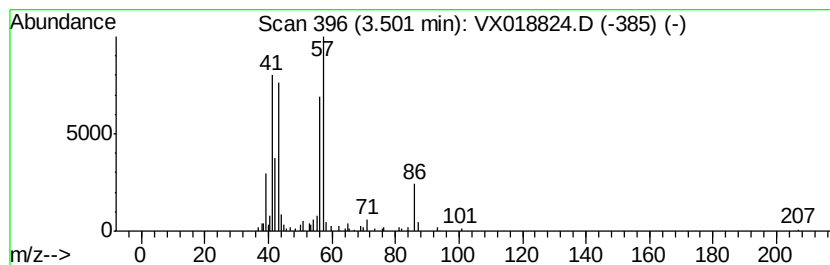

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX100720\
Data File : VX018824.D
Acq On : 07 Oct 2020 20:39
Operator : JC/SP
Sample : L4290-01
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLWS9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR100220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.50	0.7	ug/L	45720	1	6.83	337328	5.0