

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
 Data File : VX024655.D
 Acq On : 07 Oct 2021 18:57
 Operator : JC/MD
 Sample : M4000-11ME
 Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW906ME

Quant Time: Oct 07 23:10:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 07 23:05:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	283978	50.00	ug/L	0.00
28) Chlorobenzene-d5	10.061	117	256479	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	132230	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	82429	46.88	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.76%		
7) Chloroethane-d5	1.648	69	28691	24.79	ug/L	-0.01
Spiked Amount 50.000	Range 70 - 130		Recovery =	49.58%#		
11) 1,1-Dichloroethene-d2	2.264	63	115030	33.32	ug/L	-0.04
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.64%		
21) 2-Butanone-d5	4.513	46	97822	67.67	ug/L	0.05
Spiked Amount 100.000	Range 40 - 130		Recovery =	67.67%		
24) Chloroform-d	5.068	84	167281	46.98	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.96%		
26) 1,2-Dichloroethane-d4	5.964	65	122202	48.52	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.04%		
32) Benzene-d6	5.970	84	351760	48.69	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.38%		
36) 1,2-Dichloropropane-d6	7.312	67	107336	47.50	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.00%		
41) Toluene-d8	8.653	98	328679	46.69	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.38%		
43) trans-1,3-Dichloroprop...	8.958	79	46507	41.54	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.08%		
47) 2-Hexanone-d5	9.403	63	102500	96.62	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.62%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	148739	47.79	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.58%		
66) 1,2-Dichlorobenzene-d4	12.323	152	130206	50.33	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	100.66%		
Target Compounds						Qvalue
15) Methyl Acetate	2.733	43	1781	0.78	ug/L	# 65
16) Methylene chloride	2.776	84	2497	1.27	ug/L	85
34) Trichloroethene	7.129	95	178282	81.73	ug/L	96
46) Tetrachloroethene	9.275	164	3343	1.97	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
Data File : VX024655.D
Acq On : 07 Oct 2021 18:57
Operator : JC/MD
Sample : M4000-11ME
Misc : 5.01g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW906ME

Quant Time: Oct 07 23:10:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 07 23:05:28 2021
Response via : Initial Calibration




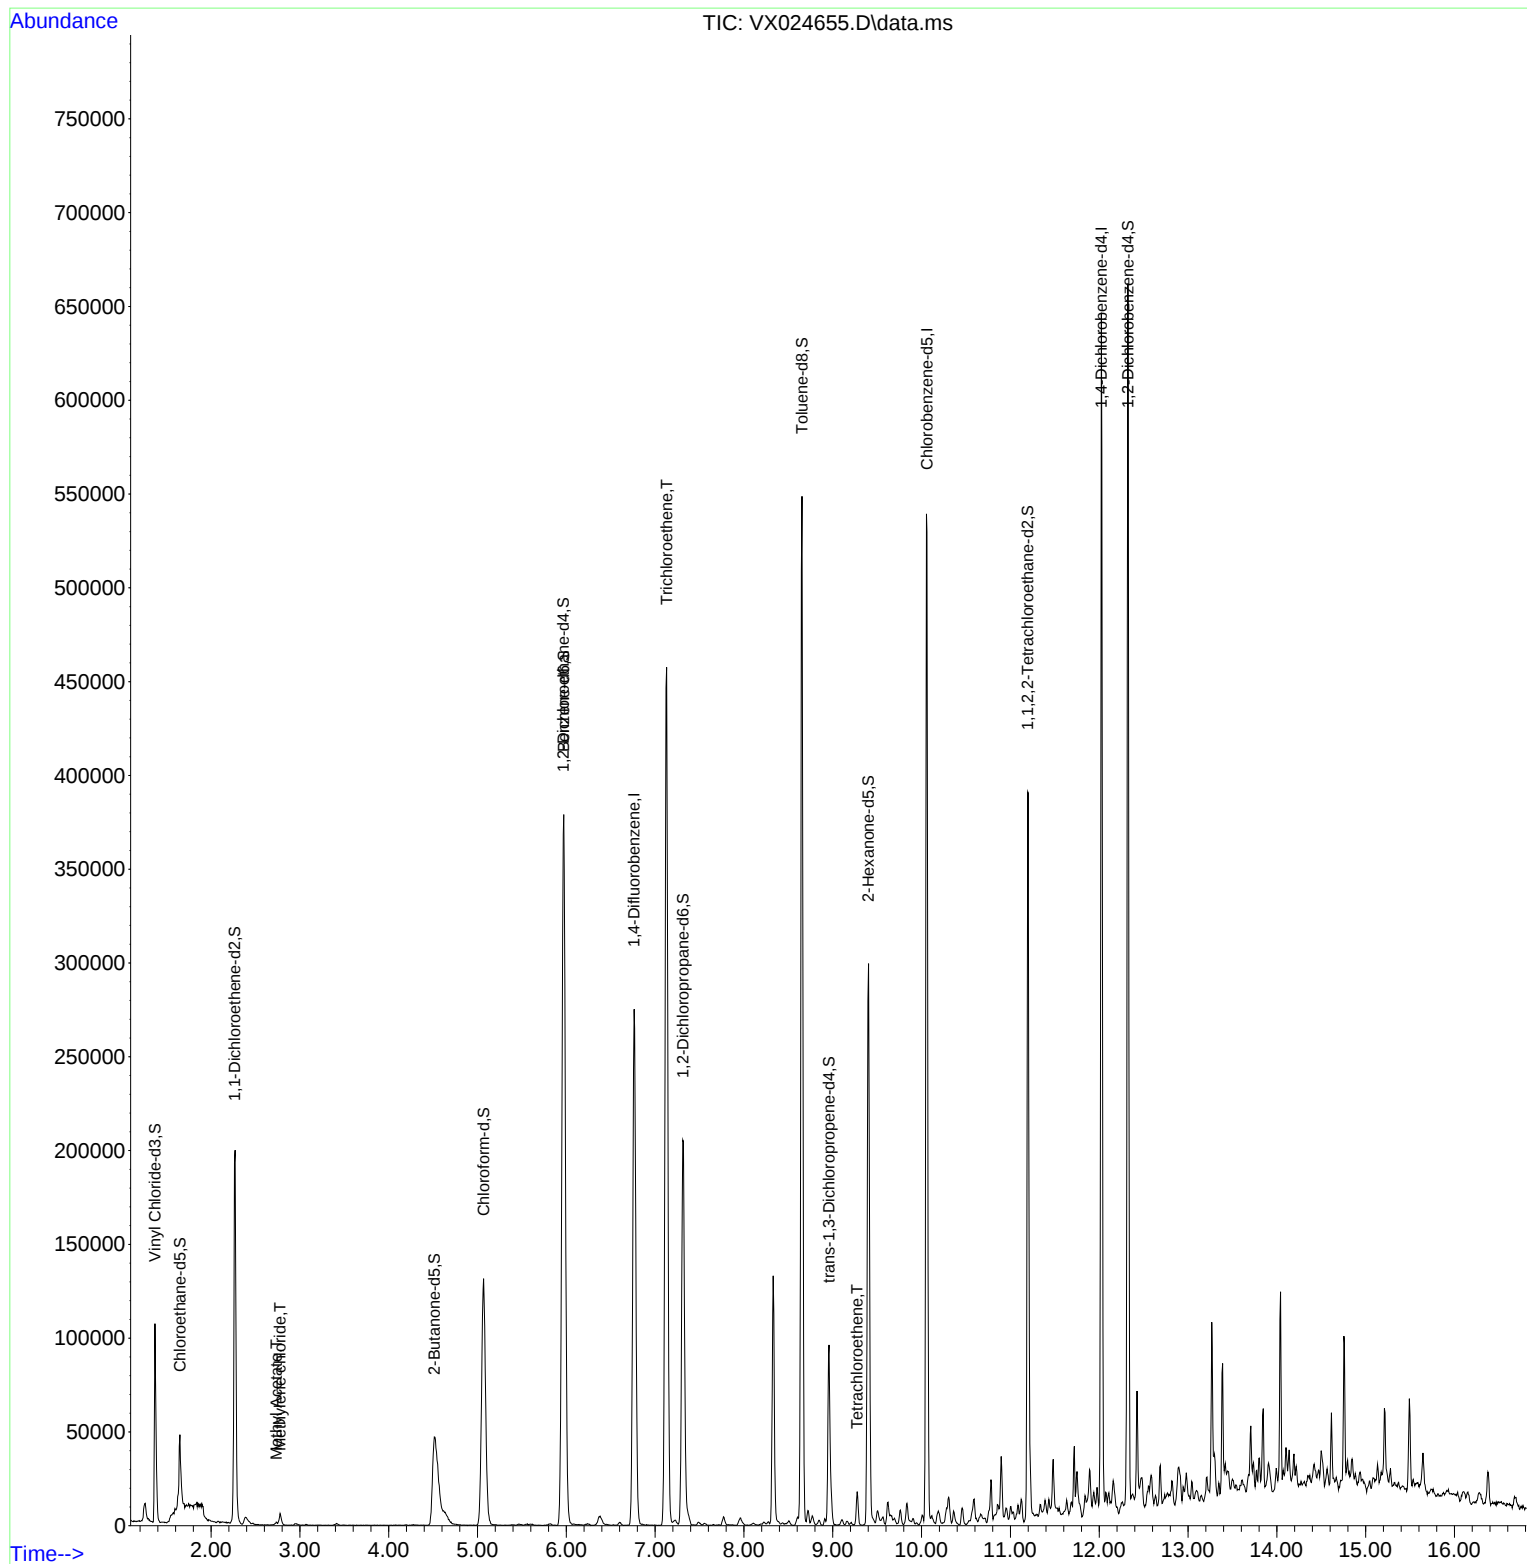


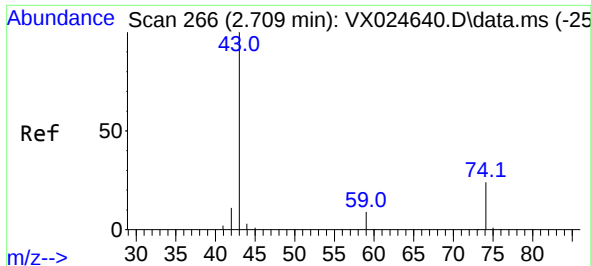

#15
Methyl Acetate
Concen: 0.78 ug/L
RT: 2.733 min Scan# 270
Delta R.T. 0.024 min
Lab File: VX024655.D
Acq: 07 Oct 2021 18:57




Instrument :
MSVOA_X
ClientSampleId :
EW906ME


Tgt Ion: 43 Resp: 1781
Ion Ratio Lower Upper
43 100
74 9.0 21.7 32.5#

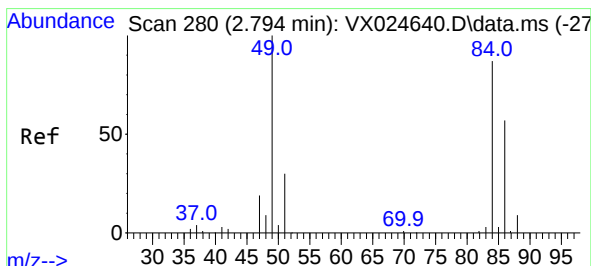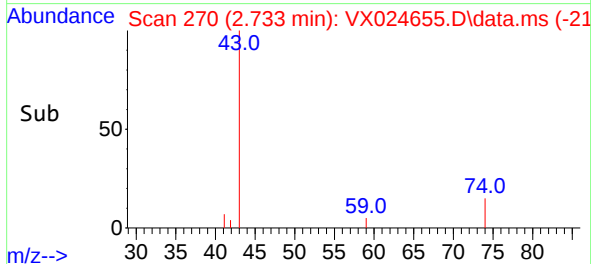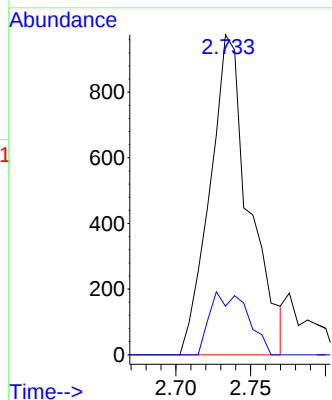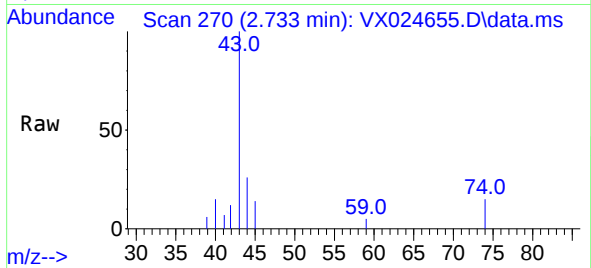

#16
Methylene chloride
Concen: 1.27 ug/L
RT: 2.776 min Scan# 277
Delta R.T. -0.018 min
Lab File: VX024655.D
Acq: 07 Oct 2021 18:57

Tgt Ion: 84 Resp: 2497
Ion Ratio Lower Upper
84 100
86 76.9 44.2 82.0
49 124.9 77.8 144.6


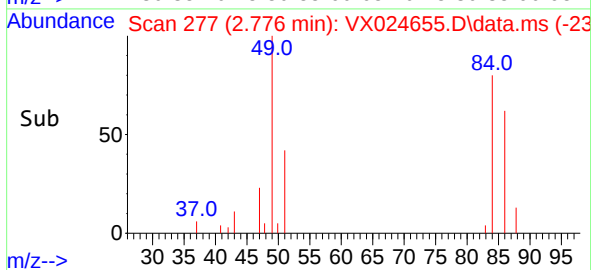
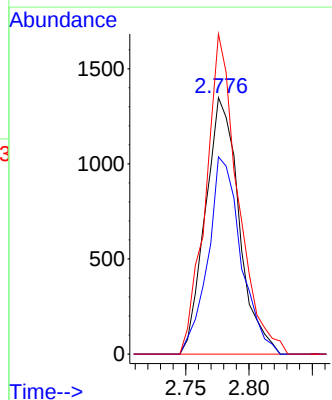
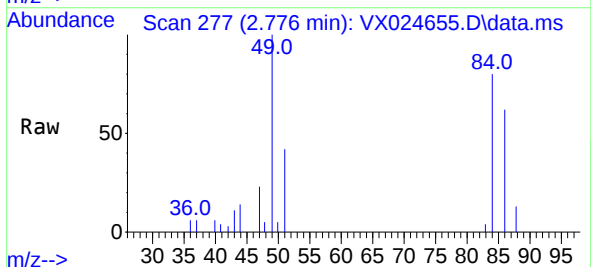


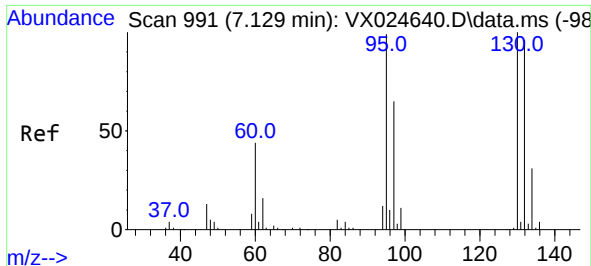

#34
Trichloroethene
Concen: 81.73 ug/L
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX024655.D
Acq: 07 Oct 2021 18:57

Instrument :
MSVOA_X
ClientSampleId :
EW906ME

Tgt Ion: 95 Resp: 178282
Ion Ratio Lower Upper
95 100
97 64.3 44.5 82.7
132 100.0 65.2 121.0
130 99.6 67.7 125.7

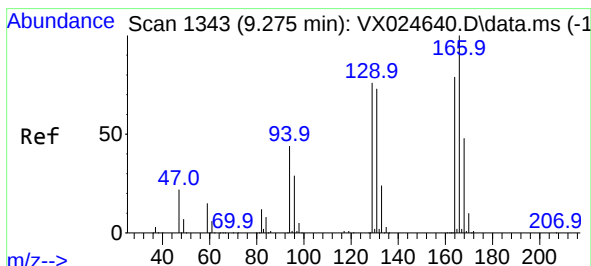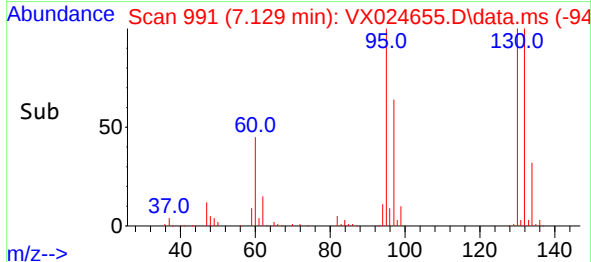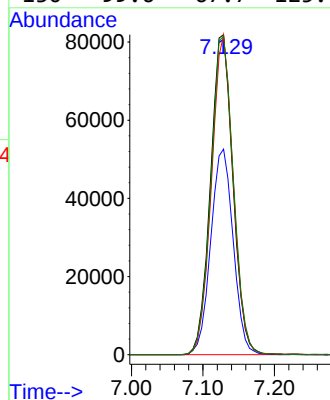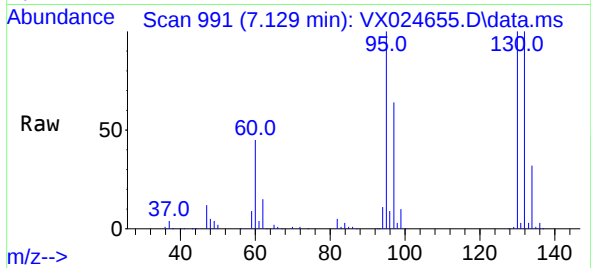

#46
Tetrachloroethene
Concen: 1.97 ug/L
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX024655.D
Acq: 07 Oct 2021 18:57

Tgt Ion: 164 Resp: 3343
Ion Ratio Lower Upper
164 100
129 86.1 65.6 121.8
131 94.2 63.7 118.3
166 123.1 93.0 172.6

