

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
 Data File : VX024643.D
 Acq On : 07 Oct 2021 14:08
 Operator : JC/MD
 Sample : M4001-01 100X
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M

Title : VOC Analysis

Signal : TIC: VX024643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	8581	12203	1.13%	0.149%
2	1.368	43	46	54	rVB	150004	138118	12.84%	1.686%
3	1.666	91	95	103	rVB	85104	104081	9.68%	1.271%
4	2.306	194	200	219	rVB	213472	345688	32.15%	4.220%
5	2.514	230	234	239	rBV2	918	1514	0.14%	0.018%
6	2.709	263	266	269	rBV3	383	542	0.05%	0.007%
7	2.794	275	280	285	rVB5	2123	3775	0.35%	0.046%
8	2.953	299	306	312	rBV2	936	1998	0.19%	0.024%
9	3.093	327	329	333	rVB3	542	776	0.07%	0.009%
10	3.440	384	386	389	rBV2	175	224	0.02%	0.003%
11	3.556	403	405	406	rBV2	199	151	0.01%	0.002%
12	4.471	545	555	570	rBV2	84834	260652	24.24%	3.182%
13	4.971	636	637	640	rBV	226	205	0.02%	0.003%
14	5.068	640	653	671	rVV	131486	421757	39.22%	5.149%
15	5.227	675	679	683	rVB2	202	318	0.03%	0.004%
16	5.477	718	720	723	rBV	247	209	0.02%	0.003%
17	5.538	726	730	731	rBV	453	477	0.04%	0.006%
18	5.751	764	765	768	rBV2	231	210	0.02%	0.003%
19	5.977	789	802	817	rBV2	371814	1075320	100.00%	13.128%
20	6.135	825	828	831	rVB2	330	311	0.03%	0.004%
21	6.476	882	884	887	rVB	334	303	0.03%	0.004%
22	6.543	893	895	896	rBV2	259	227	0.02%	0.003%
23	6.672	912	916	917	rBV2	133	134	0.01%	0.002%
24	6.769	922	932	948	rBV	286739	672797	62.57%	8.214%
25	7.062	979	980	983	rVB	319	191	0.02%	0.002%
26	7.129	983	991	1003	rBV2	42612	98726	9.18%	1.205%
27	7.312	1013	1021	1038	rBV	214095	472226	43.91%	5.765%
28	7.476	1044	1048	1049	rBV2	578	634	0.06%	0.008%
29	7.775	1095	1097	1098	rBV2	148	137	0.01%	0.002%
30	7.933	1118	1123	1128	rVB3	632	979	0.09%	0.012%
31	7.982	1128	1131	1132	rVB2	170	135	0.01%	0.002%
32	8.092	1147	1149	1152	rVB	339	321	0.03%	0.004%
33	8.116	1152	1153	1156	rBV	217	235	0.02%	0.003%
34	8.159	1158	1160	1163	rVV	171	155	0.01%	0.002%
35	8.330	1181	1188	1199	rBV	146802	241193	22.43%	2.945%
36	8.458	1205	1209	1213	rBV4	259	623	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
 Data File : VX024643.D
 Acq On : 07 Oct 2021 14:08
 Operator : JC/MD
 Sample : M4001-01 100X
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis

37	8.653	1234	1241	1248	rBV	539275	848493	78.91%	10.359%
38	8.726	1249	1253	1259	rVB	8070	12777	1.19%	0.156%
39	8.952	1285	1290	1306	rVB	107677	159306	14.81%	1.945%
40	9.275	1339	1343	1347	rVV2	1144	1472	0.14%	0.018%
41	9.391	1356	1362	1382	rBV	368834	537213	49.96%	6.559%
42	9.610	1394	1398	1400	rBV	230	290	0.03%	0.004%
43	9.750	1418	1421	1422	rBV2	200	177	0.02%	0.002%
44	10.055	1465	1471	1490	rVV	523189	726805	67.59%	8.873%
45	10.195	1492	1494	1500	rVB2	901	1007	0.09%	0.012%
46	10.305	1506	1512	1516	rBV	1790	2406	0.22%	0.029%
47	10.384	1523	1525	1527	rBV	171	194	0.02%	0.002%
48	10.604	1559	1561	1562	rBV2	204	134	0.01%	0.002%
49	10.653	1564	1569	1573	rVV4	994	1412	0.13%	0.017%
50	10.756	1584	1586	1590	rVB2	292	261	0.02%	0.003%
51	10.921	1611	1613	1616	rBV2	144	144	0.01%	0.002%
52	10.963	1616	1620	1624	rVB3	581	781	0.07%	0.010%
53	11.031	1628	1631	1632	rBV2	191	207	0.02%	0.003%
54	11.091	1637	1641	1642	rBV	292	350	0.03%	0.004%
55	11.122	1642	1646	1652	rVB2	3801	5018	0.47%	0.061%
56	11.195	1652	1658	1665	rBV	393417	505884	47.04%	6.176%
57	11.451	1698	1700	1702	rVB	613	462	0.04%	0.006%
58	11.482	1702	1705	1709	rBV3	1068	1583	0.15%	0.019%
59	11.555	1715	1717	1721	rVB3	539	412	0.04%	0.005%
60	11.616	1725	1727	1730	rBV	177	219	0.02%	0.003%
61	11.713	1741	1743	1746	rBV2	433	439	0.04%	0.005%
62	11.750	1746	1749	1756	rVV2	4056	4887	0.45%	0.060%
63	11.854	1761	1766	1769	rVB3	535	830	0.08%	0.010%
64	11.933	1776	1779	1783	rBV3	1579	2165	0.20%	0.026%
65	11.969	1783	1785	1789	rVV3	1108	1282	0.12%	0.016%
66	12.024	1789	1794	1807	rVV	591182	732631	68.13%	8.945%
67	12.122	1807	1810	1813	rVV3	1453	2414	0.22%	0.029%
68	12.152	1813	1815	1822	rVB2	3084	3488	0.32%	0.043%
69	12.232	1825	1828	1830	rBV	324	316	0.03%	0.004%
70	12.323	1836	1843	1850	rBV	602665	765848	71.22%	9.350%
71	12.427	1857	1860	1864	rVB4	1097	1392	0.13%	0.017%
72	12.475	1866	1868	1874	rVB3	675	929	0.09%	0.011%
73	12.536	1875	1878	1879	rVB2	182	146	0.01%	0.002%
74	12.579	1883	1885	1886	rBV	293	191	0.02%	0.002%
75	12.841	1927	1928	1931	rBV2	234	173	0.02%	0.002%
76	13.055	1959	1963	1968	rVB4	574	820	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
 Data File : VX024643.D
 Acq On : 07 Oct 2021 14:08
 Operator : JC/MD
 Sample : M4001-01 100X
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EW916

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
 Title : VOC Analysis

77	13.115	1968	1973	1976	rVB3	924	846	0.08%	0.010%
78	13.298	2000	2003	2004	rVB2	179	165	0.02%	0.002%
79	13.317	2004	2006	2008	rBV2	193	181	0.02%	0.002%
80	13.353	2010	2012	2015	rVB2	152	150	0.01%	0.002%
81	13.524	2037	2040	2041	rBV	229	297	0.03%	0.004%
82	13.591	2048	2051	2054	rVB2	882	876	0.08%	0.011%
83	13.780	2078	2082	2086	rBV2	463	706	0.07%	0.009%
84	13.969	2110	2113	2117	rVB4	549	657	0.06%	0.008%
85	13.999	2117	2118	2120	rVB	302	142	0.01%	0.002%
86	14.085	2129	2132	2135	rBV2	194	264	0.02%	0.003%
87	14.128	2135	2139	2143	rBV2	332	403	0.04%	0.005%
88	14.280	2163	2164	2167	rBV	138	157	0.01%	0.002%
89	14.310	2167	2169	2170	rVB	236	163	0.02%	0.002%
90	14.573	2210	2212	2214	rBV2	262	156	0.01%	0.002%
91	14.646	2223	2224	2227	rBV2	297	198	0.02%	0.002%
92	14.859	2257	2259	2260	rBV	299	167	0.02%	0.002%
93	15.127	2301	2303	2305	rBV2	347	274	0.03%	0.003%
94	15.481	2359	2361	2362	rBV	403	276	0.03%	0.003%
95	15.646	2386	2388	2389	rBV2	426	312	0.03%	0.004%
96	15.798	2411	2413	2418	rBV3	447	746	0.07%	0.009%
97	15.926	2432	2434	2436	rBV2	536	345	0.03%	0.004%
98	15.944	2436	2437	2439	rVB	429	226	0.02%	0.003%
99	16.273	2489	2491	2492	rBV	328	141	0.01%	0.002%
100	16.621	2546	2548	2550	rBV2	536	501	0.05%	0.006%


Sum of corrected areas: 8190852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
Data File : VX024643.D
Acq On : 07 Oct 2021 14:08
Operator : JC/MD
Sample : M4001-01 100X
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

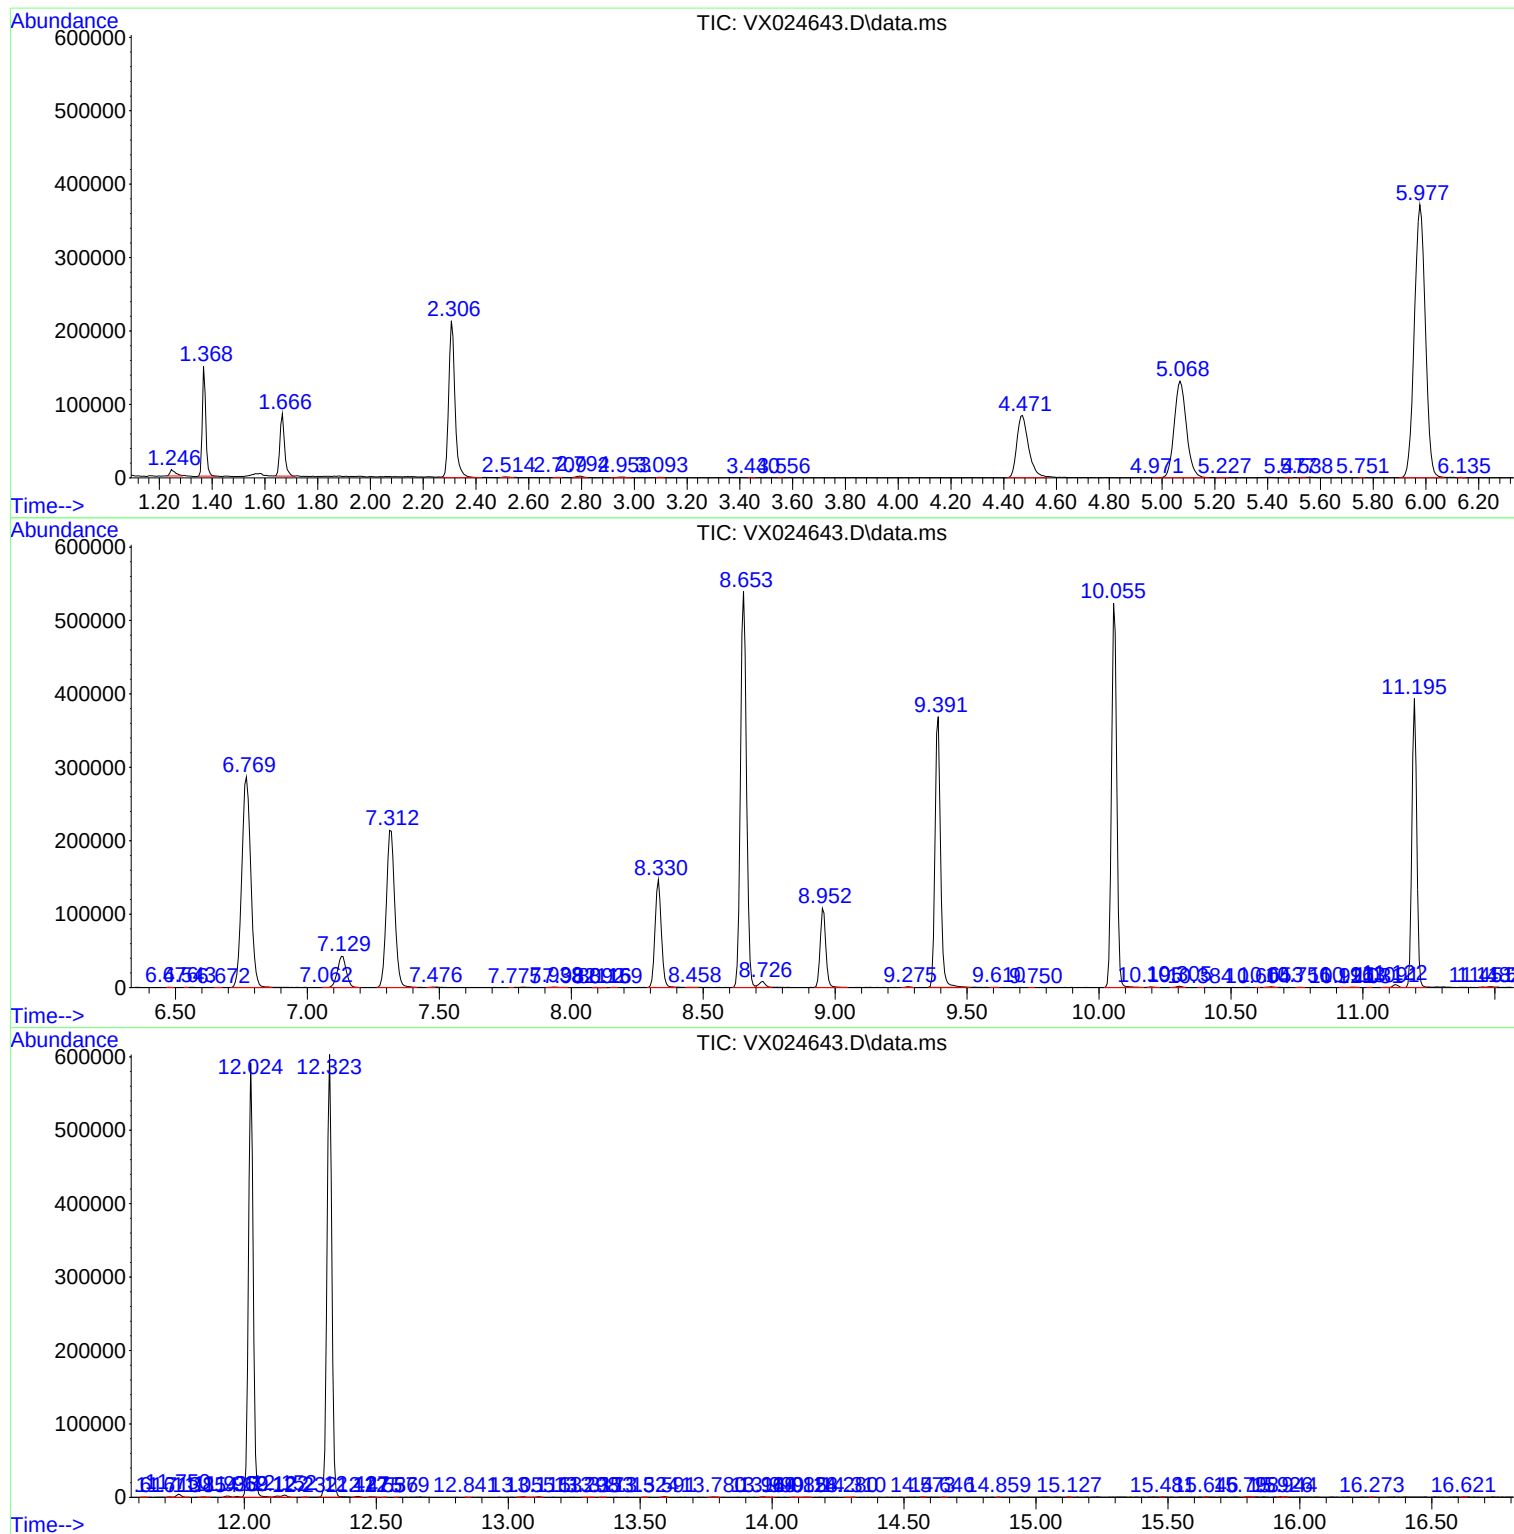

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
Data File : VX024643.D
Acq On : 07 Oct 2021 14:08
Operator : JC/MD
Sample : M4001-01 100X
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
Data File : VX024643.D
Acq On : 07 Oct 2021 14:08
Operator : JC/MD
Sample : M4001-01 100X
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EW916

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML100721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc