
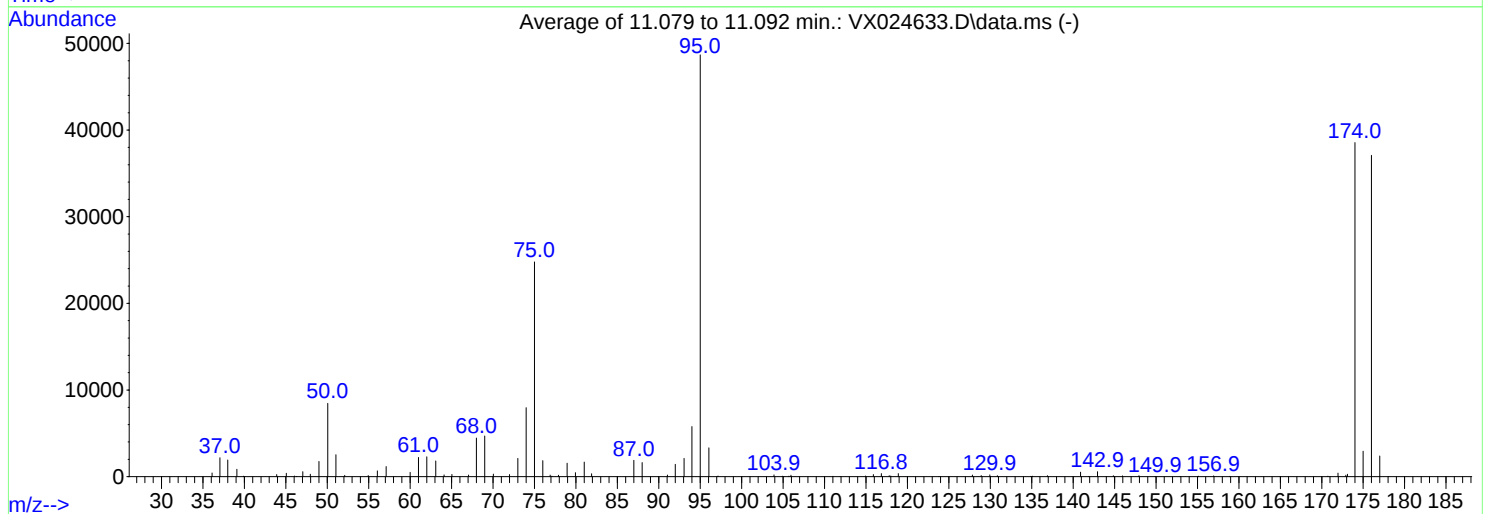


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100721\
 Data File : VX024633.D
 Acq On : 07 Oct 2021 09:00
 Operator : JC/MD
 Sample : BFB603
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB603

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM100721WMA.M
 Title : VOC Analysis
 Last Update : Mon Oct 18 01:29:23 2021

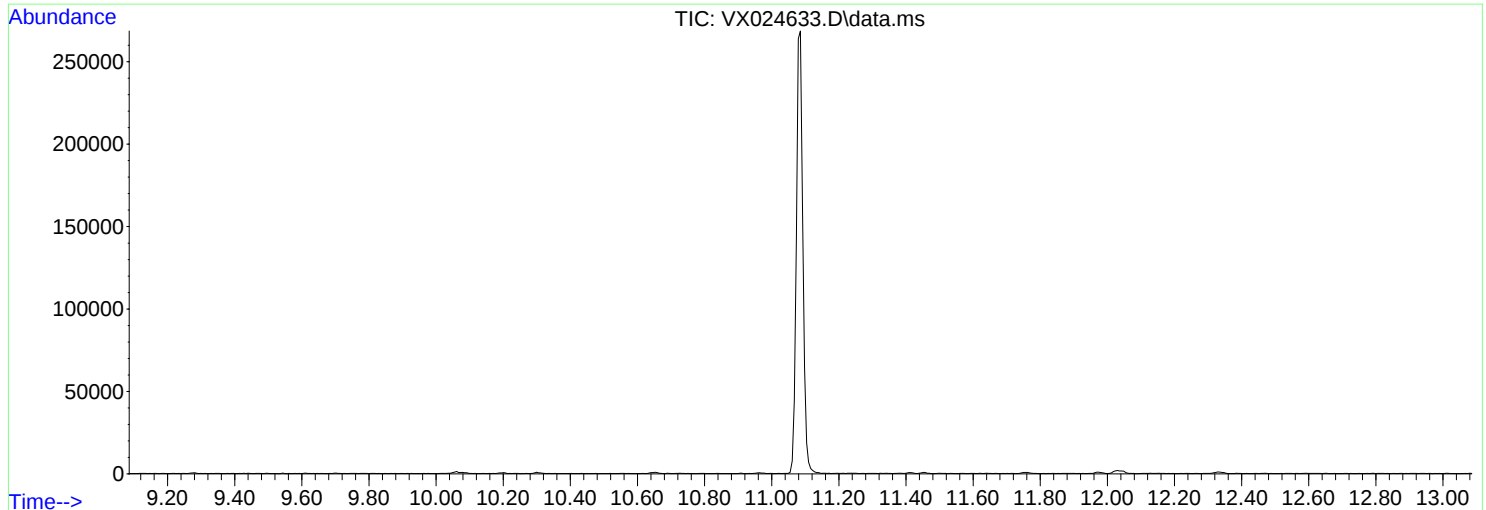

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	8466	PASS
75	95	30	80	50.9	24781	PASS
95	95	100	100	100.0	48683	PASS
96	95	5	9	6.8	3322	PASS
173	174	0.00	2	0.7	285	PASS
174	95	50	120	79.2	38557	PASS
175	174	5	9	7.6	2935	PASS
176	174	95	101	96.2	37080	PASS
177	176	5	9	6.4	2391	PASS

m/z	Abundance
40.10	145.0
44.00	147.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	520.0
37.00	2822.0
38.00	2302.0
39.10	1008.0
39.90	148.0
43.90	392.0
45.00	603.0
46.00	96.0
47.10	586.0
48.00	382.0
49.00	2458.0
50.00	10516.0
51.00	3188.0
52.10	158.0
55.00	135.0
56.10	781.0
57.10	1520.0
60.00	504.0
61.00	2700.0
62.00	2733.0
63.10	2047.0
64.00	262.0
65.10	259.0
67.10	176.0
68.00	5328.0
69.00	5669.0
70.00	287.0
72.10	273.0
73.00	2639.0
74.00	9886.0
75.00	29872.0
76.00	2340.0
76.90	305.0
77.90	189.0
79.00	1833.0
79.90	520.0
81.00	1911.0
81.90	424.0
87.00	2254.0
88.00	1843.0
91.00	203.0
92.00	1563.0
93.00	2494.0
94.00	6810.0
95.00	56704.0
96.10	4082.0
97.20	110.0
103.90	233.0
104.90	104.0
105.90	217.0
111.00	70.0
114.90	104.0
116.00	319.0
116.90	438.0
117.80	225.0
118.90	437.0
127.80	168.0
128.90	177.0
129.90	267.0
130.90	126.0
134.90	93.0
136.90	148.0
140.90	436.0
141.90	117.0
142.90	662.0
144.00	52.0
144.80	151.0
145.90	79.0
147.90	100.0
155.10	93.0
156.90	65.0
172.00	472.0
172.90	497.0
174.00	39608.0
175.00	3152.0
176.00	39016.0
177.00	2492.0
178.10	86.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.10	509.0
37.10	2644.0
38.00	2147.0
39.10	1013.0
40.10	141.0
43.90	512.0
45.10	385.0
46.10	115.0
47.00	802.0
47.90	353.0
49.00	1894.0
50.10	9608.0
51.10	2877.0
52.10	203.0
54.90	133.0
56.00	796.0
57.10	1342.0
60.00	646.0
61.00	2631.0
62.00	2571.0
63.10	2122.0
64.10	222.0
65.00	261.0
67.00	192.0
68.00	5096.0
69.00	5403.0
70.10	455.0
71.90	327.0
73.00	2352.0
74.00	8871.0
75.00	28696.0
76.00	1947.0
76.90	250.0
77.90	159.0
78.90	1744.0
80.00	435.0
81.00	2025.0
81.80	362.0
87.00	2292.0
88.00	2007.0
91.10	203.0
92.00	1757.0
93.10	2480.0
94.00	6657.0
95.00	56744.0
96.00	3818.0
97.10	99.0
103.90	262.0
104.90	73.0
106.00	312.0
111.00	62.0
111.90	68.0
115.00	57.0
115.90	233.0
116.80	412.0
118.00	227.0
118.90	418.0
127.80	244.0
128.90	136.0
130.00	150.0
130.80	105.0
135.10	109.0
136.90	122.0
140.90	640.0
143.00	644.0
144.90	133.0
145.90	100.0
148.00	94.0
155.10	102.0
156.90	134.0
158.90	54.0
170.70	65.0
171.90	456.0
173.10	478.0
174.00	45344.0
175.00	3425.0
176.00	42904.0
177.00	2770.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603

m/z	Abundance
36.00	273.0
37.00	1059.0
38.00	1315.0
39.00	517.0
40.10	116.0
44.00	246.0
45.10	188.0
46.30	62.0
47.10	345.0
47.80	127.0
49.00	894.0
50.00	5275.0
51.10	1540.0
52.10	82.0
54.90	102.0
56.00	445.0
57.00	641.0
59.90	369.0
61.00	1331.0
62.00	1579.0
63.00	1258.0
64.20	133.0
65.10	229.0
67.00	187.0
68.00	2928.0
69.10	2986.0
70.10	132.0
72.00	139.0
73.00	1340.0
74.00	5125.0
75.00	15776.0
76.00	1246.0
77.10	164.0
77.90	130.0
78.90	1096.0
80.00	443.0
80.90	1080.0
82.00	230.0
87.00	1081.0
88.00	1036.0
91.00	165.0
92.00	927.0
93.00	1335.0
94.00	3892.0
95.10	32600.0
96.10	2065.0
104.00	98.0
105.10	54.0
105.70	143.0
115.00	50.0
115.80	171.0
116.80	232.0
117.80	110.0
118.90	191.0
123.80	58.0
127.90	173.0
128.80	83.0
130.00	215.0
130.80	99.0
135.10	85.0
136.90	52.0
140.90	505.0
142.90	422.0
145.00	56.0
146.00	87.0
148.00	142.0
149.90	70.0
152.90	50.0
157.00	86.0
158.90	51.0
170.80	81.0
172.00	317.0
173.10	376.0
174.00	30720.0
175.00	2229.0
176.00	29320.0
177.00	1911.0

Instrument :
MSVOA_X
ClientSampleId :
BFB603