

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100722\
 Data File : VX031954.D
 Acq On : 07 Oct 2022 12:06
 Operator : JC/MD
 Sample : N4925-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Oct 08 05:09:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 06 14:28:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	59470	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	94628	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	99492	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	63267	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	62404	50.810	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	101.620%
35) Dibromofluoromethane	5.385	113	52531	49.042	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.080%
50) Toluene-d8	8.647	98	188990	49.033	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.060%
62) 4-Bromofluorobenzene	11.079	95	65552	48.108	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	96.220%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100722\
Data File : VX031954.D
Acq On : 07 Oct 2022 12:06
Operator : JC/MD
Sample : N4925-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Oct 08 05:09:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 06 14:28:46 2022
Response via : Initial Calibration




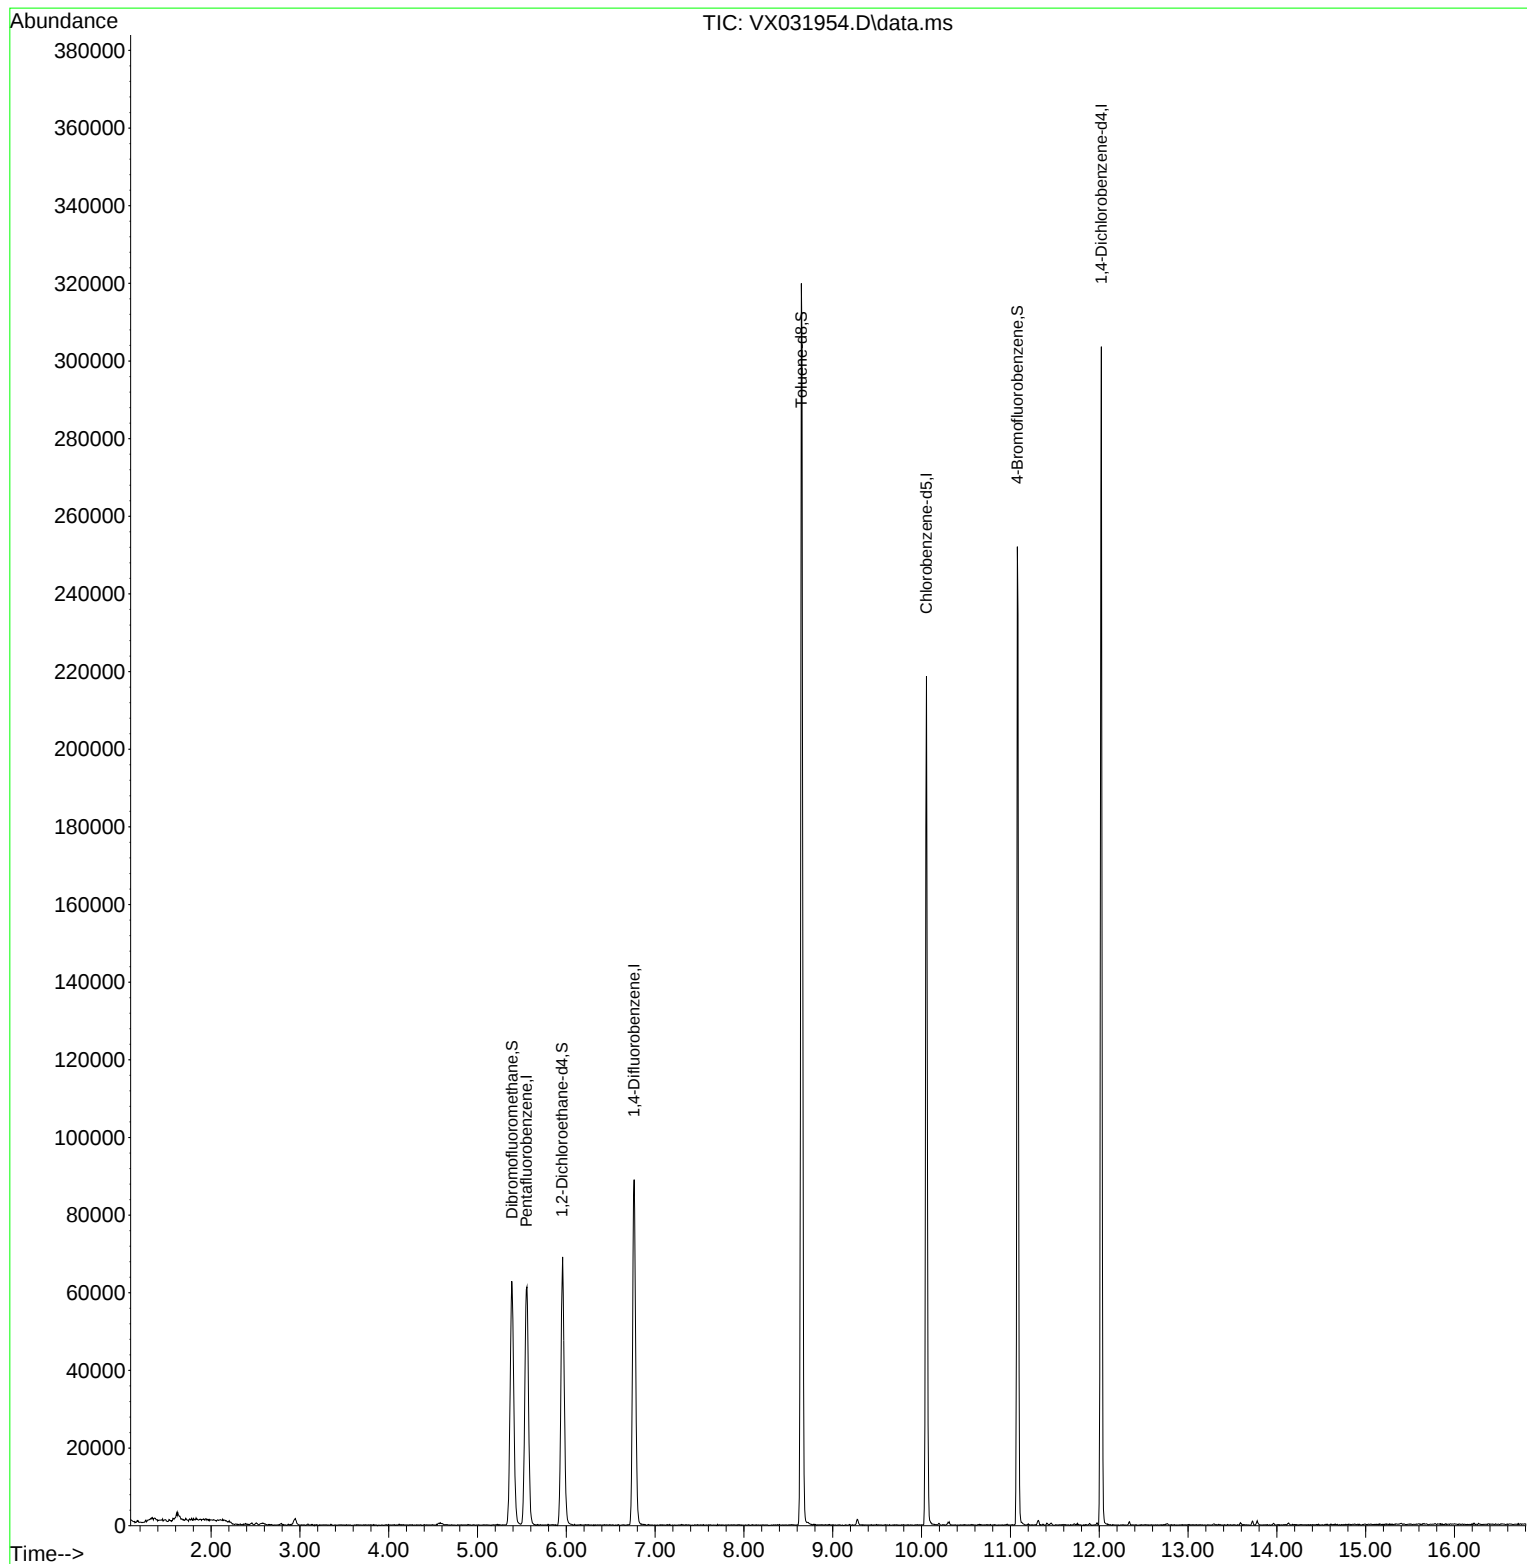


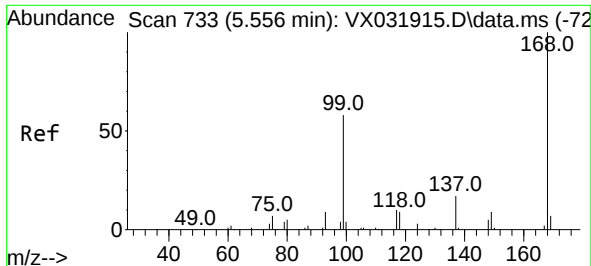

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 59470
Ion Ratio Lower Upper
168 100
99 54.6 48.8 73.2

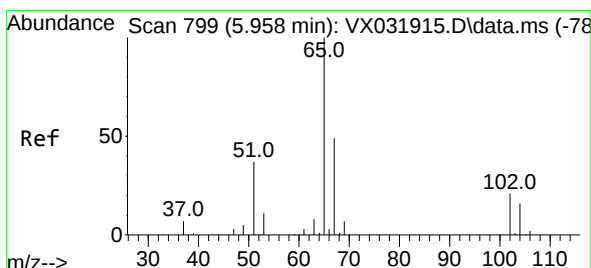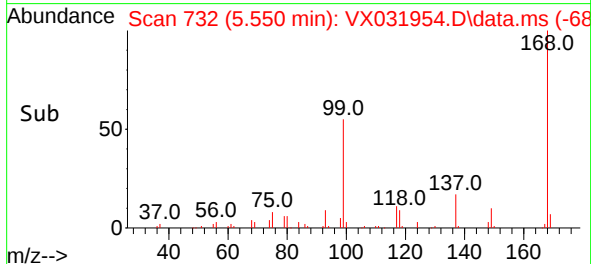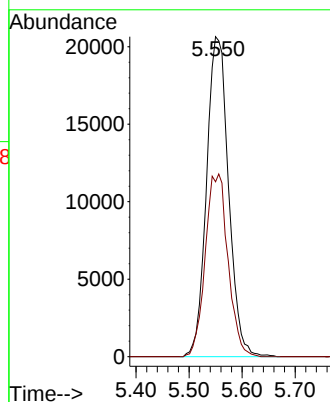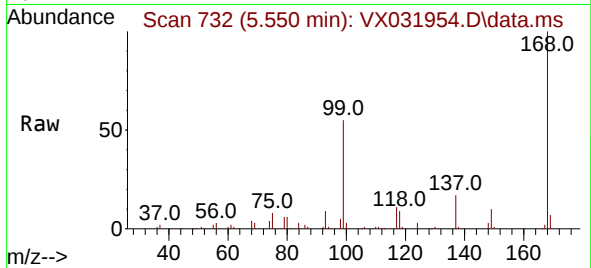

#33
1,2-Dichloroethane-d4
Concen: 50.810 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06

Tgt Ion: 65 Resp: 62404
Ion Ratio Lower Upper
65 100
67 51.8 0.0 102.4


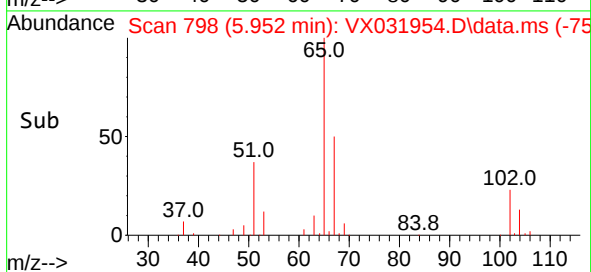
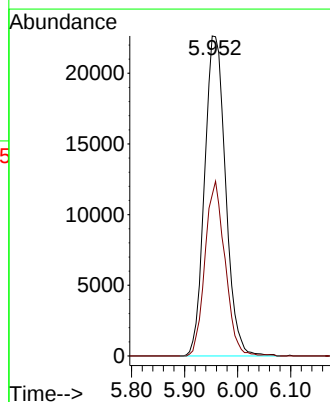
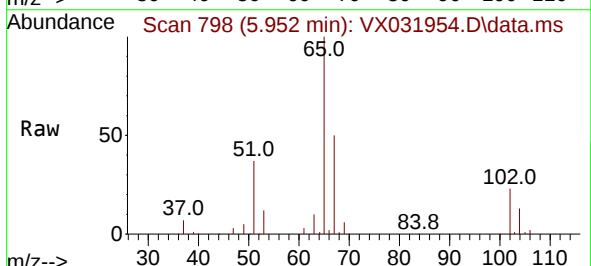


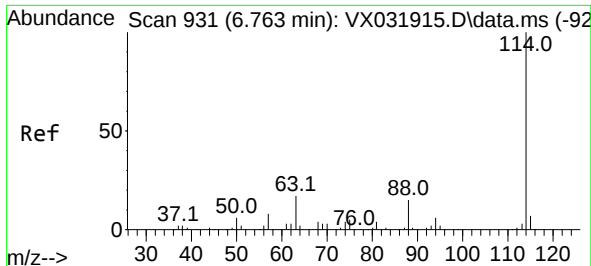

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 94628
Ion Ratio Lower Upper
114 100
63 19.5 0.0 42.6
88 15.9 0.0 33.0

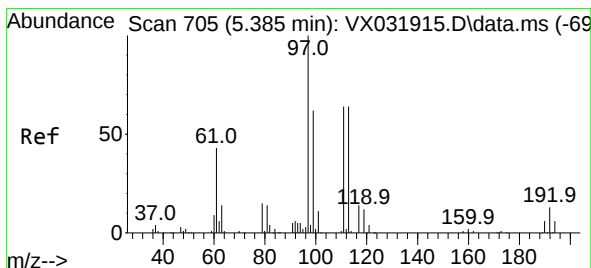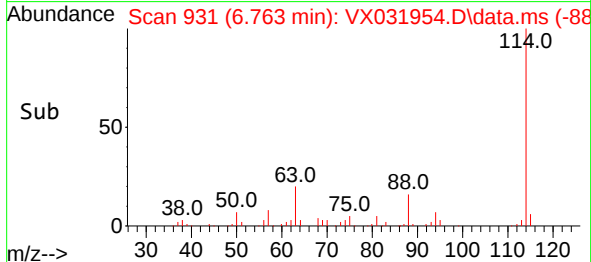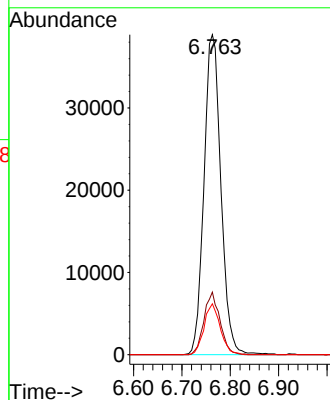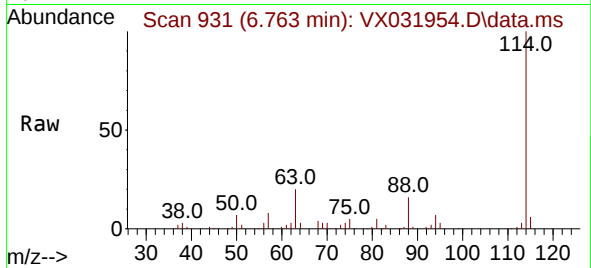

#35
Dibromofluoromethane
Concen: 49.042 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06

Tgt Ion:113 Resp: 52531
Ion Ratio Lower Upper
113 100
111 103.7 82.4 123.6
192 19.3 14.1 21.1


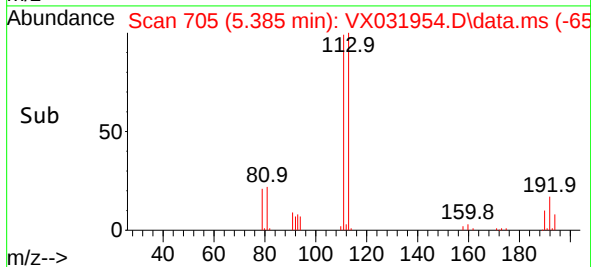
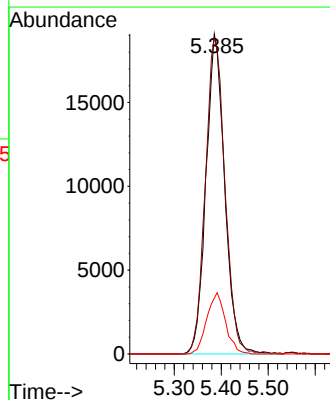
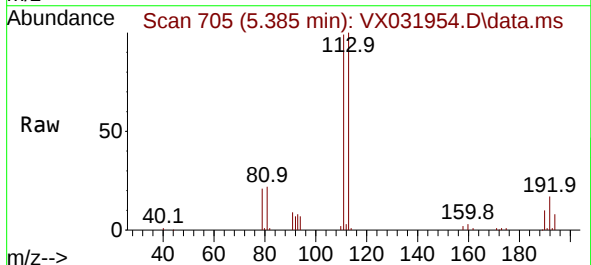


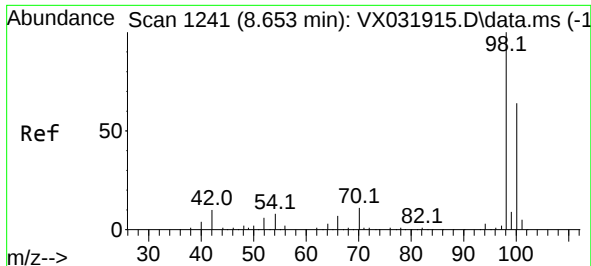

#50
Toluene-d8
Concen: 49.033 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 188990
Ion Ratio Lower Upper
98 100
100 66.2 52.5 78.7

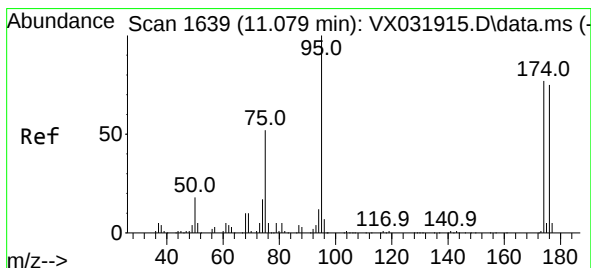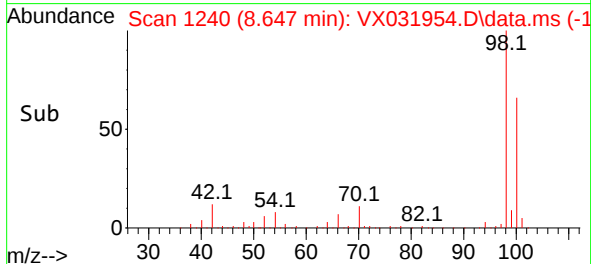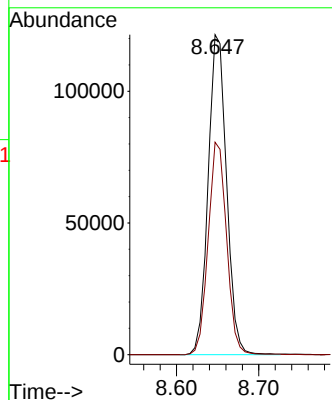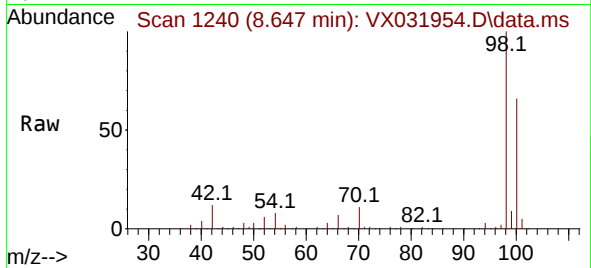

#62
4-Bromofluorobenzene
Concen: 48.108 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06

Tgt Ion: 95 Resp: 65552
Ion Ratio Lower Upper
95 100
174 79.7 0.0 153.2
176 76.7 0.0 144.0


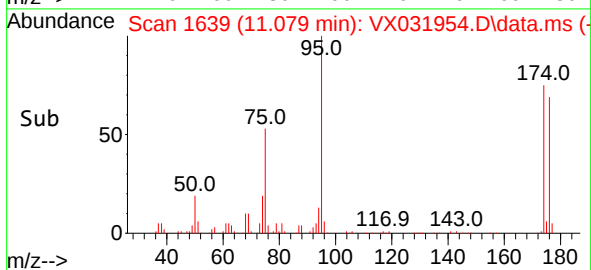
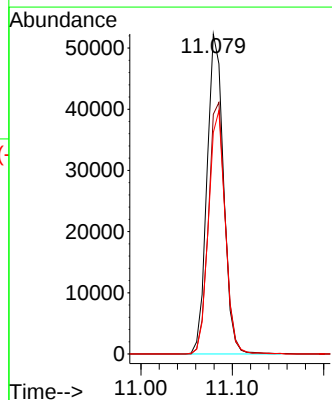
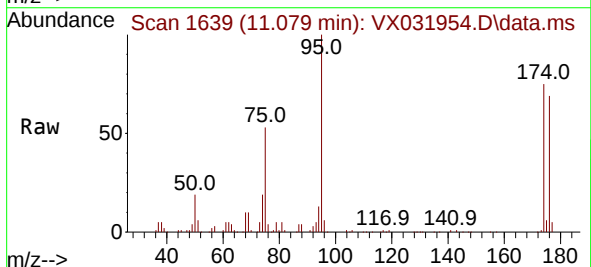


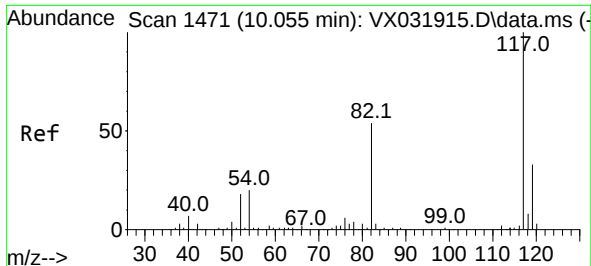

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 99492
Ion Ratio Lower Upper
117 100
82 52.9 46.8 70.2
119 32.6 26.4 39.6

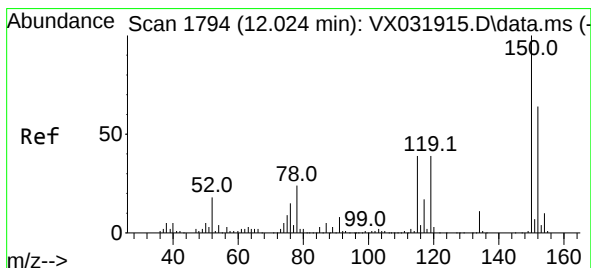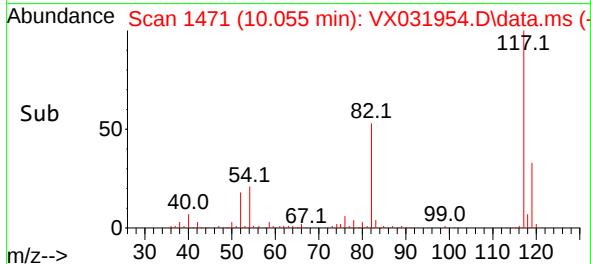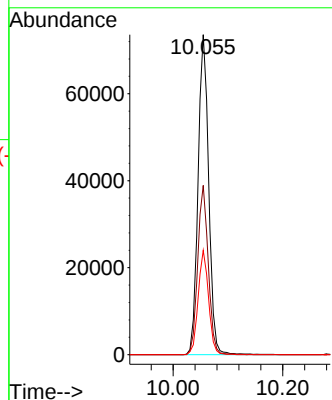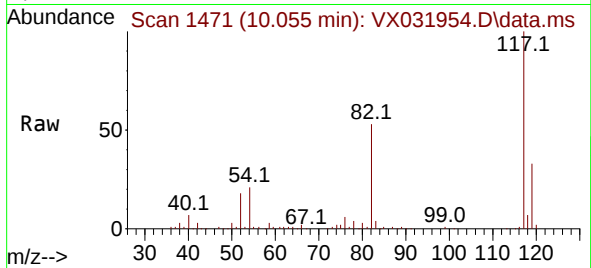

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031954.D
Acq: 07 Oct 2022 12:06

Tgt Ion:152 Resp: 63267
Ion Ratio Lower Upper
152 100
115 57.7 43.4 130.1
150 153.9 0.0 346.8

