

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100722\
 Data File : VX031967.D
 Acq On : 07 Oct 2022 17:08
 Operator : JC/MD
 Sample : N4882-20 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-132

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX031967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	295	305	308	rBV2	7693	17483	3.53%	0.714%
2	3.111	323	332	345	rVB	85548	197973	40.00%	8.086%
3	5.391	694	706	722	rBV2	62072	180668	36.51%	7.379%
4	5.556	722	733	746	rVB2	61625	171703	34.69%	7.013%
5	5.958	789	799	813	rBV	67021	179355	36.24%	7.326%
6	6.330	851	860	871	rBV4	4275	12145	2.45%	0.496%
7	6.763	922	931	943	rBV	90186	211481	42.73%	8.638%
8	8.647	1234	1240	1249	rBV	313349	494909	100.00%	20.214%
9	10.055	1465	1471	1485	rBV	220458	292618	59.13%	11.952%
10	11.079	1634	1639	1655	rVB	246858	318387	64.33%	13.004%
11	12.024	1789	1794	1804	rVB	293885	371602	75.08%	15.178%




Sum of corrected areas: 2448324

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100722\
Data File : VX031967.D
Acq On : 07 Oct 2022 17:08
Operator : JC/MD
Sample : N4882-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

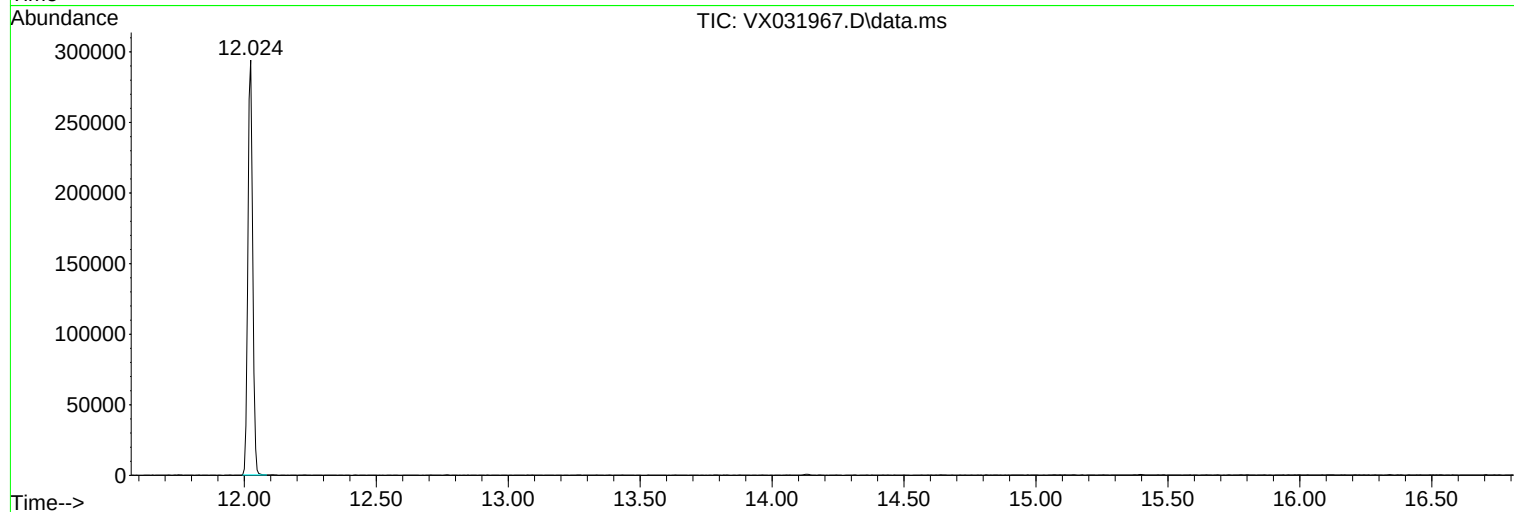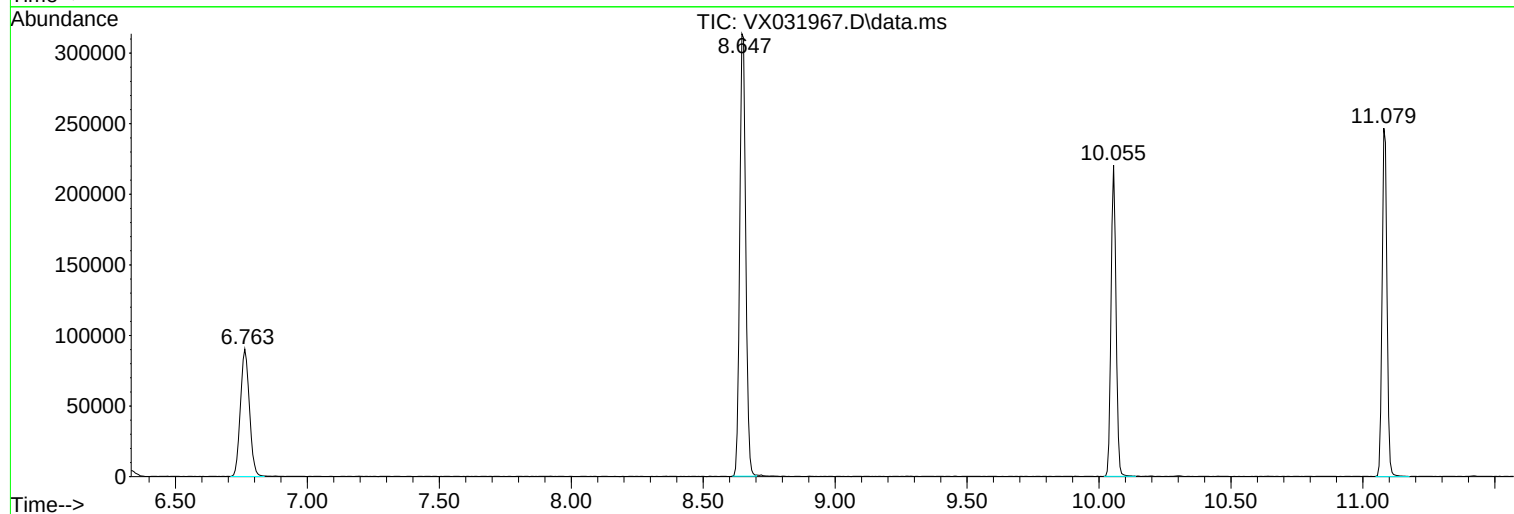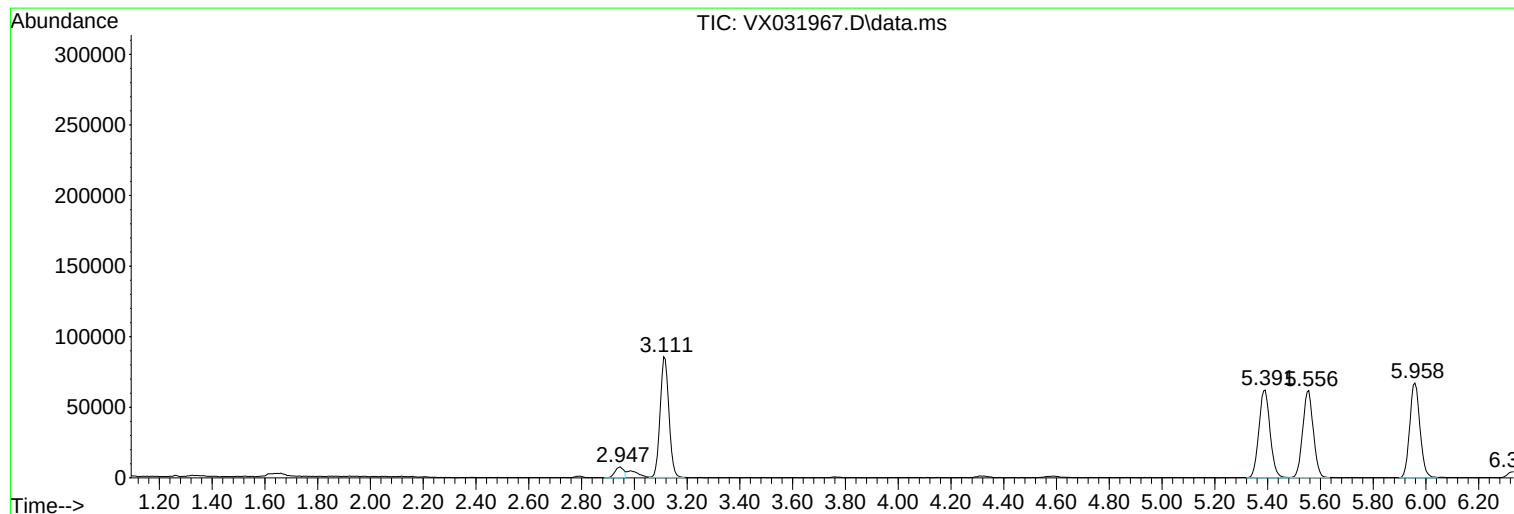

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100722\
Data File : VX031967.D
Acq On : 07 Oct 2022 17:08
Operator : JC/MD
Sample : N4882-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100722\
Data File : VX031967.D
Acq On : 07 Oct 2022 17:08
Operator : JC/MD
Sample : N4882-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------