

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100722\  
Data File : VX031972.D  
Acq On : 07 Oct 2022 19:04  
Operator : JC/MD  
Sample : N4883-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-137

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100622W.M

Title : SW846 8260

Signal : TIC: VX031972.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.111       | 322           | 332         | 347          | rVB      | 105113         | 240175        | 53.65%          | 10.692%       |
| 2         | 5.385       | 695           | 705         | 722          | rBV      | 56236          | 162568        | 36.32%          | 7.237%        |
| 3         | 5.550       | 722           | 732         | 744          | rVV      | 53196          | 150746        | 33.68%          | 6.711%        |
| 4         | 5.958       | 790           | 799         | 813          | rBV      | 63183          | 162574        | 36.32%          | 7.238%        |
| 5         | 6.324       | 851           | 859         | 871          | rVB4     | 2520           | 7173          | 1.60%           | 0.319%        |
| 6         | 6.763       | 922           | 931         | 949          | rVB      | 81179          | 189822        | 42.41%          | 8.451%        |
| 7         | 8.647       | 1234          | 1240        | 1257         | rBV      | 278701         | 447639        | 100.00%         | 19.928%       |
| 8         | 10.055      | 1465          | 1471        | 1485         | rBV      | 200295         | 266084        | 59.44%          | 11.846%       |
| 9         | 11.079      | 1634          | 1639        | 1650         | rBV      | 221984         | 284620        | 63.58%          | 12.671%       |
| 10        | 12.024      | 1788          | 1794        | 1802         | rBV      | 268085         | 334866        | 74.81%          | 14.908%       |




Sum of corrected areas: 2246267

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100722\  
Data File : VX031972.D  
Acq On : 07 Oct 2022 19:04  
Operator : JC/MD  
Sample : N4883-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

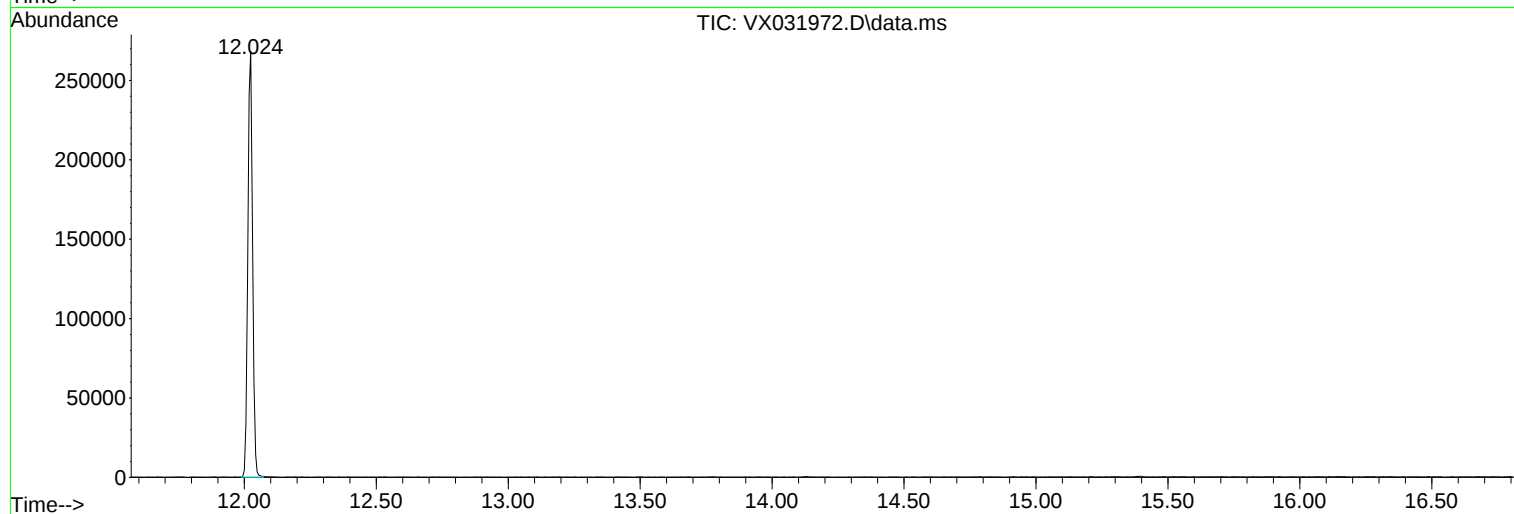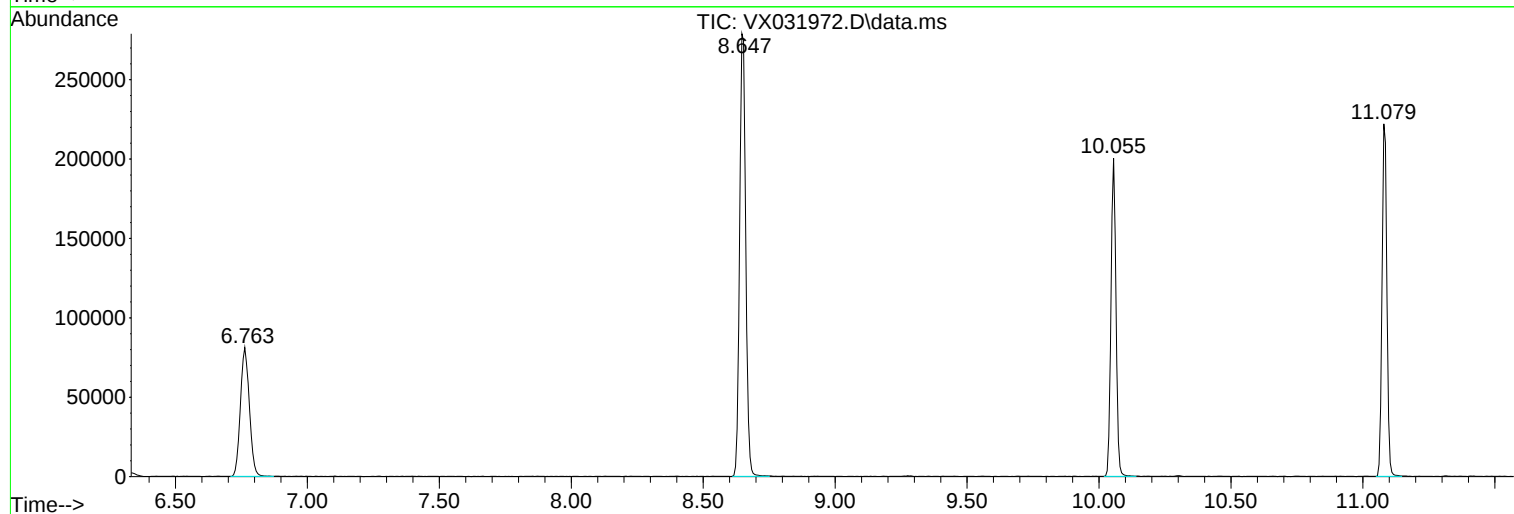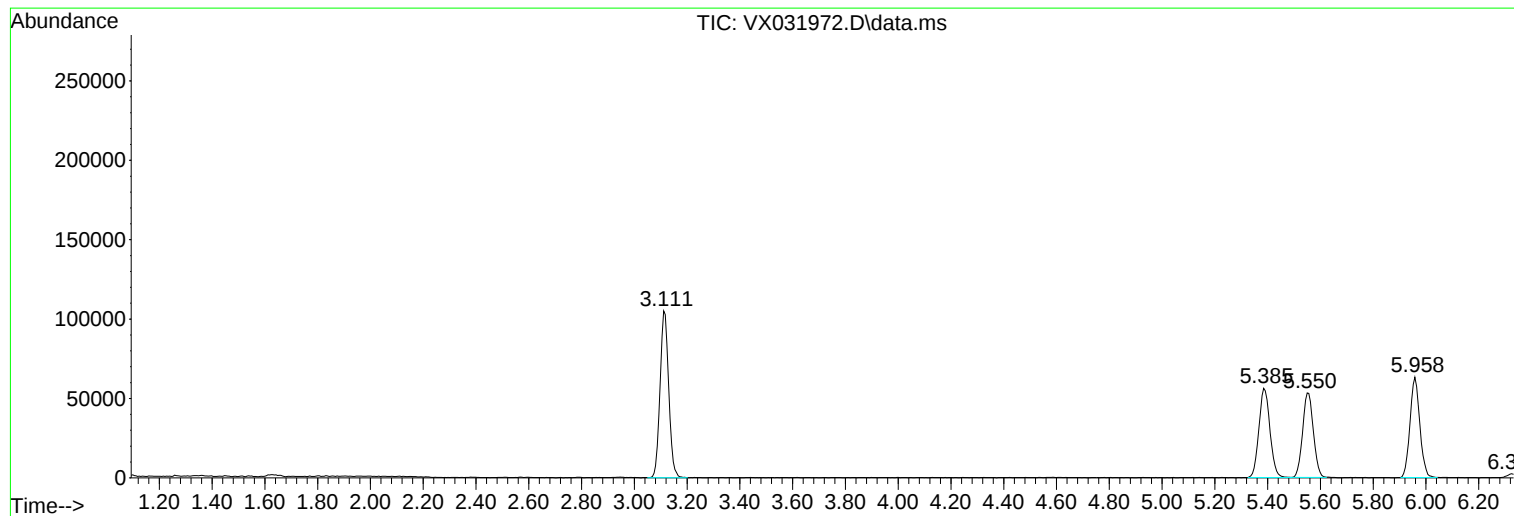

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100722\  
Data File : VX031972.D  
Acq On : 07 Oct 2022 19:04  
Operator : JC/MD  
Sample : N4883-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX100722\  
Data File : VX031972.D  
Acq On : 07 Oct 2022 19:04  
Operator : JC/MD  
Sample : N4883-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-137

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X100622W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|