

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100724\
 Data File : VX043300.D
 Acq On : 07 Oct 2024 09:32
 Operator : JC/MD
 Sample : VX1007WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1007WBL01

Quant Time: Oct 08 01:40:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 02 16:50:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	90256	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	168477	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	147650	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	61464	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	76288	51.755	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	103.520%
35) Dibromofluoromethane	5.379	113	57322	49.335	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.680%
50) Toluene-d8	8.647	98	203384	50.512	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.020%
62) 4-Bromofluorobenzene	11.079	95	73028	49.924	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	99.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100724\
Data File : VX043300.D
Acq On : 07 Oct 2024 09:32
Operator : JC/MD
Sample : VX1007WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1007WBL01

Quant Time: Oct 08 01:40:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Quant Title : SW846 8260
QLast Update : Wed Oct 02 16:50:57 2024
Response via : Initial Calibration




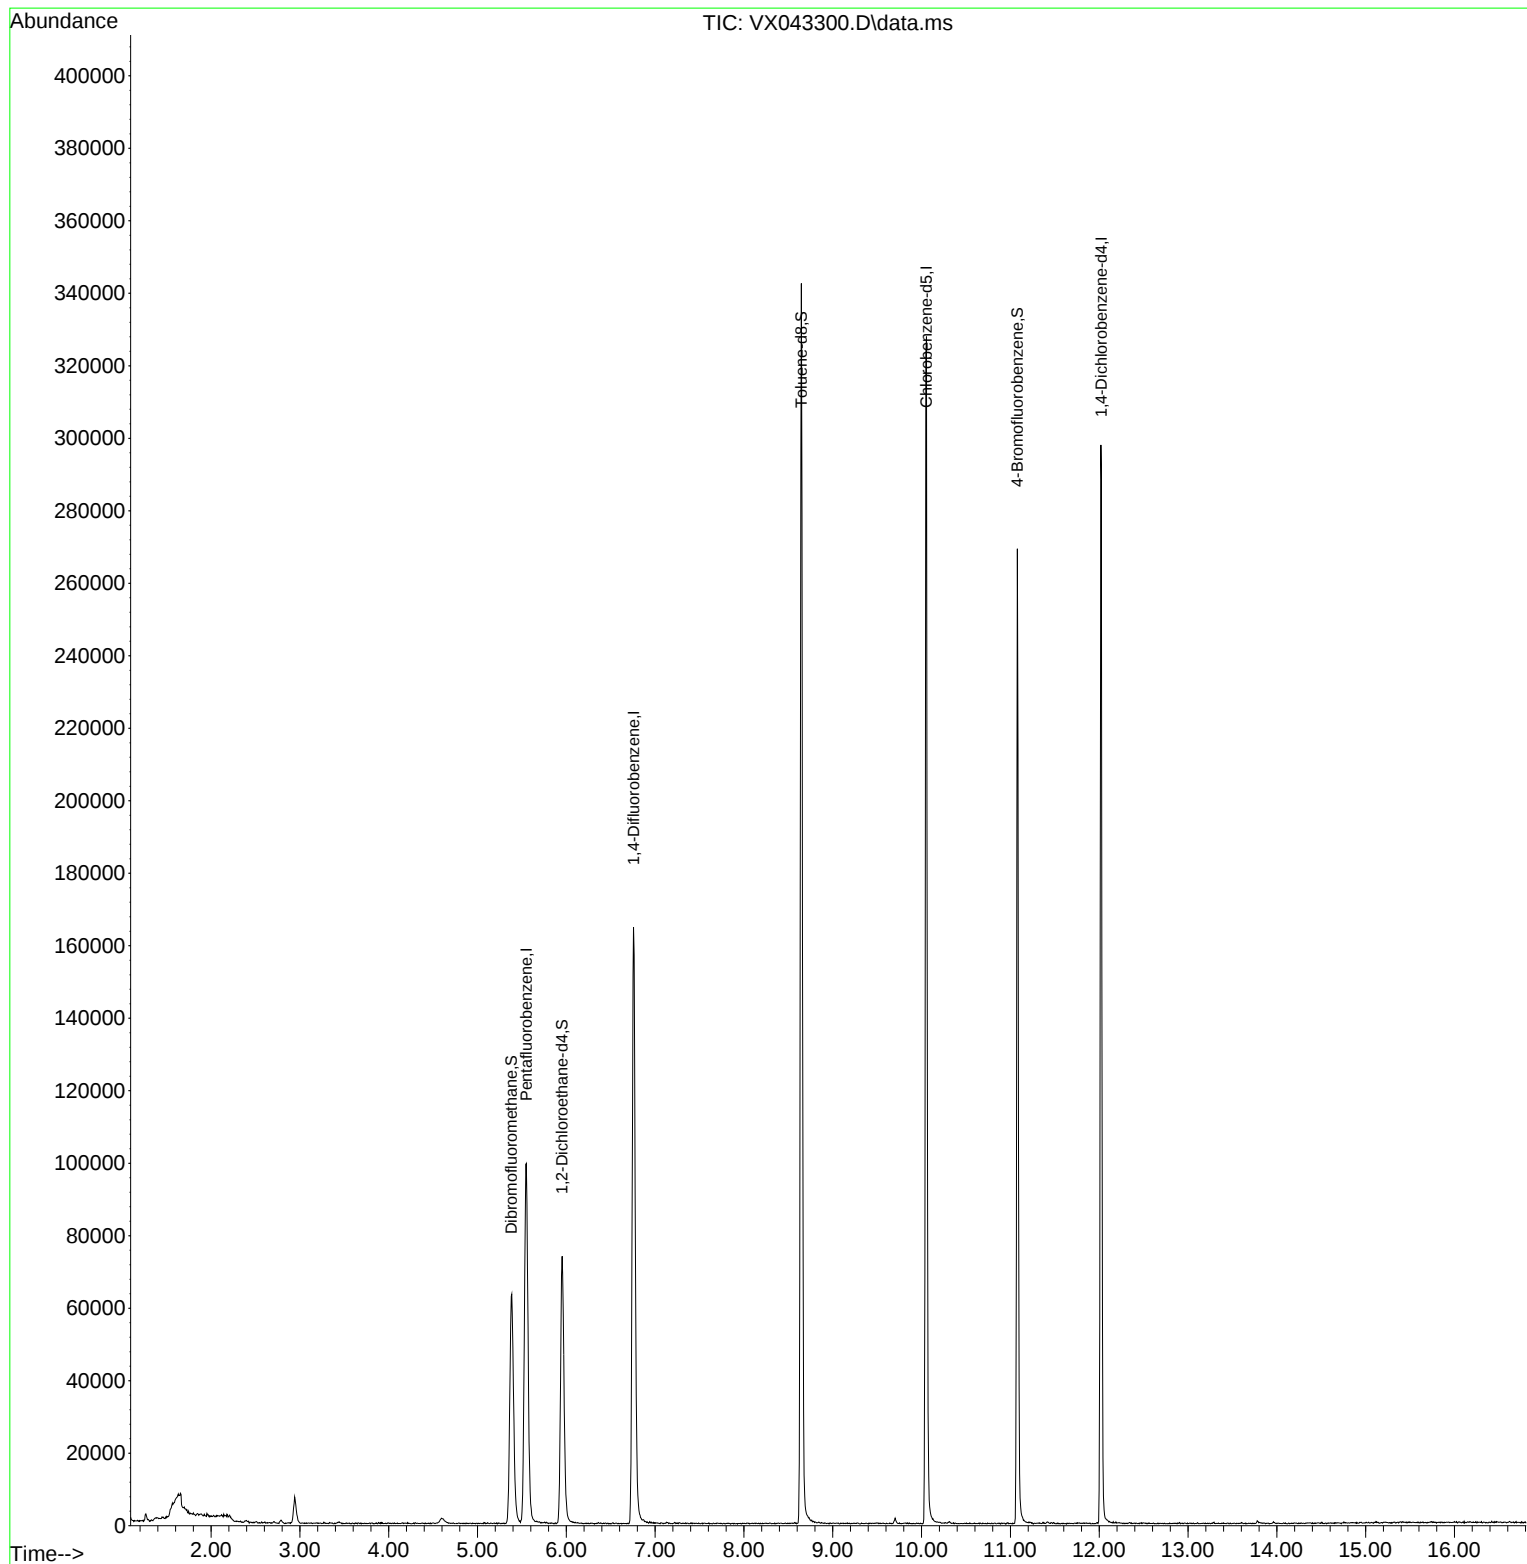


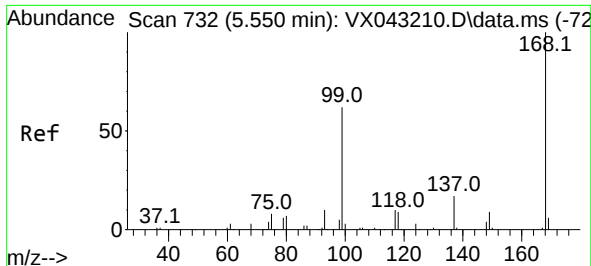

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32




Instrument :
MSVOA_X
ClientSampleId :
VX1007WBL01


Tgt Ion:168 Resp: 90256
Ion Ratio Lower Upper
168 100
99 63.5 49.7 74.5

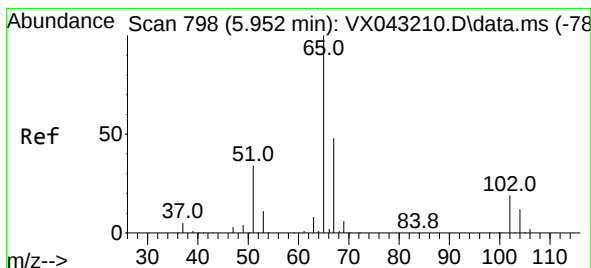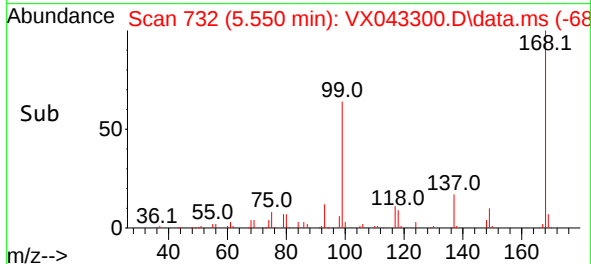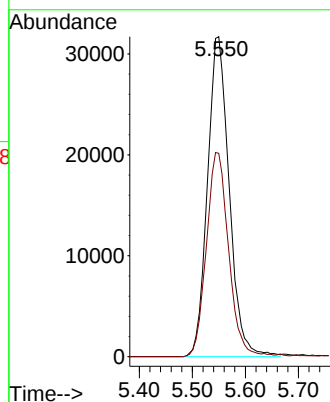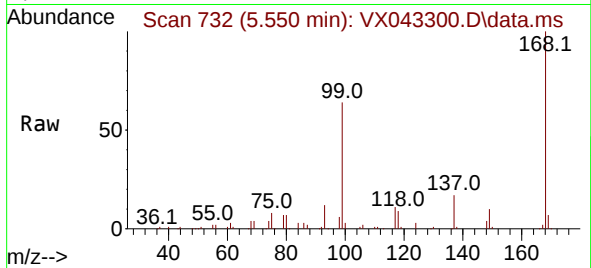

#33
1,2-Dichloroethane-d4
Concen: 51.755 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32

Tgt Ion: 65 Resp: 76288
Ion Ratio Lower Upper
65 100
67 48.8 0.0 99.0


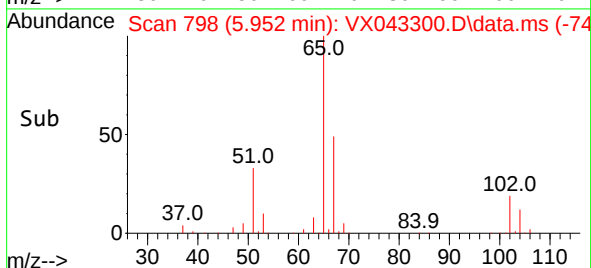
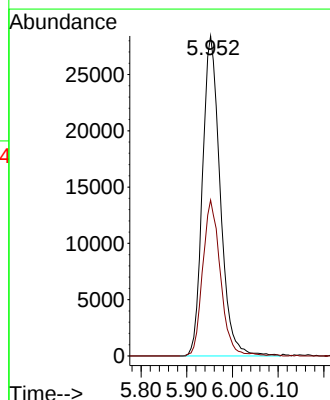
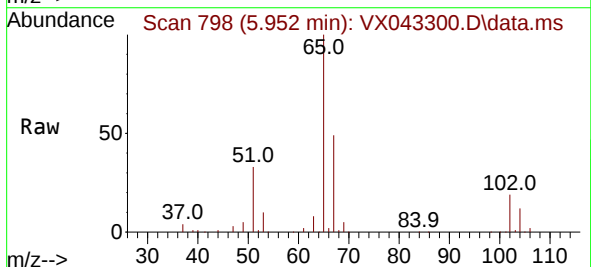


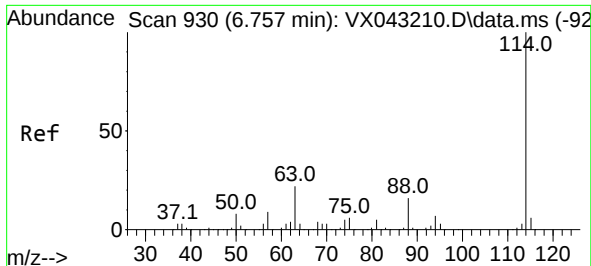

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32




Instrument :
MSVOA_X
ClientSampleId :
VX1007WBL01


Tgt Ion:114 Resp: 168477
Ion Ratio Lower Upper
114 100
63 21.2 0.0 43.0
88 15.7 0.0 33.0

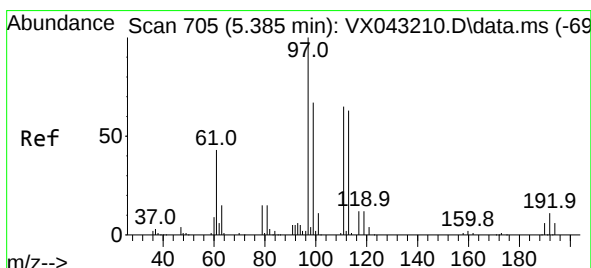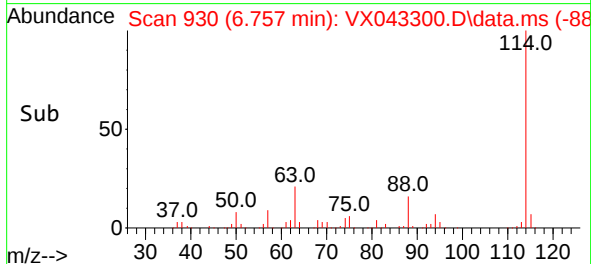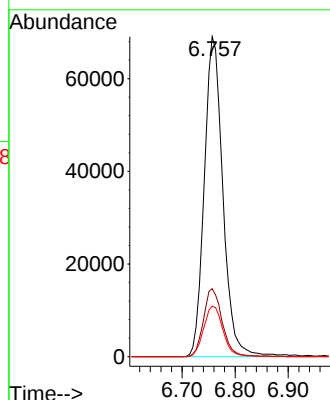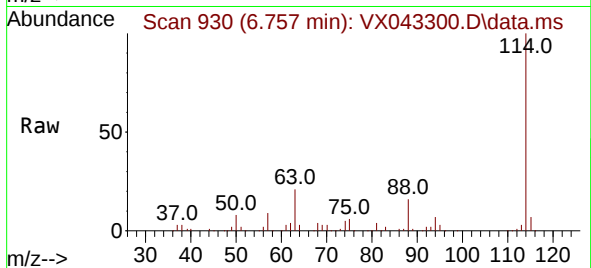

#35
Dibromofluoromethane
Concen: 49.335 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32

Tgt Ion:113 Resp: 57322
Ion Ratio Lower Upper
113 100
111 100.6 83.4 125.0
192 16.9 14.1 21.1


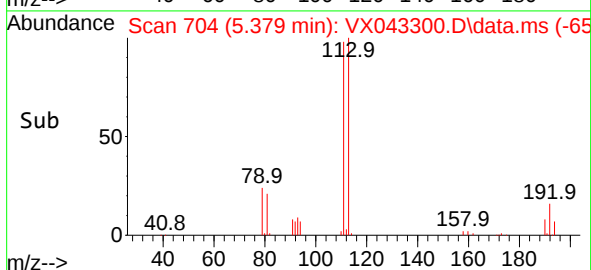
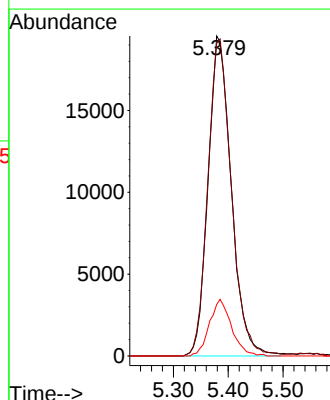
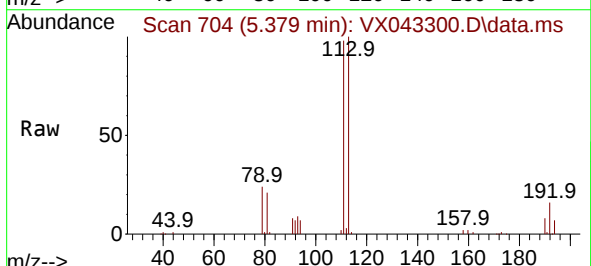


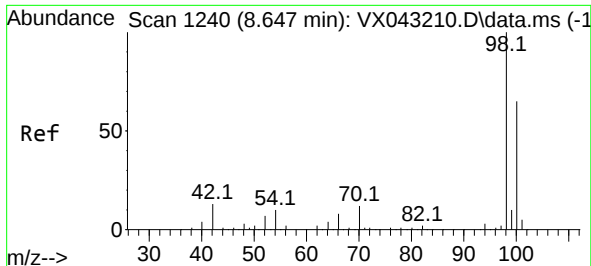

#50
Toluene-d8
Concen: 50.512 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32




Instrument :
MSVOA_X
ClientSampleId :
VX1007WBL01


Tgt Ion: 98 Resp: 203384
Ion Ratio Lower Upper
98 100
100 64.9 52.4 78.6

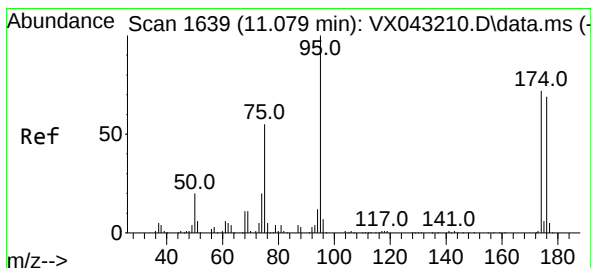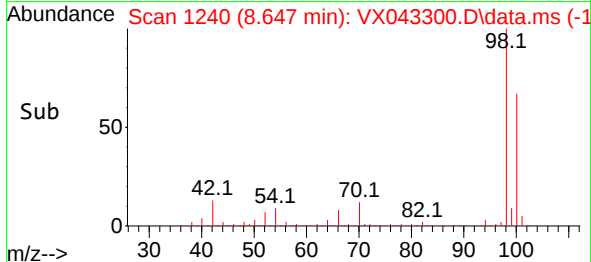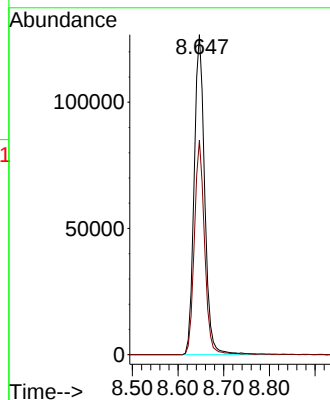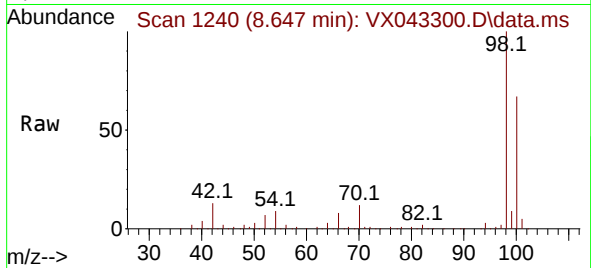

#62
4-Bromofluorobenzene
Concen: 49.924 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32

Tgt Ion: 95 Resp: 73028
Ion Ratio Lower Upper
95 100
174 70.2 0.0 145.0
176 69.1 0.0 143.0


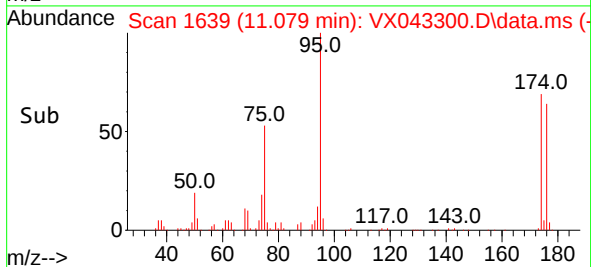
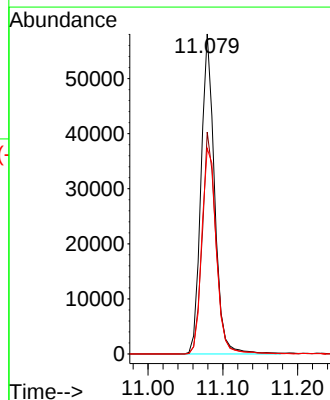
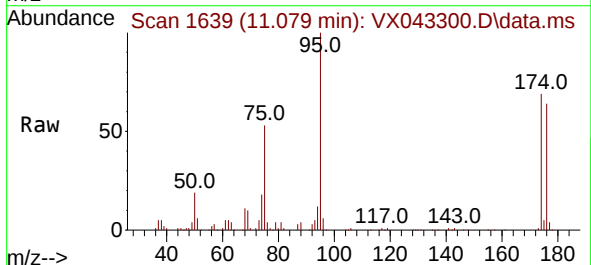


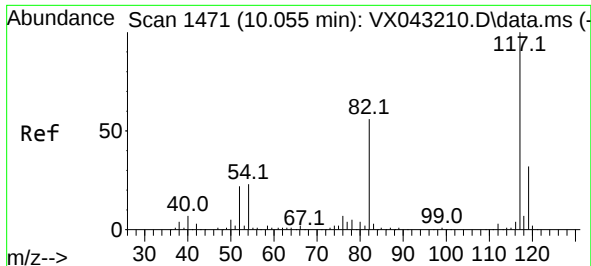

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32

Instrument :
MSVOA_X
ClientSampleId :
VX1007WBL01

Tgt Ion:117 Resp: 147650
Ion Ratio Lower Upper
117 100
82 55.1 45.0 67.6
119 32.0 25.3 37.9

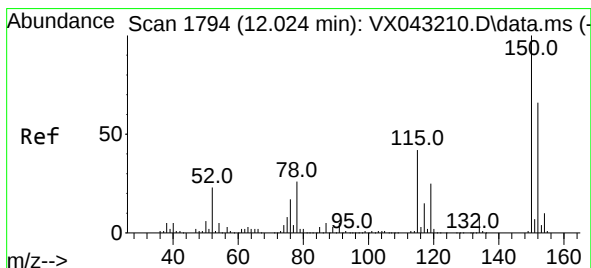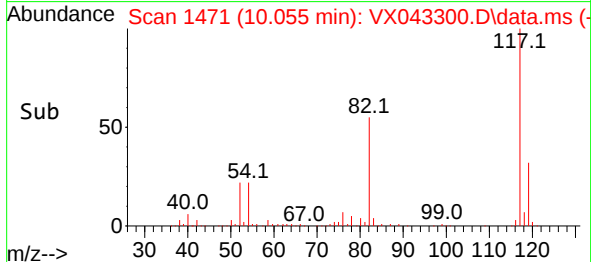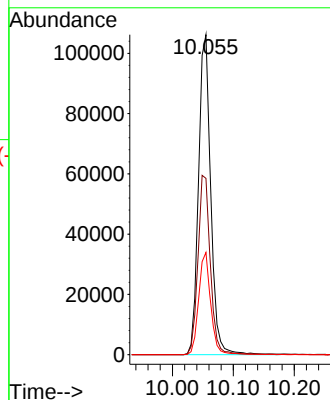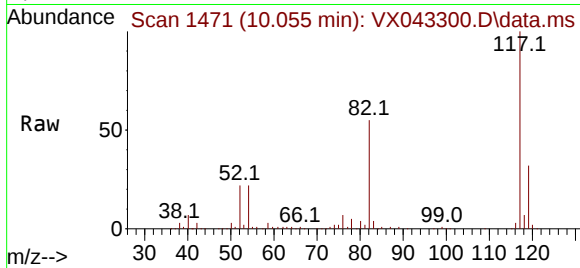

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX043300.D
Acq: 07 Oct 2024 09:32

Tgt Ion:152 Resp: 61464
Ion Ratio Lower Upper
152 100
115 63.0 44.1 132.3
150 160.2 0.0 347.4

