



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100724\
Data File : VX043297.D
Acq On : 07 Oct 2024 07:57
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X100124W.M
Title : SW846 8260
Last Update : Wed Oct 02 16:50:57 2024

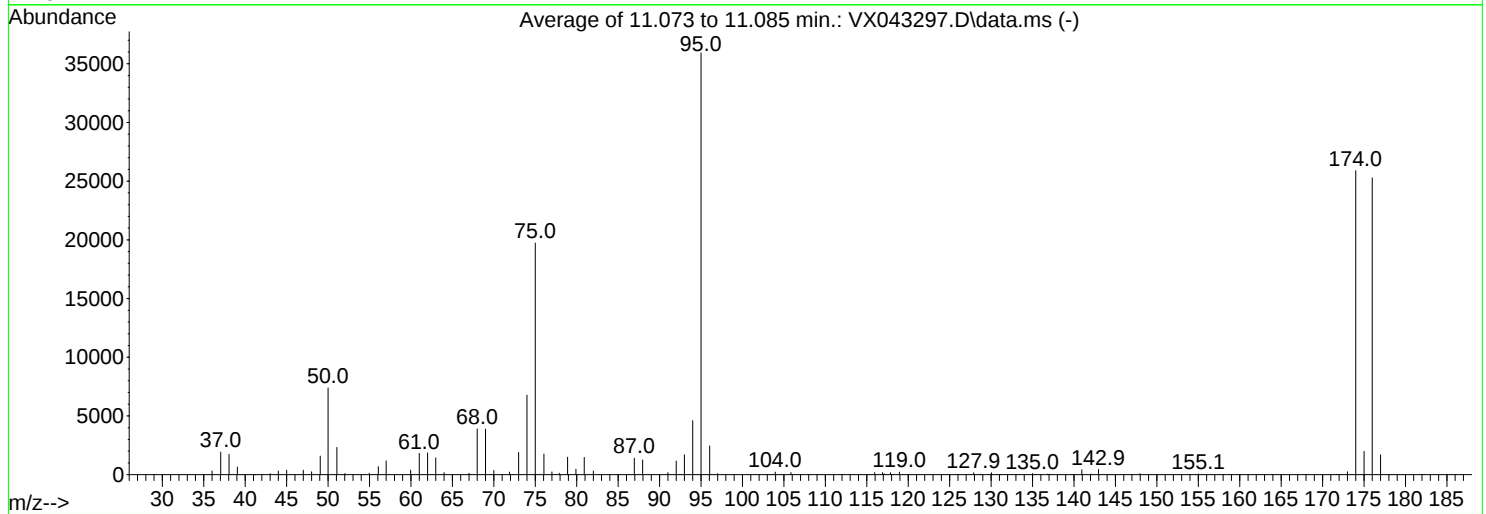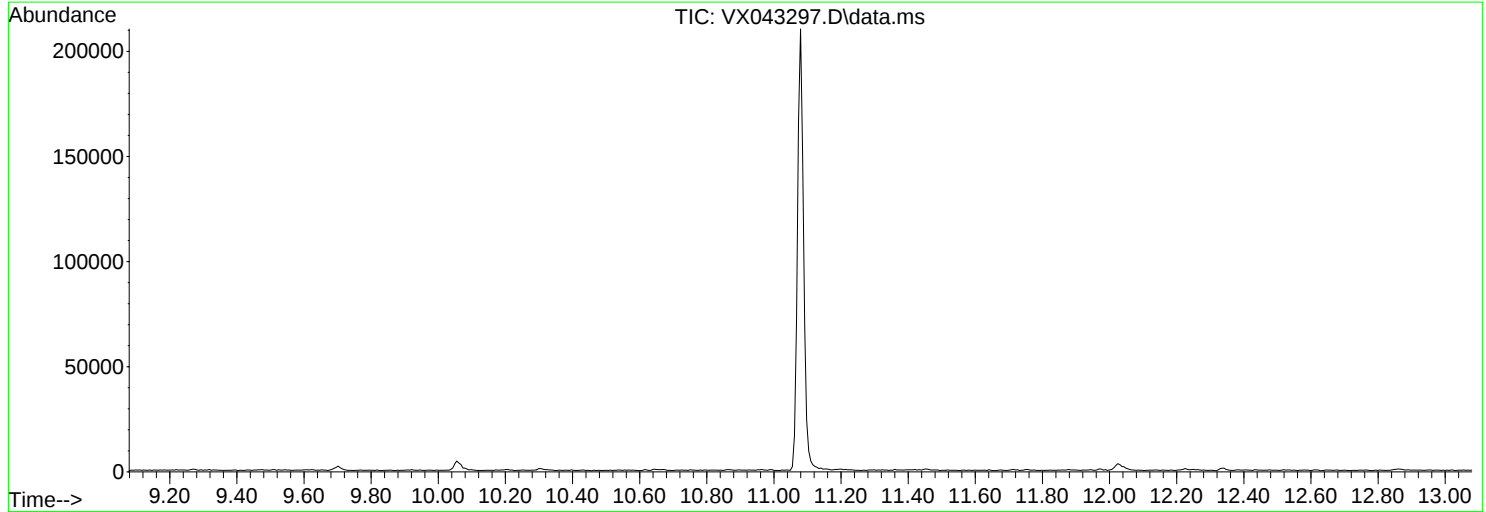

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	7395	PASS
75	95	30	60	54.9	19741	PASS
95	95	100	100	100.0	35931	PASS
96	95	5	9	6.8	2459	PASS
173	174	0.00	2	0.9	245	PASS
174	95	50	100	72.1	25901	PASS
175	174	5	9	7.7	1993	PASS
176	174	95	101	97.6	25288	PASS
177	176	5	9	6.7	1692	PASS