
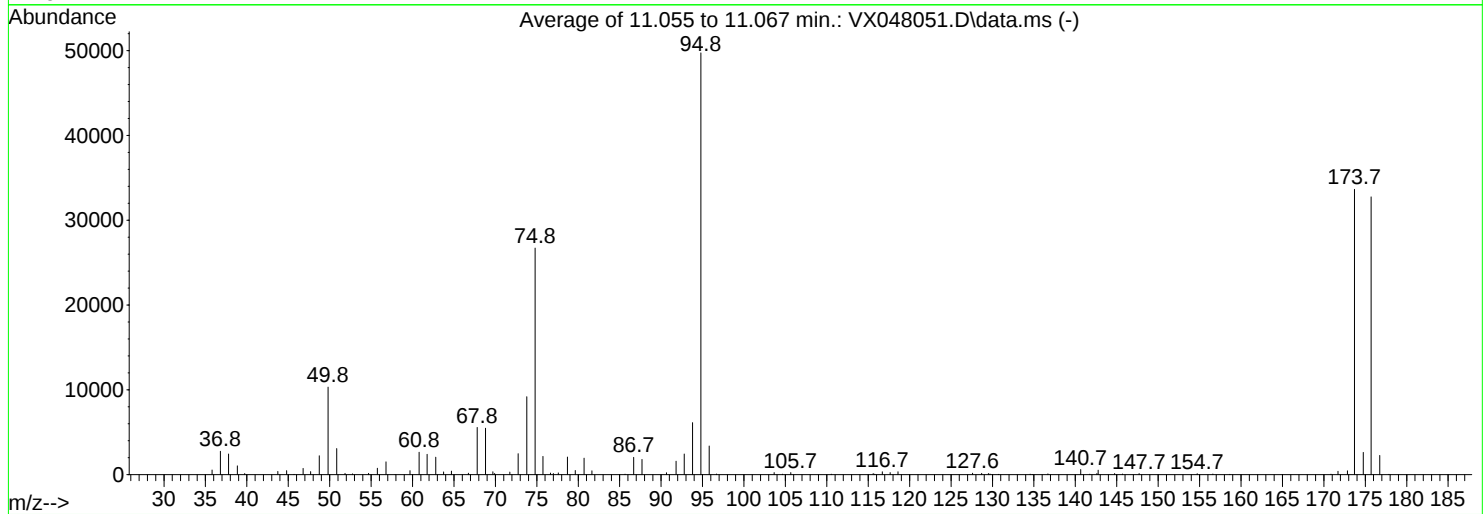


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX100725\
Data File : VX048051.D
Acq On : 07 Oct 2025 16:19
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X100725W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Oct 08 02:46:46 2025

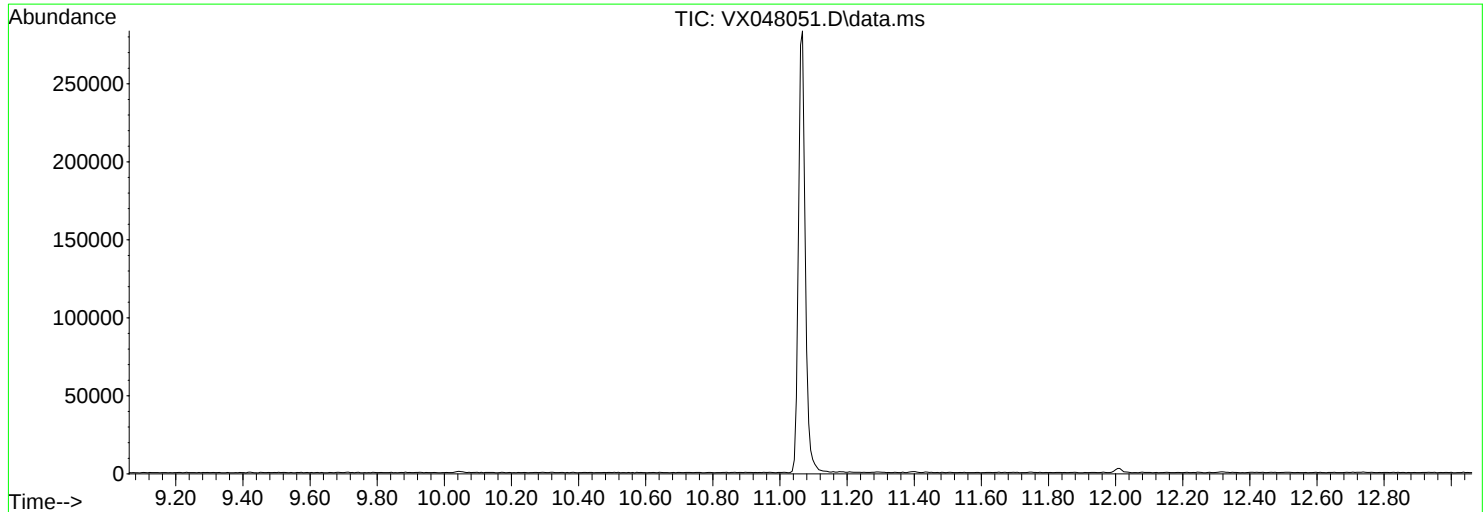

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10322	PASS
75	95	30	60	53.7	26720	PASS
95	95	100	100	100.0	49741	PASS
96	95	5	9	6.8	3375	PASS
173	174	0.00	2	1.3	452	PASS
174	95	50	100	67.7	33651	PASS
175	174	5	9	7.8	2622	PASS
176	174	95	101	97.3	32755	PASS
177	176	5	9	6.9	2263	PASS