


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100818\
Data File : VX005111.D
Acq On : 08 Oct 2018 07:44
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Title : SVOA CALIBRATION
Last Update : Mon Oct 08 04:03:43 2018

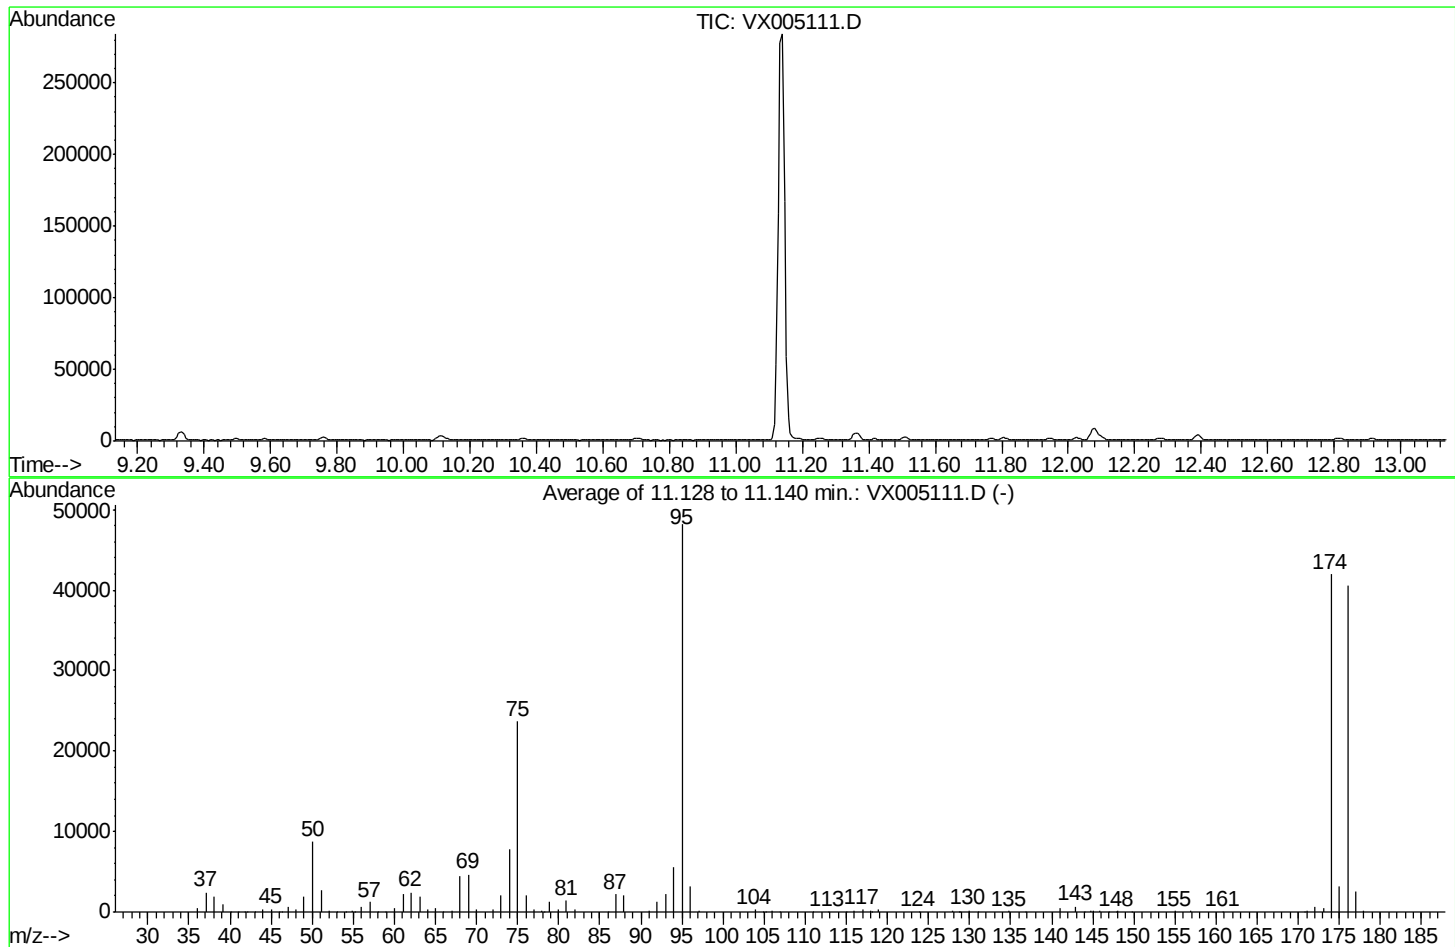

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	8721	PASS
75	95	30	60	49.1	23669	PASS
95	95	100	100	100.0	48173	PASS
96	95	5	9	6.5	3143	PASS
173	174	0.00	2	1.3	558	PASS
174	95	50	100	87.0	41928	PASS
175	174	5	9	7.5	3152	PASS
176	174	95	101	96.8	40578	PASS
177	176	5	9	6.4	2615	PASS