


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100818\
Data File : VX005138.D
Acq On : 08 Oct 2018 20:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Title : SVOA CALIBRATION
Last Update : Mon Oct 08 04:03:43 2018

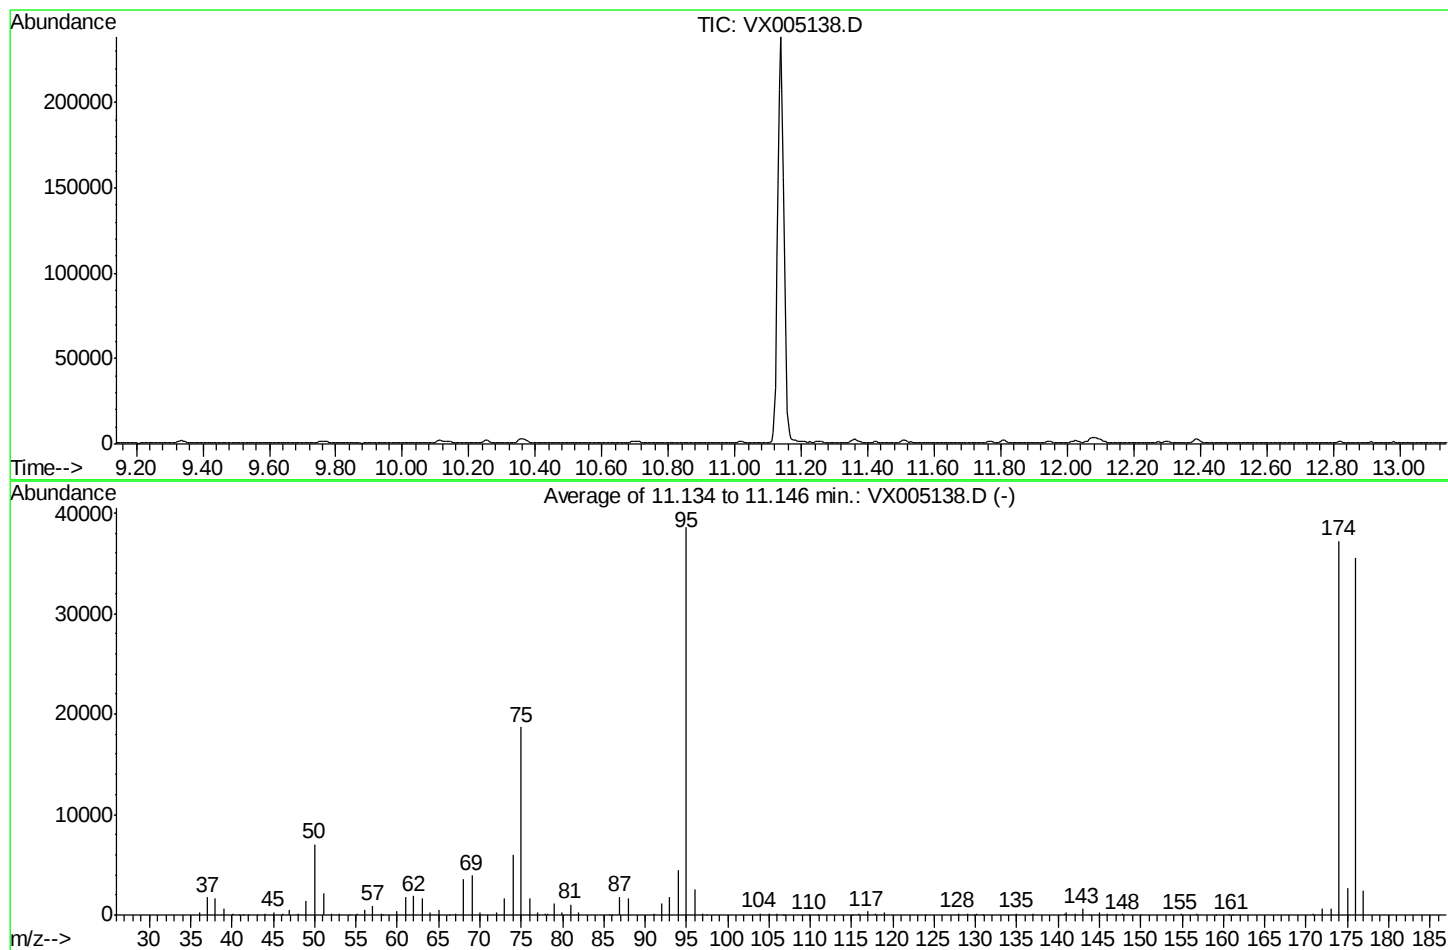

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	7013	PASS
75	95	30	60	48.4	18696	PASS
95	95	100	100	100.0	38589	PASS
96	95	5	9	6.6	2544	PASS
173	174	0.00	2	1.8	659	PASS
174	95	50	100	96.6	37258	PASS
175	174	5	9	7.2	2692	PASS
176	174	95	101	95.4	35554	PASS
177	176	5	9	6.7	2372	PASS