



t-1,3-Dichloropropene

Response Ratio

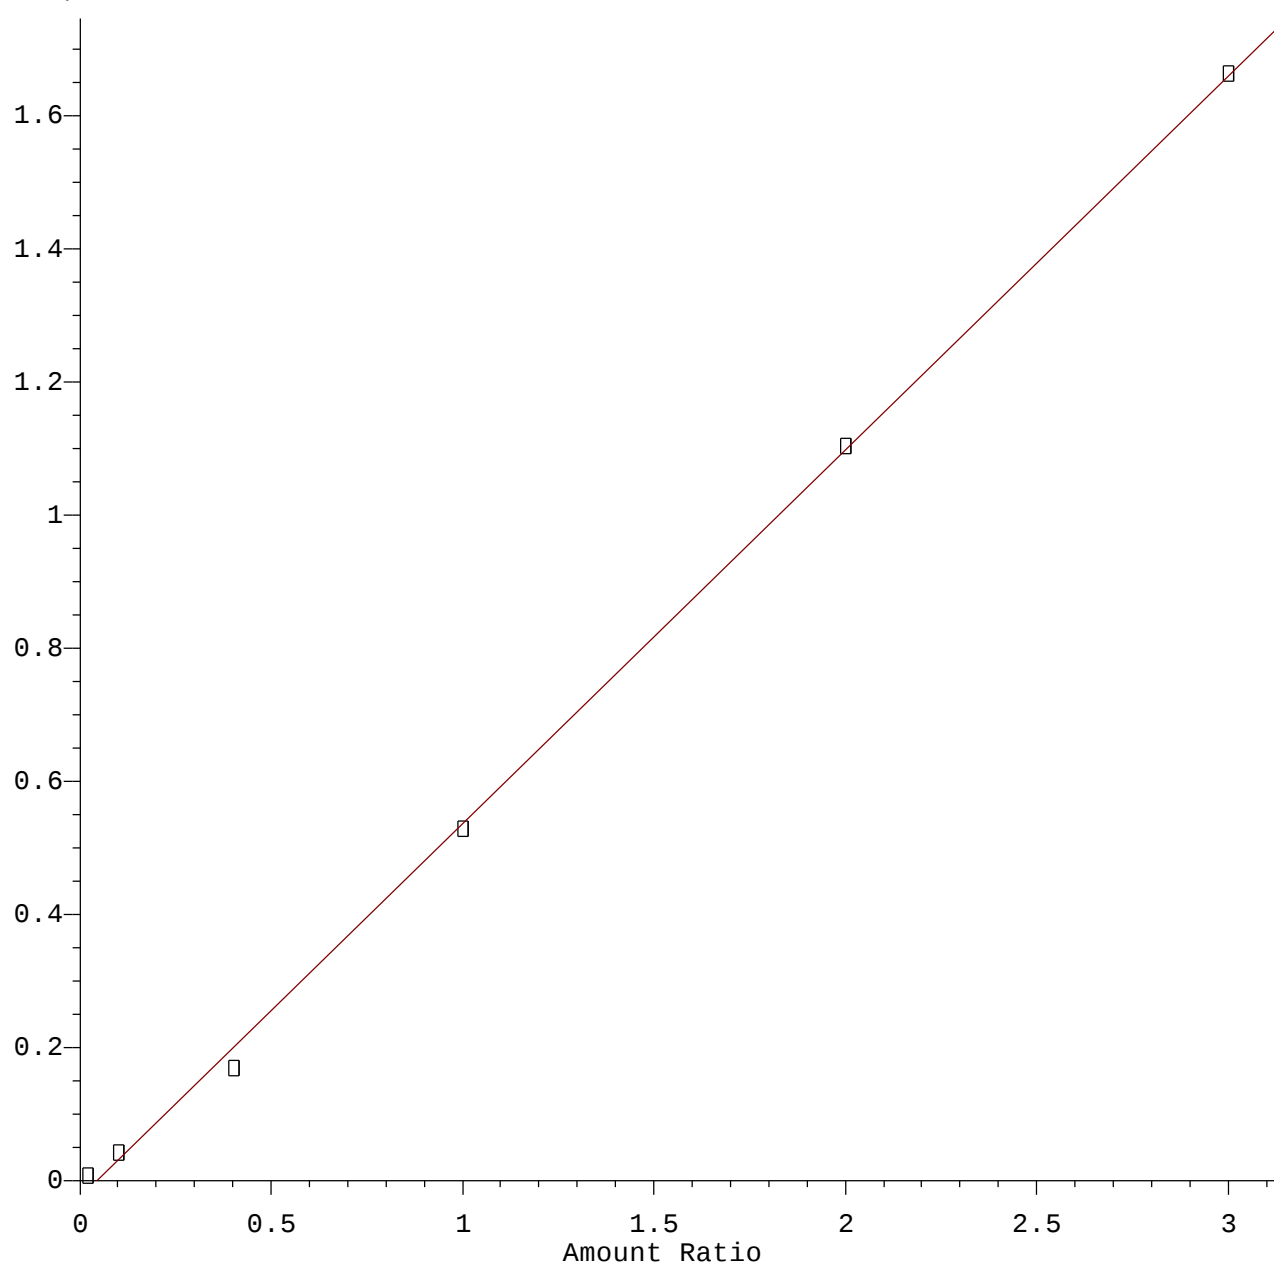


Resp Ratio = 5.61e-001 * Amt - 2.43e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

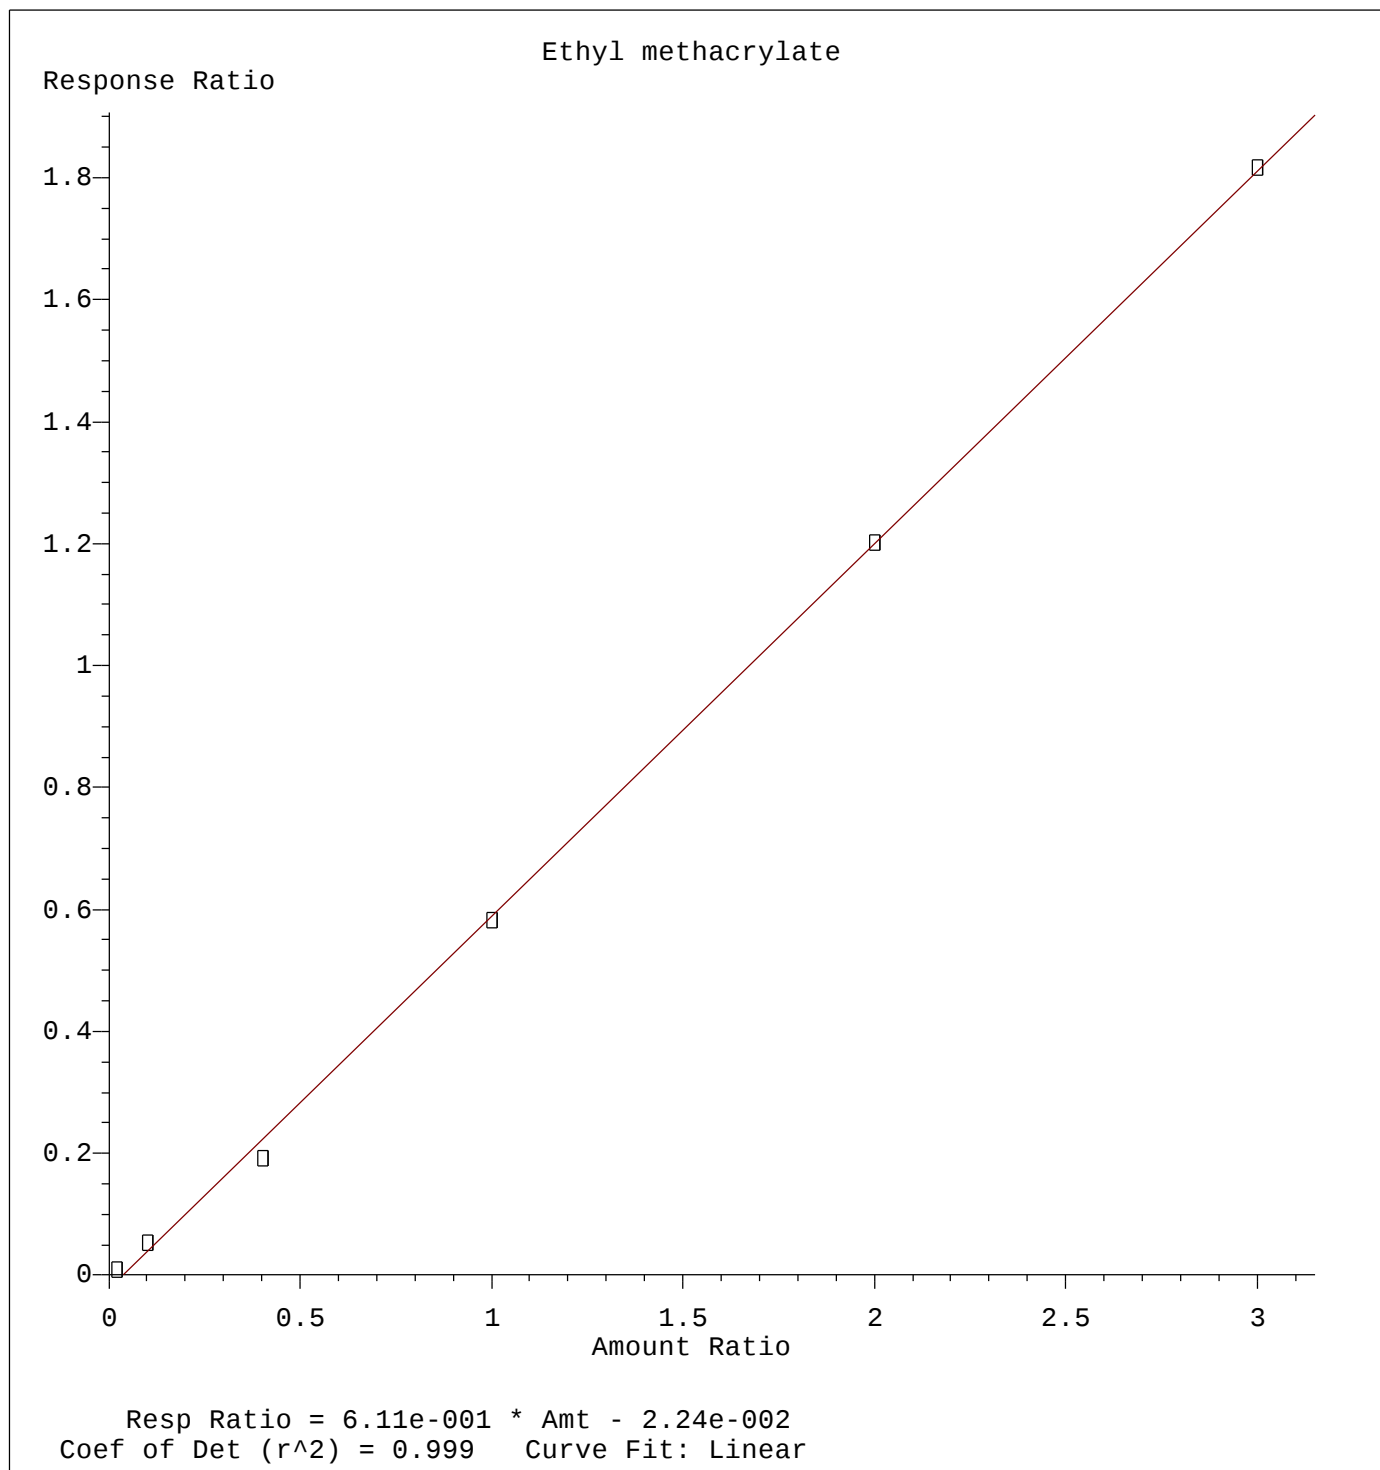

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

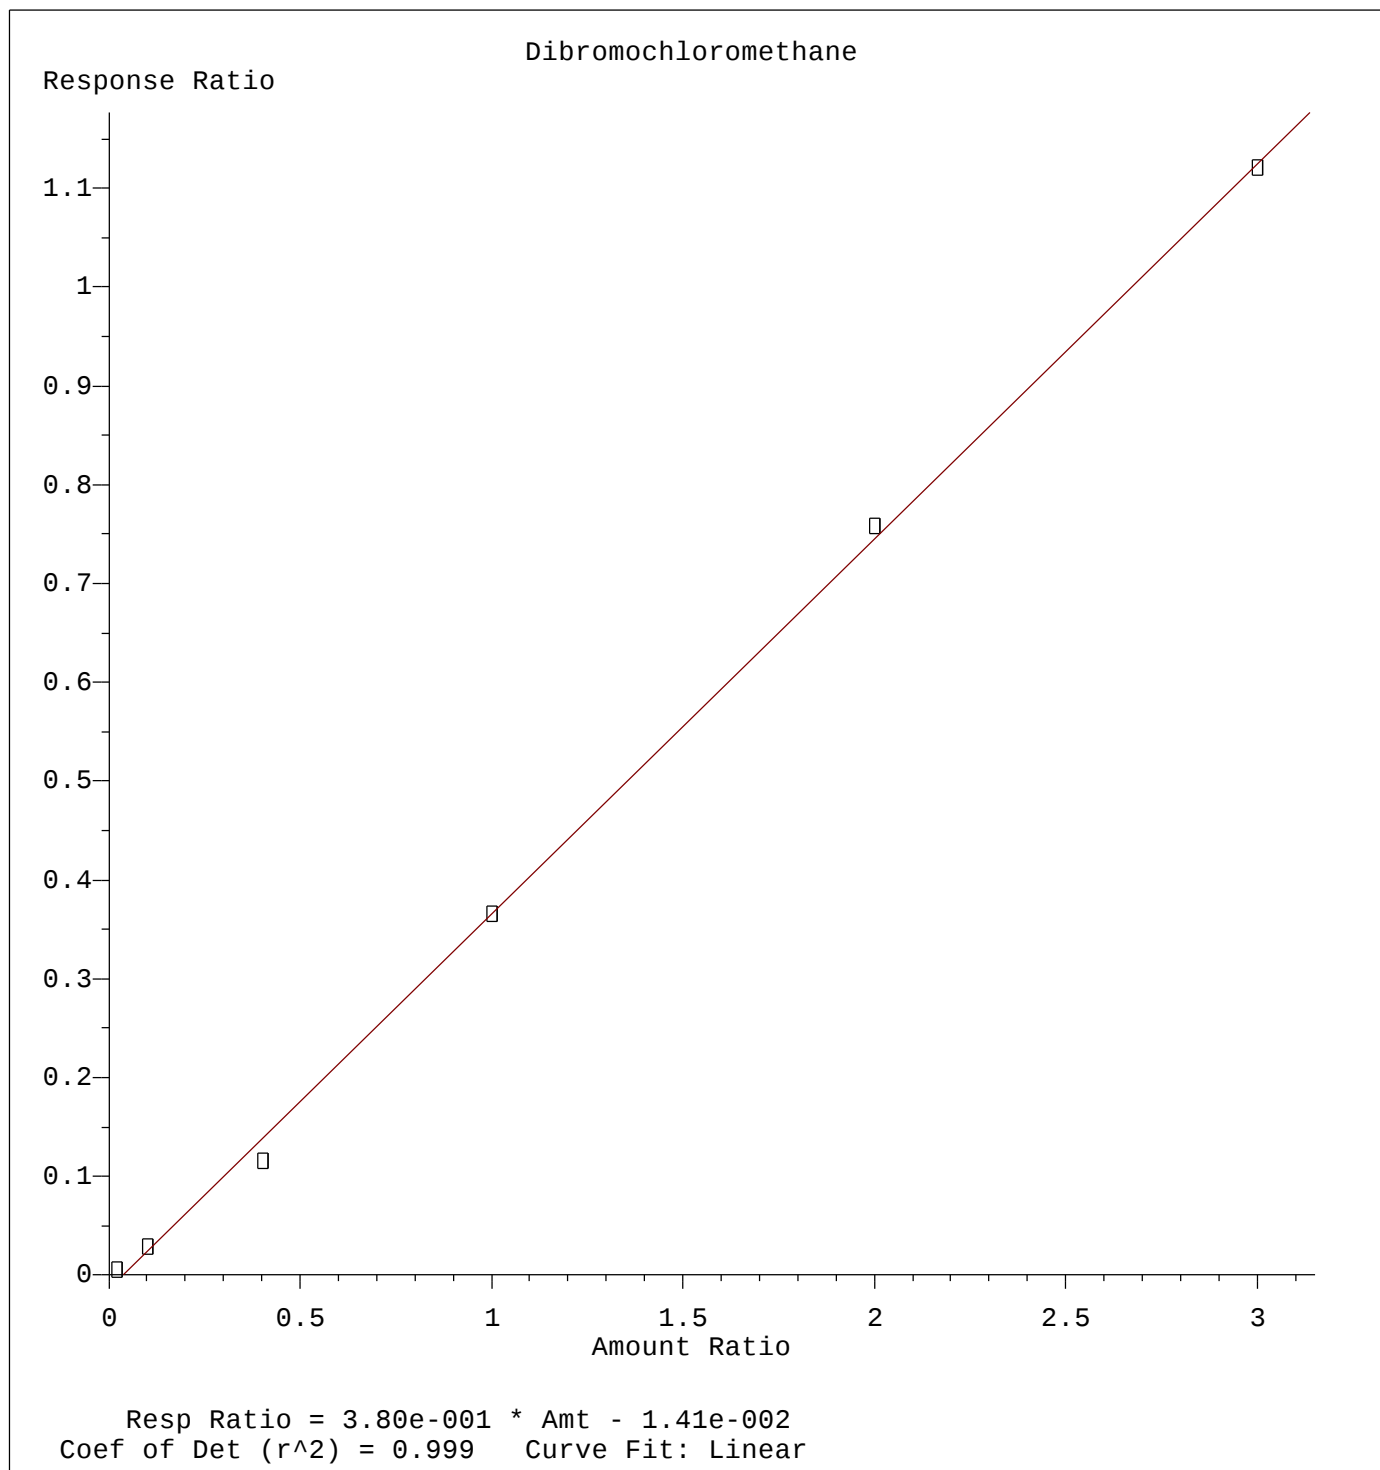


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

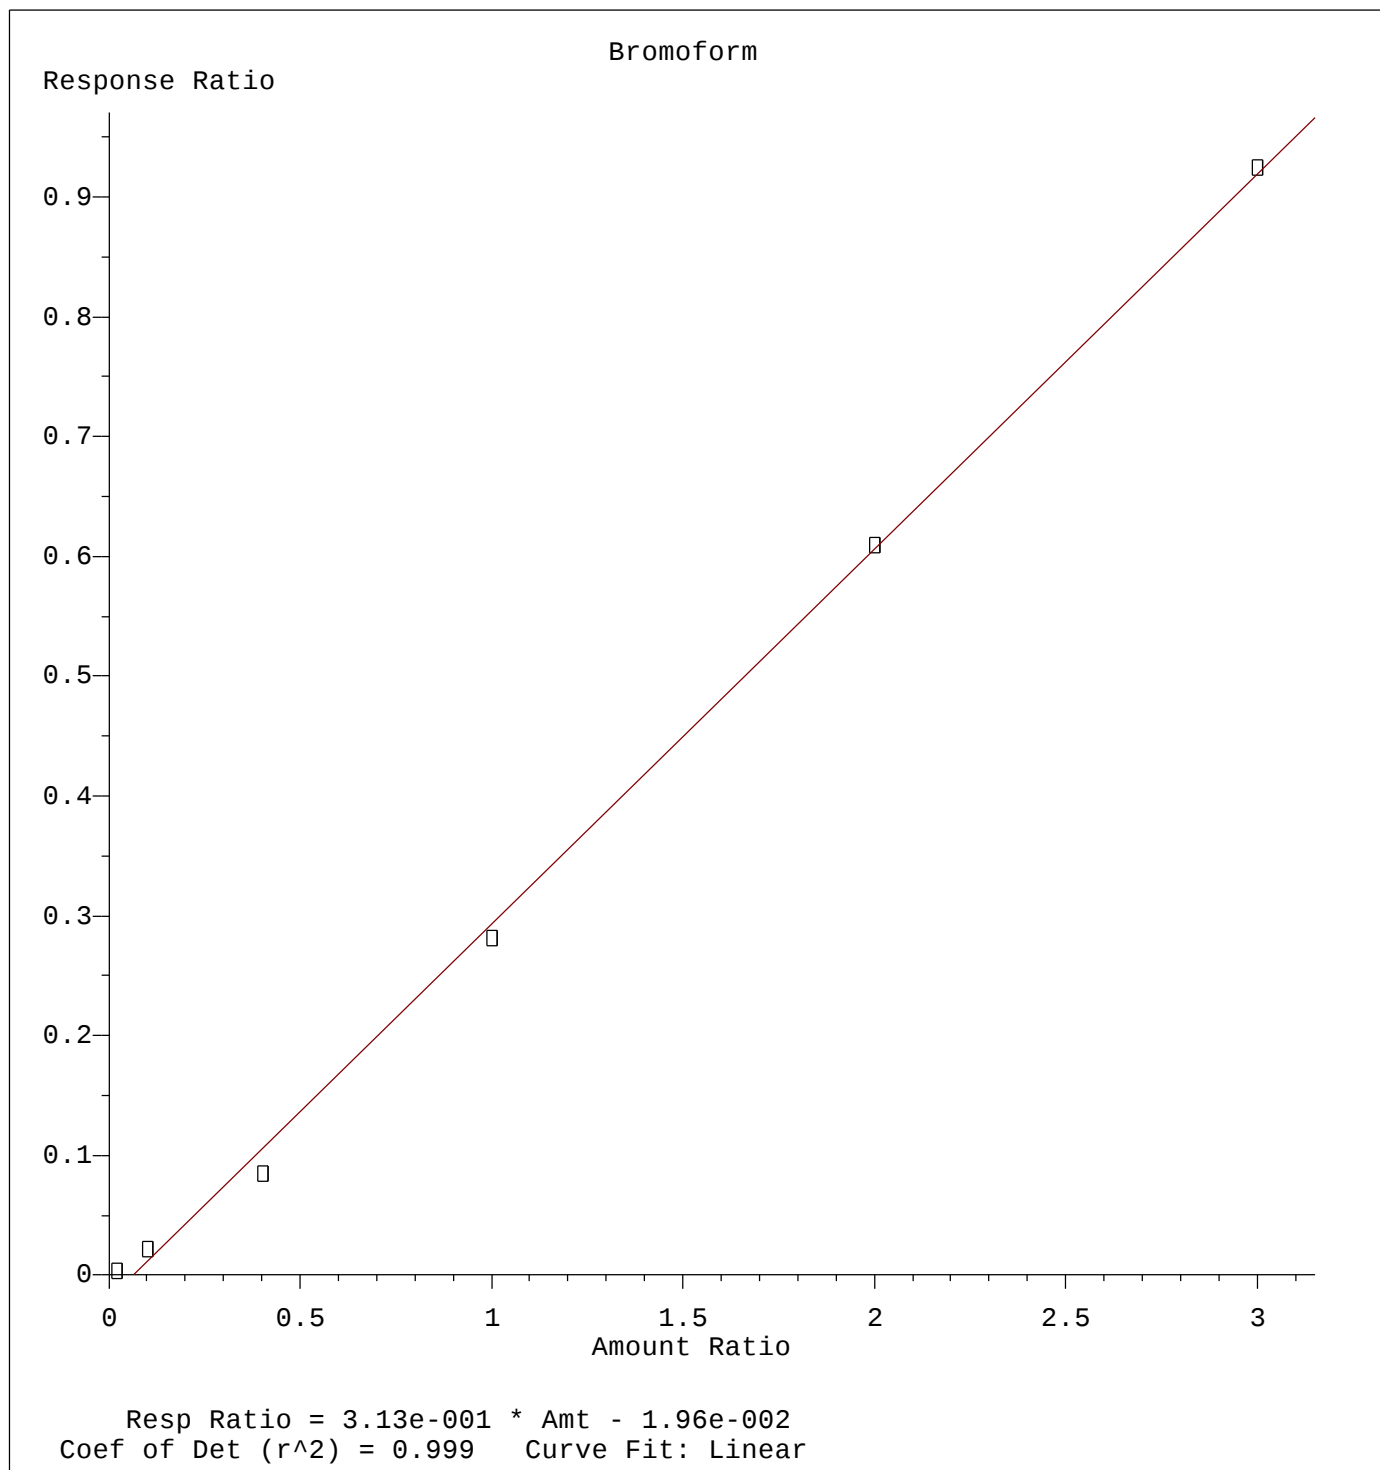

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019


trans-1,4-Dichloro-2-butene

Response Ratio

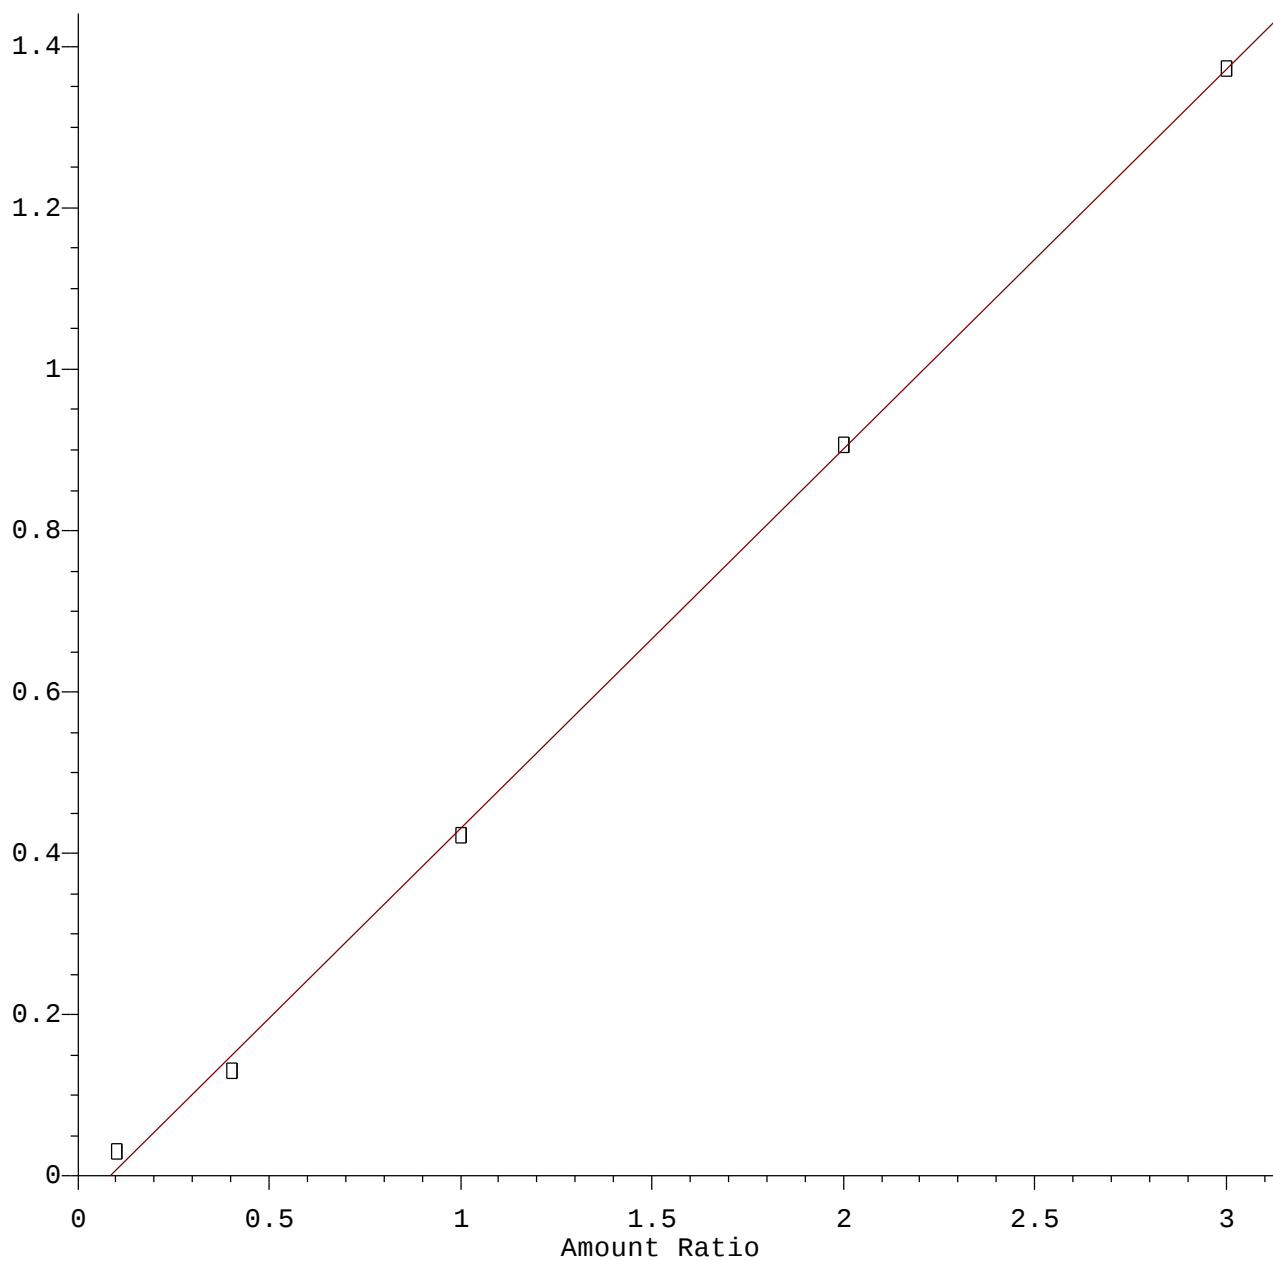


Resp Ratio = $4.70 \times 10^{-1} \times \text{Amt} - 3.84 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

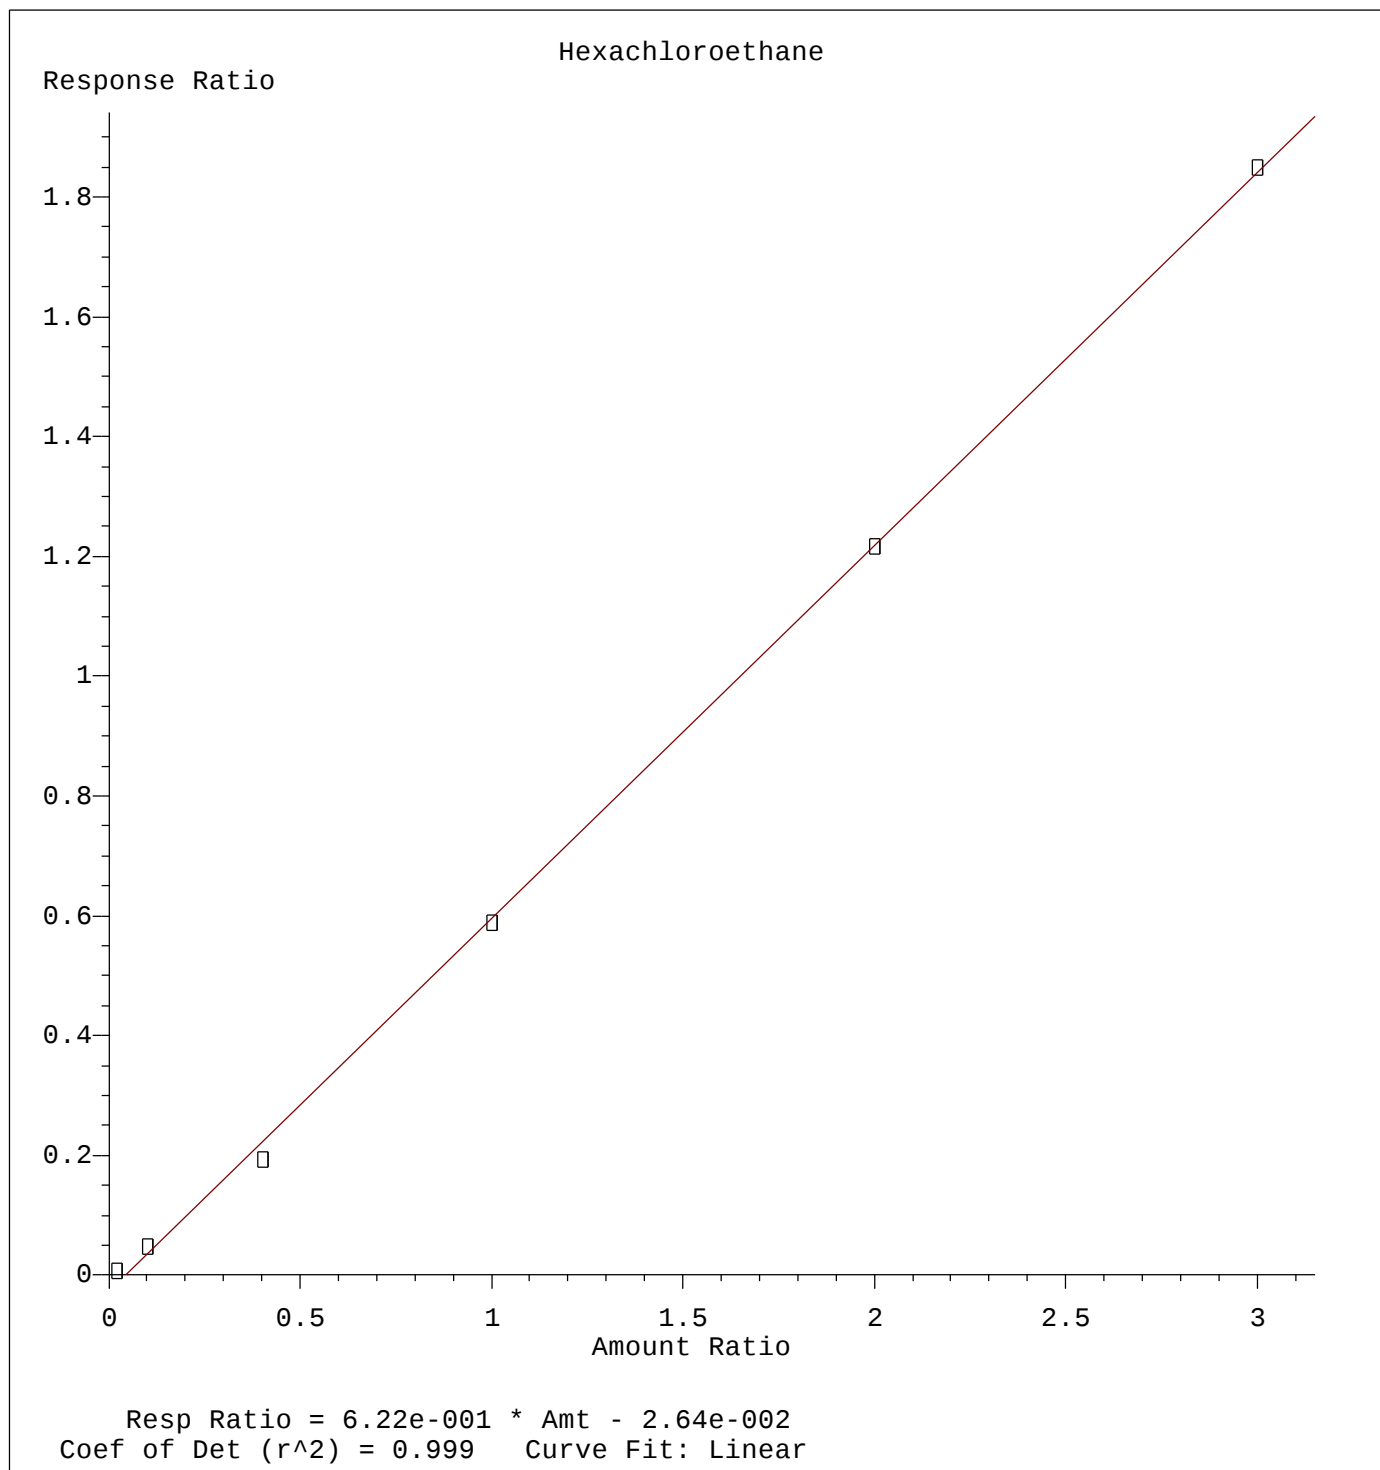


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

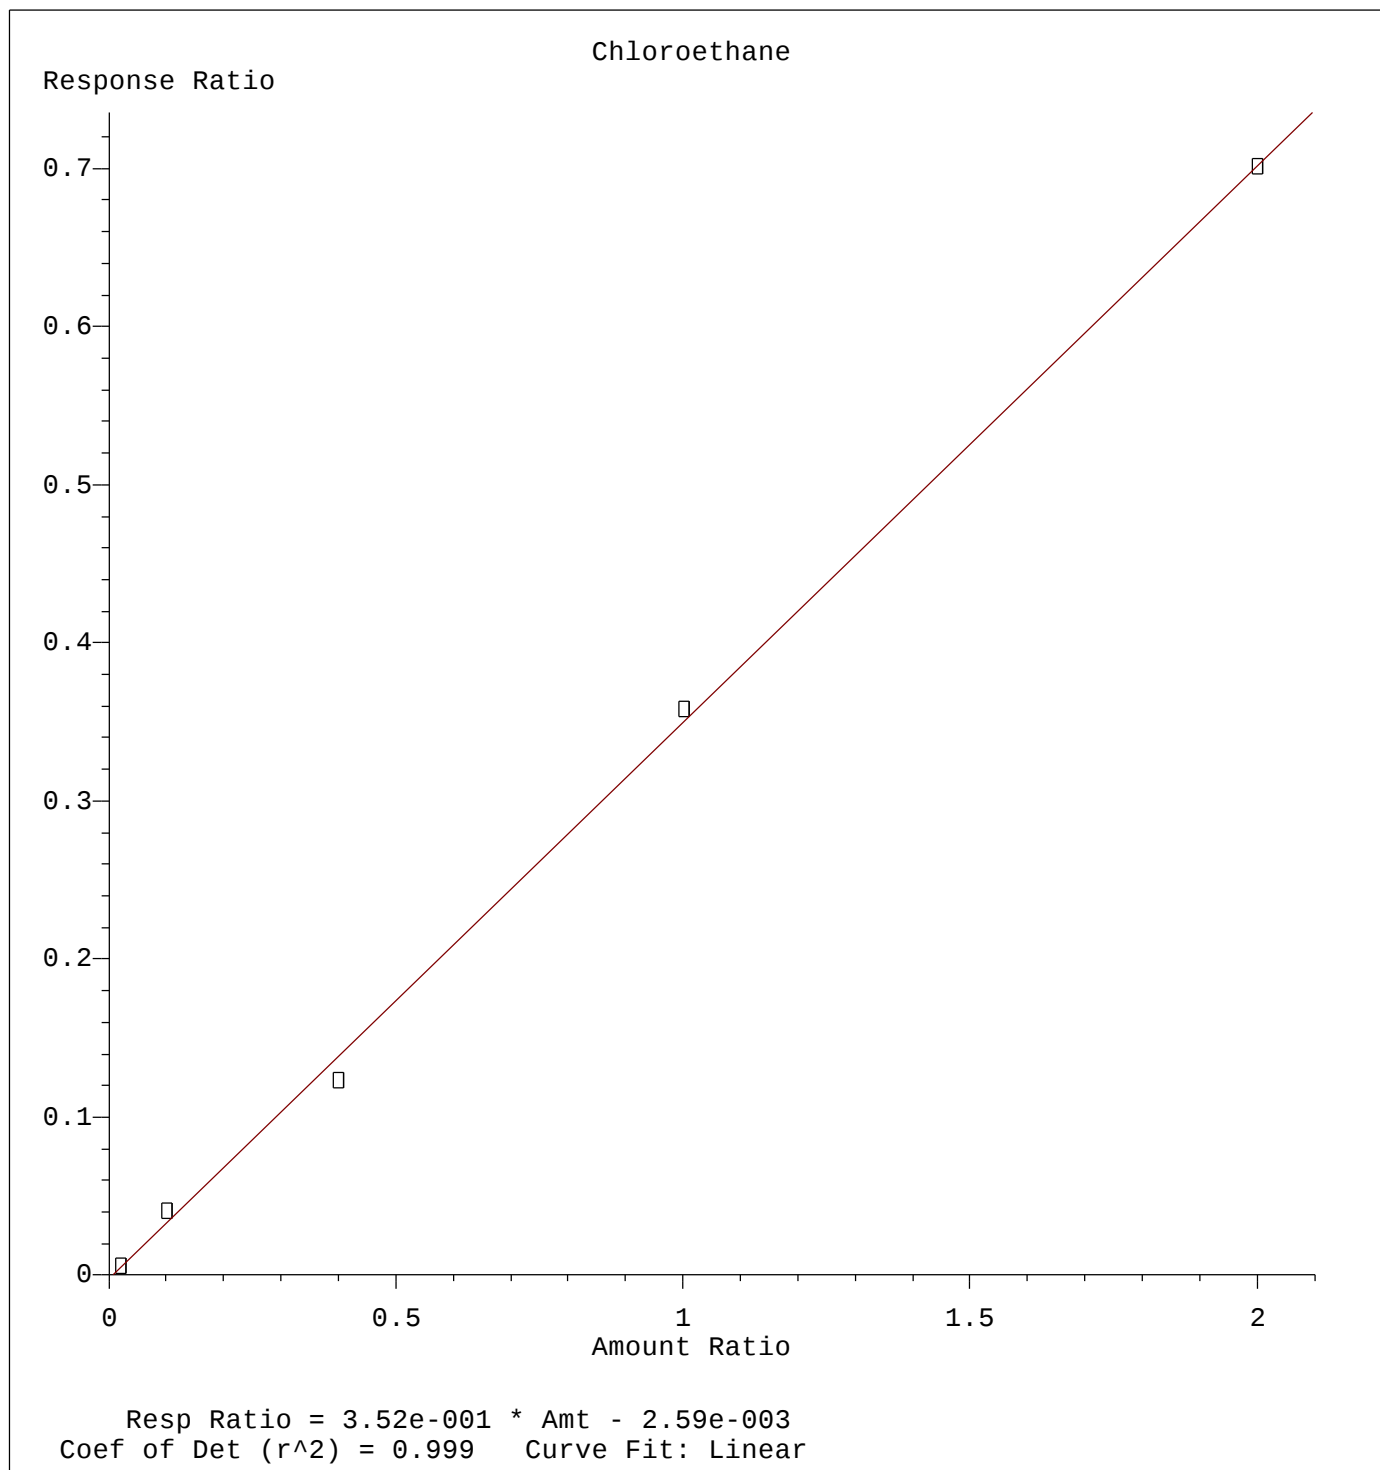

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

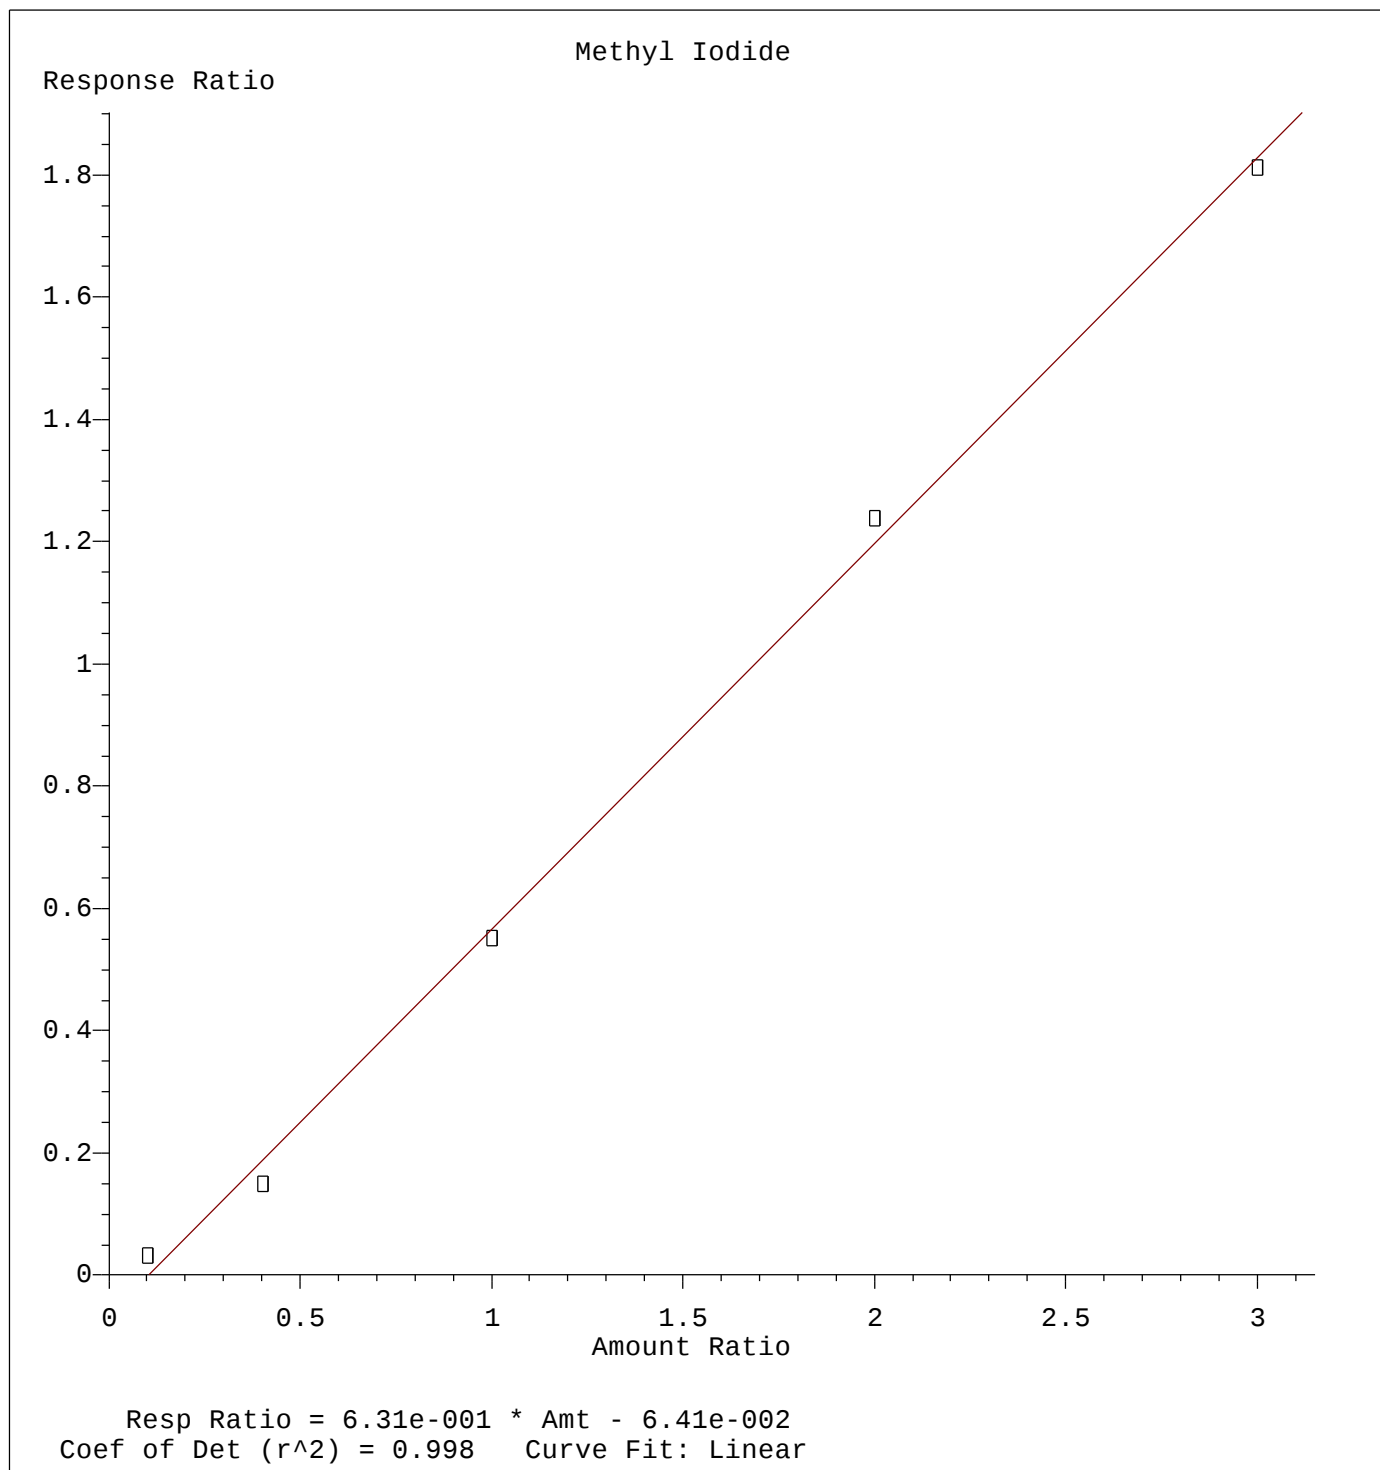


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

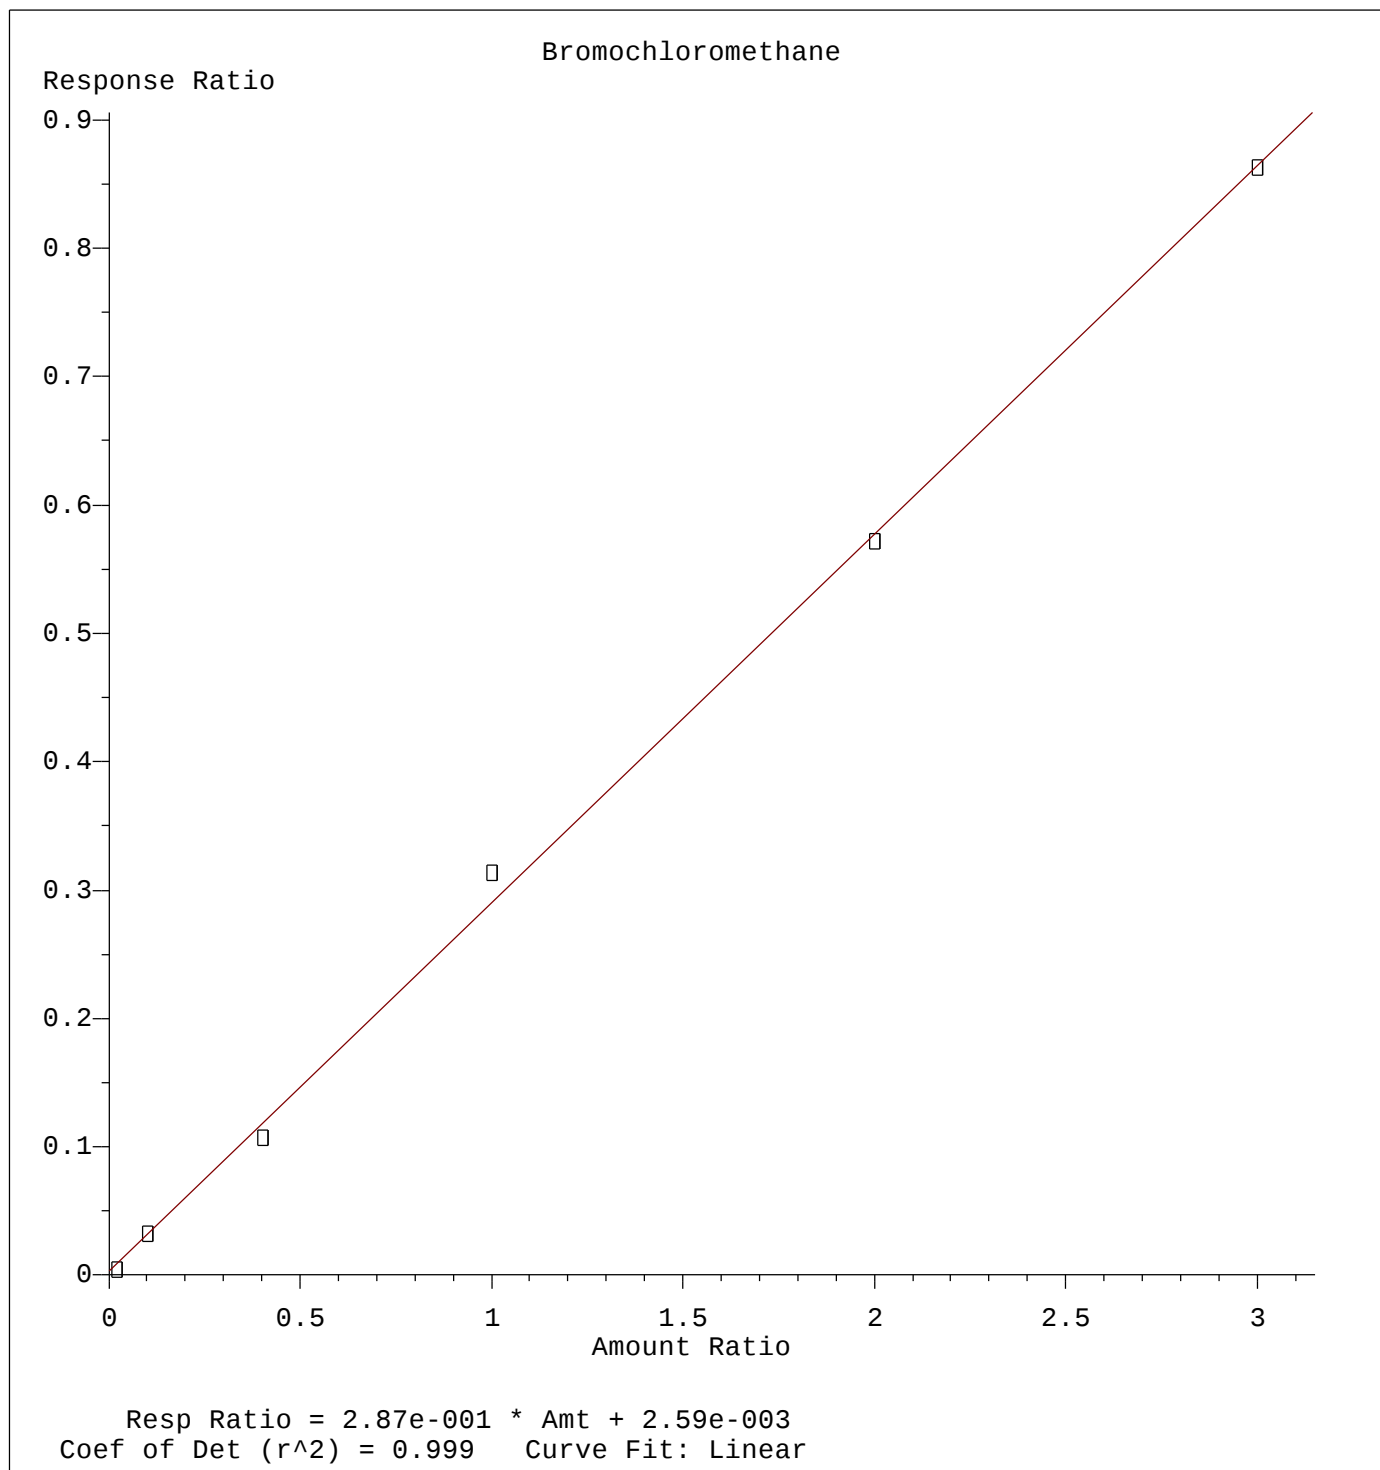

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019

1,4-Dioxane

Response Ratio

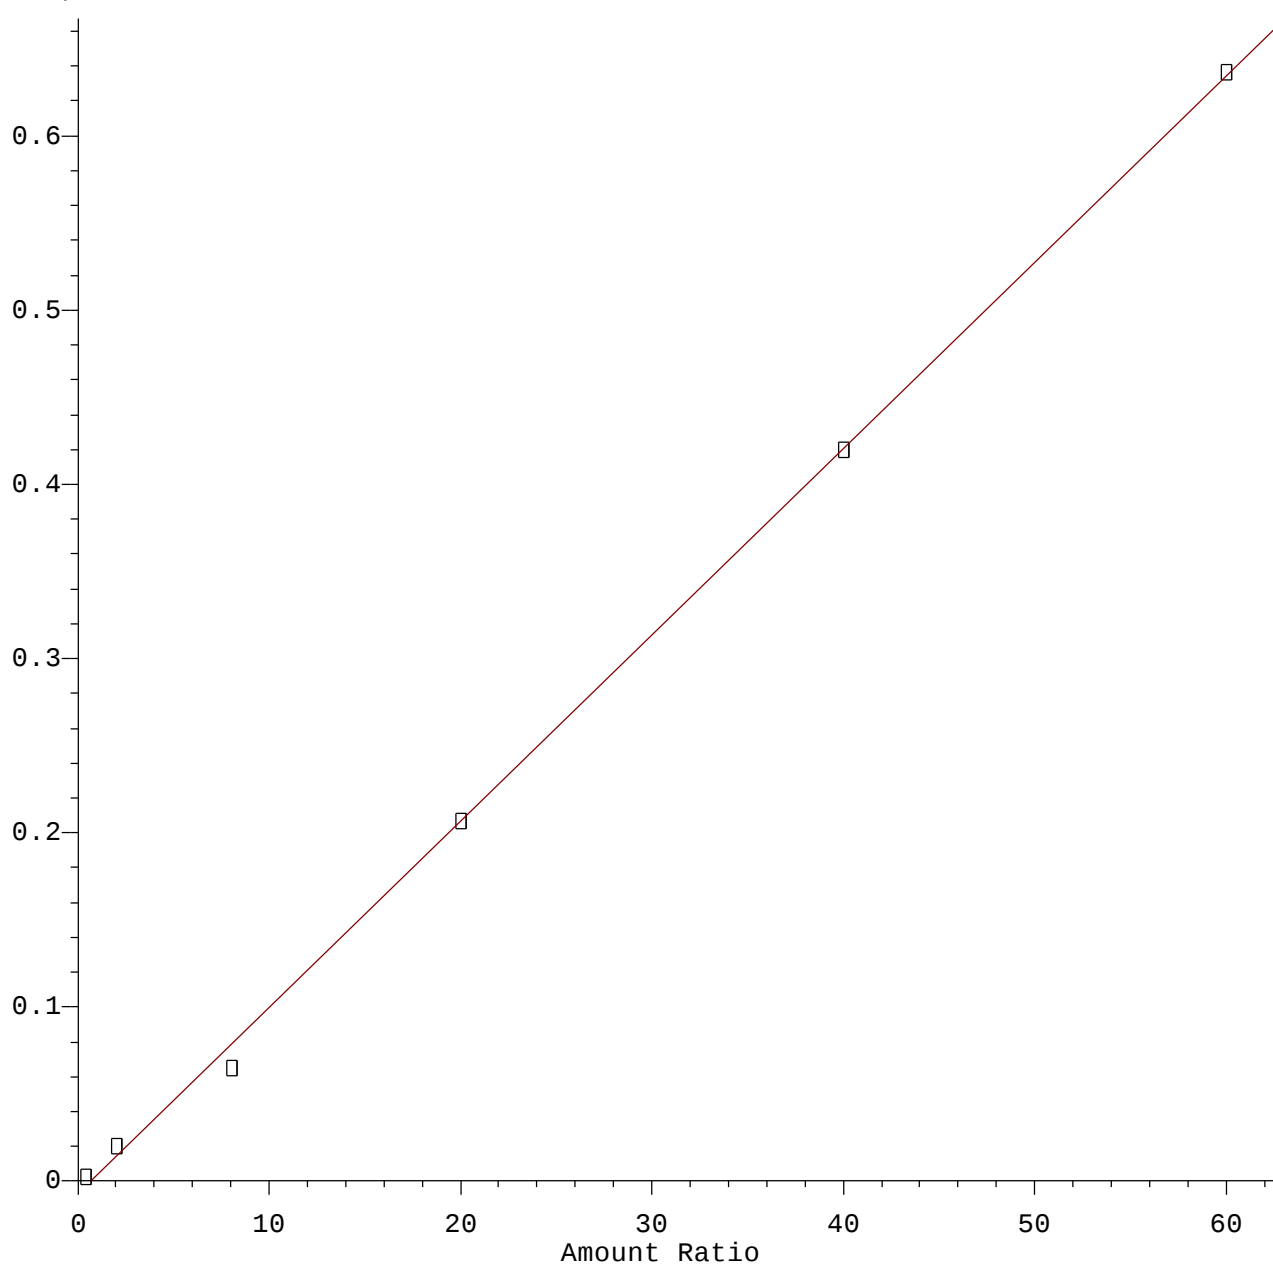

Resp Ratio = $1.07 \times 10^{-2} \times \text{Amt} - 7.50 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Calibration Table Last Updated: Wed Oct 09 01:51:23 2019