

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100819\
 Data File : VX012910.D
 Acq On : 09 Oct 2019 00:26
 Operator : JC/SP
 Sample : K5190-07
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FC-MW10S-20191002

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	268392	331660	33.41%	6.028%
2	1.265	58	62	69	rBV	20232	27375	2.76%	0.498%
3	2.429	248	253	264	rVB	6822	12103	1.22%	0.220%
4	2.594	270	280	289	rBV	39109	72694	7.32%	1.321%
5	5.490	742	755	769	rBV	111239	306342	30.86%	5.568%
6	5.648	771	781	798	rVV	202101	563606	56.77%	10.243%
7	6.051	837	847	862	rBV	124815	335724	33.82%	6.102%
8	6.849	968	978	992	rBV	307076	735665	74.10%	13.370%
9	8.709	1276	1283	1300	rBV	638625	992808	100.00%	18.044%
10	10.111	1507	1513	1522	rBV	595956	831722	83.77%	15.116%
11	11.135	1675	1681	1694	rBV	465969	596496	60.08%	10.841%
12	12.074	1829	1835	1847	rBV	561521	696037	70.11%	12.650%


Sum of corrected areas: 5502232

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100819\
Data File : VX012910.D
Acq On : 09 Oct 2019 00:26
Operator : JC/SP
Sample : K5190-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10S-20191002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

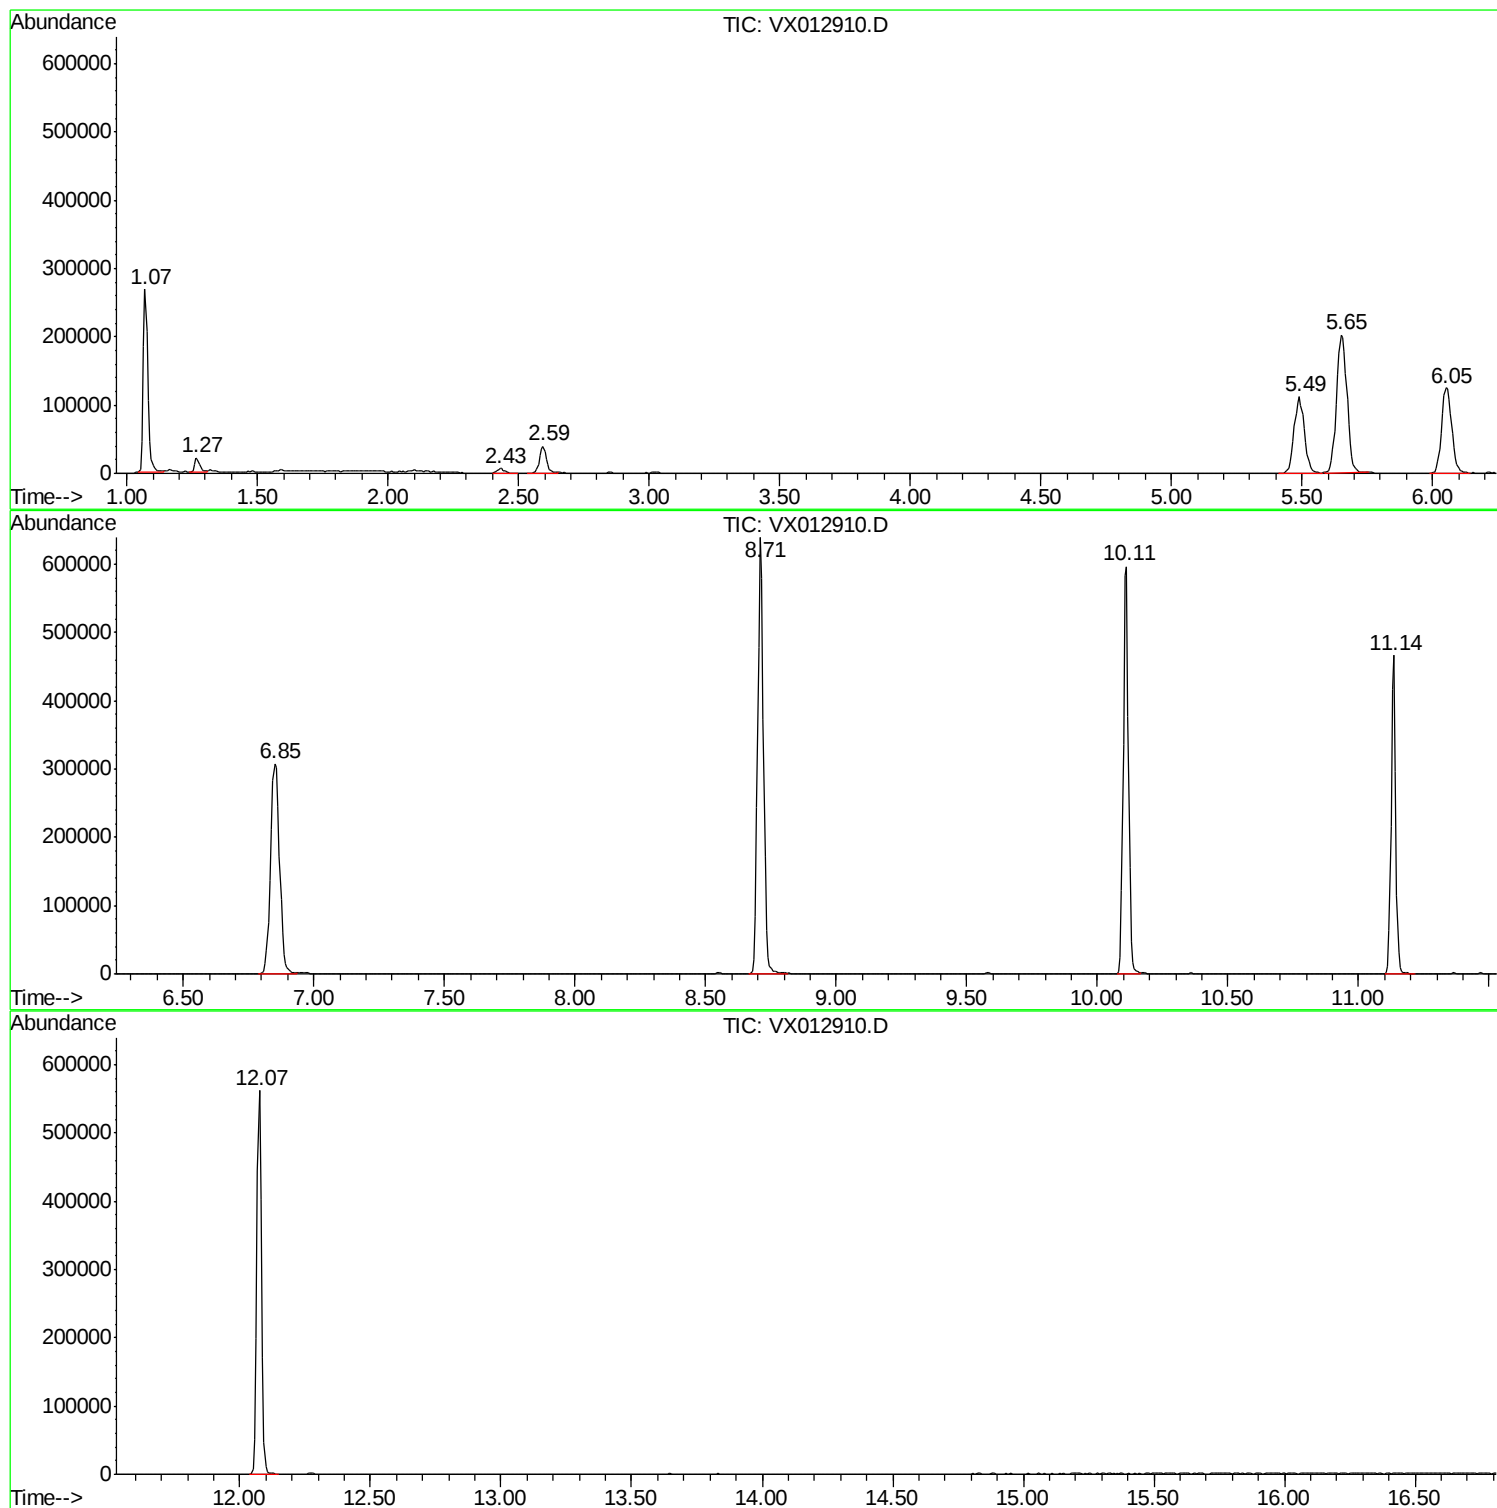

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100819\
Data File : VX012910.D
Acq On : 09 Oct 2019 00:26
Operator : JC/SP
Sample : K5190-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10S-20191002










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	6.45 ug/l	72694	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	90
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		Formamide	45	CH3NO	000075-12-7	5
4		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	4
5		Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

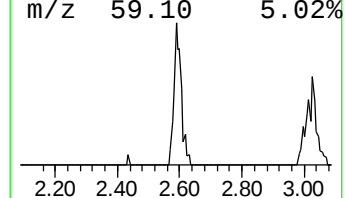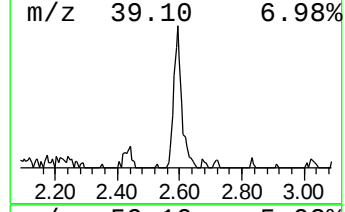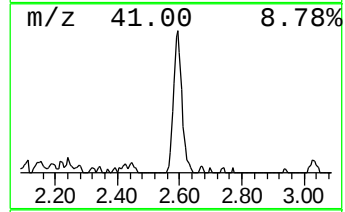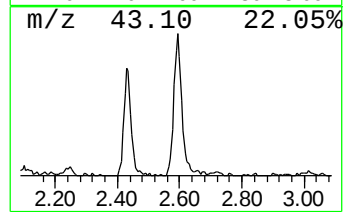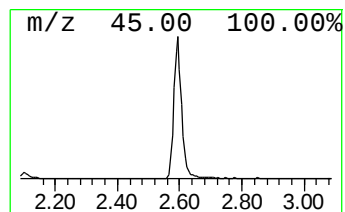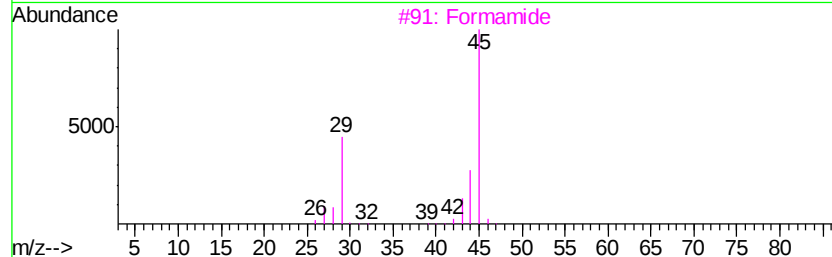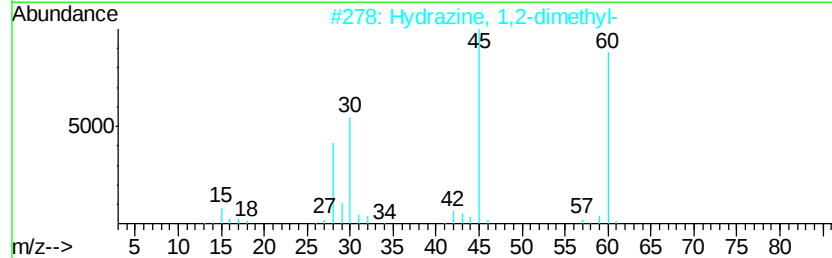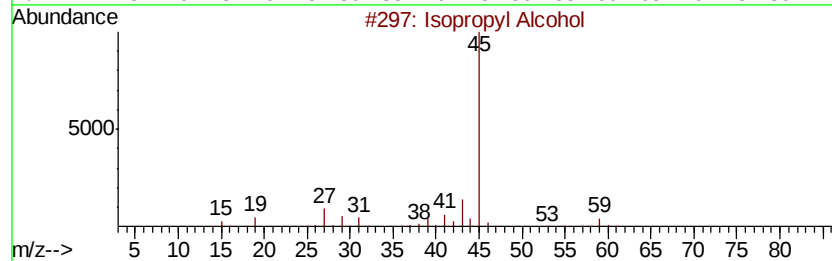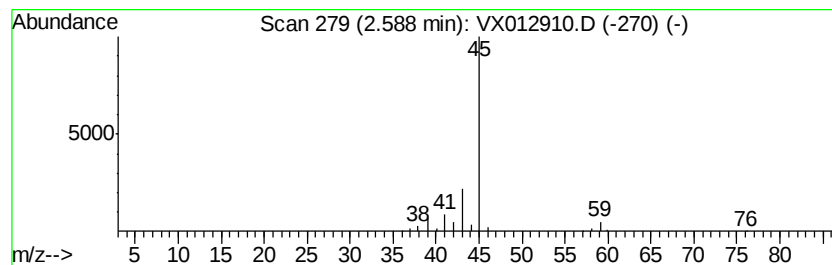

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100819\
Data File : VX012910.D
Acq On : 09 Oct 2019 00:26
Operator : JC/SP
Sample : K5190-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10S-20191002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	6.5	ug/l	72694	1	5.65	563606	50.0