

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100819\
 Data File : VX012911.D
 Acq On : 09 Oct 2019 00:49
 Operator : JC/SP
 Sample : K5190-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FC-MW10I-20191002

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	40	rBV	270986	334369	34.90%	6.348%
2	1.265	58	62	69	rBV	20435	25277	2.64%	0.480%
3	2.430	247	253	262	rVB	6659	11883	1.24%	0.226%
4	2.594	273	280	288	rBV	29523	55085	5.75%	1.046%
5	5.490	744	755	770	rBV2	105399	298776	31.19%	5.672%
6	5.655	771	782	797	rVB	190341	547789	57.18%	10.400%
7	6.051	837	847	864	rBV	123456	325600	33.99%	6.181%
8	6.850	968	978	994	rBV	302149	717042	74.84%	13.613%
9	8.709	1276	1283	1300	rBV	616067	958064	100.00%	18.189%
10	10.105	1506	1512	1527	rBV	563888	794970	82.98%	15.092%
11	11.135	1675	1681	1695	rBV	431029	559647	58.41%	10.625%
12	12.074	1829	1835	1844	rBV	511320	638877	66.68%	12.129%


Sum of corrected areas: 5267379

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100819\
Data File : VX012911.D
Acq On : 09 Oct 2019 00:49
Operator : JC/SP
Sample : K5190-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10I-20191002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

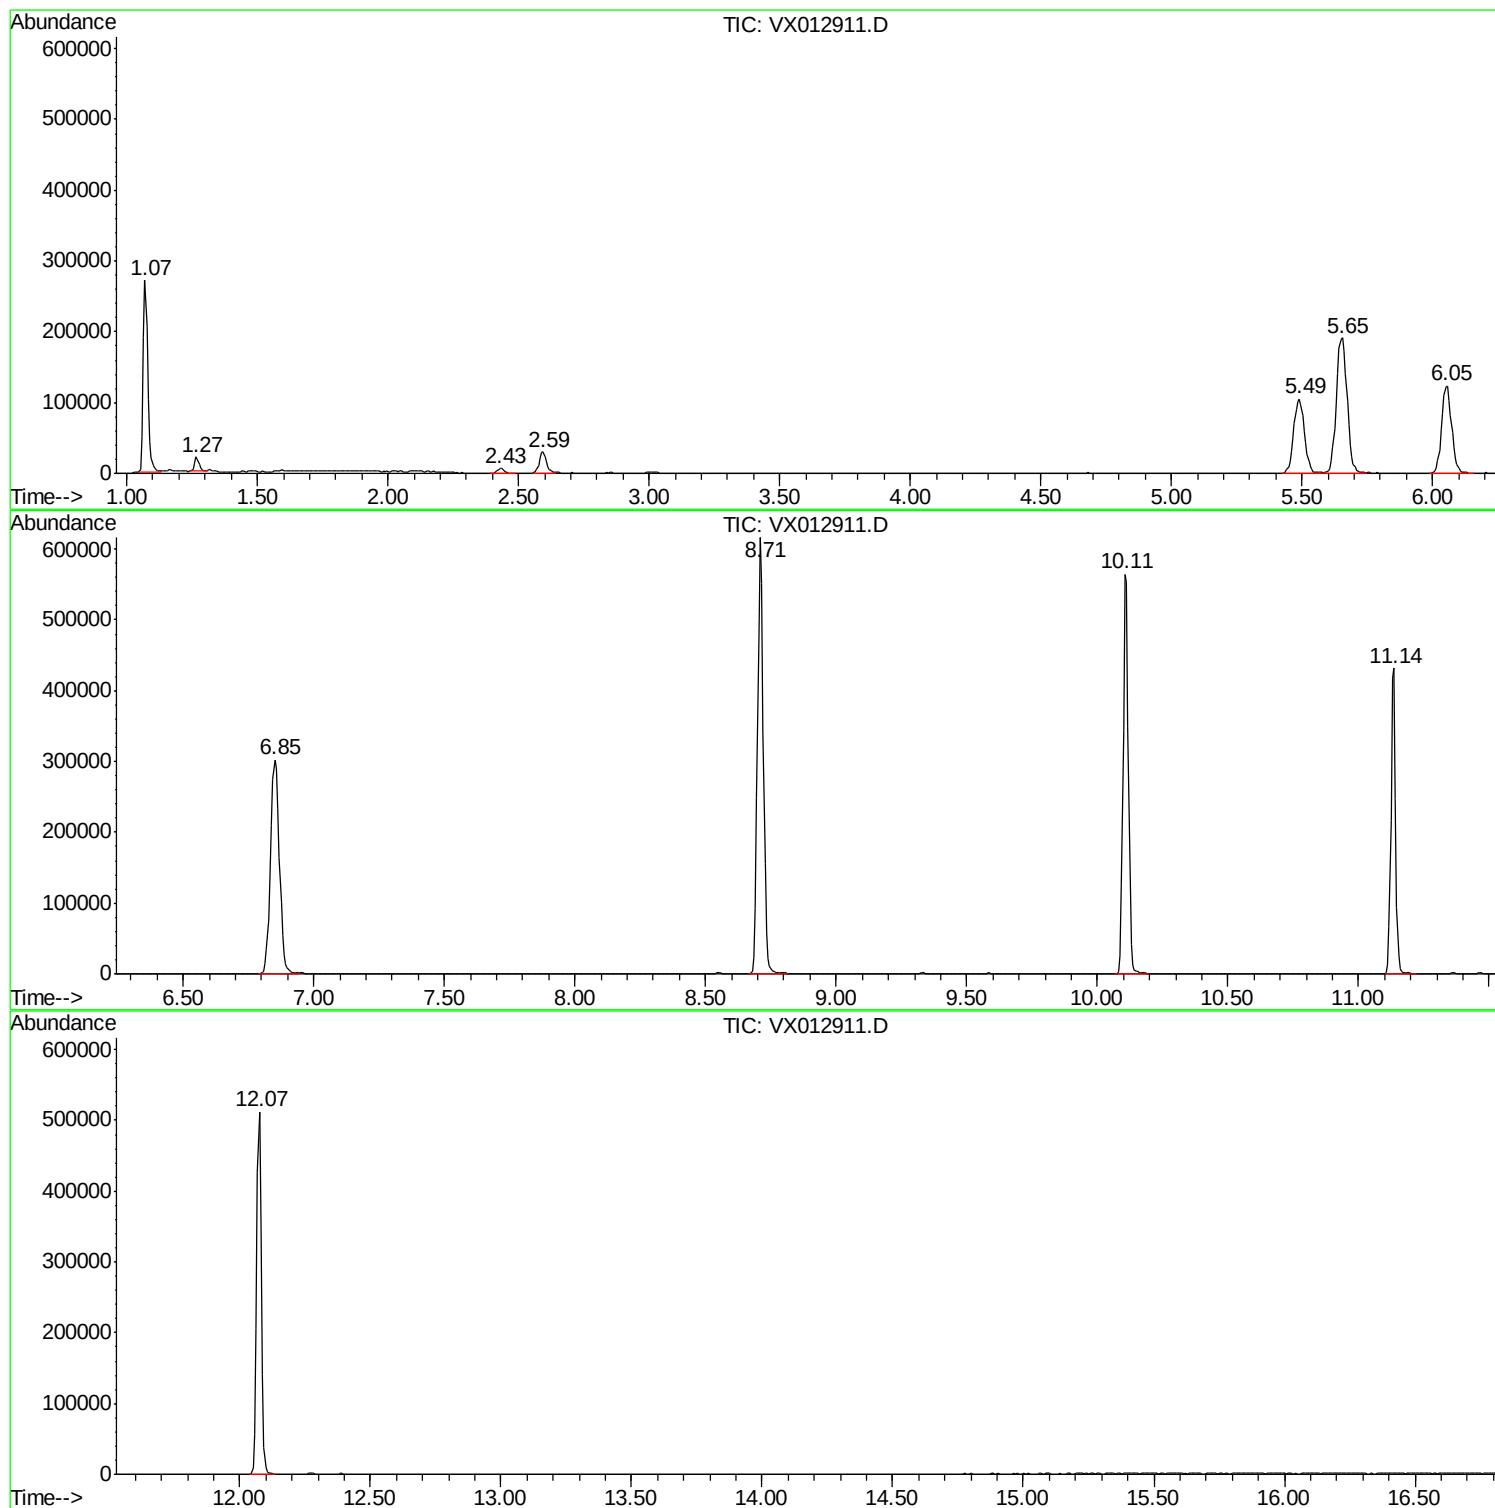

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100819\
Data File : VX012911.D
Acq On : 09 Oct 2019 00:49
Operator : JC/SP
Sample : K5190-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10I-20191002










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	5.03 ug/l	55085	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
4		Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4
5		2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	4

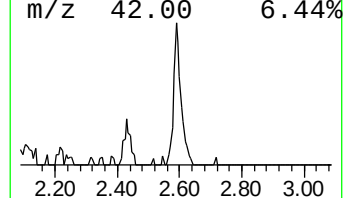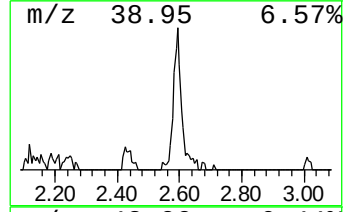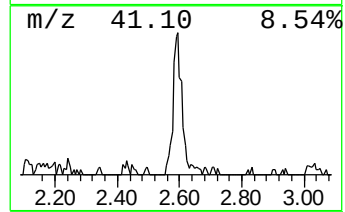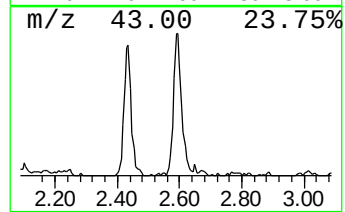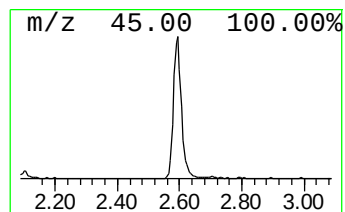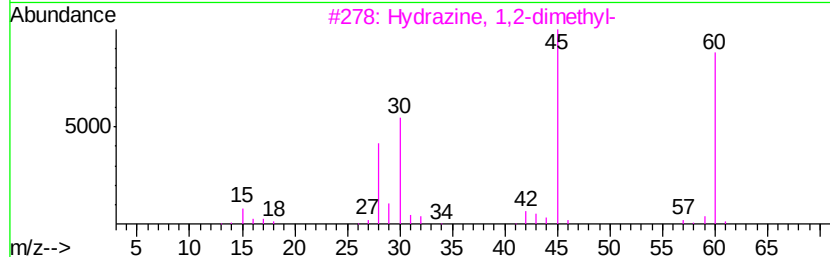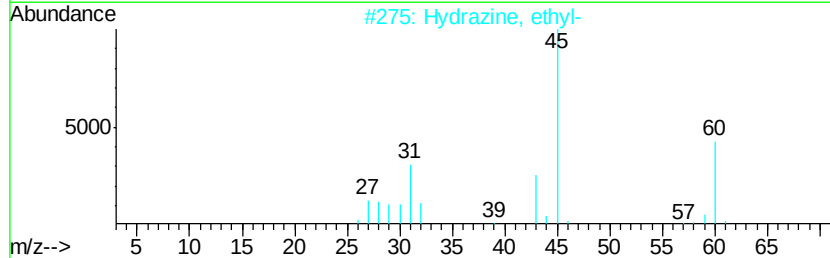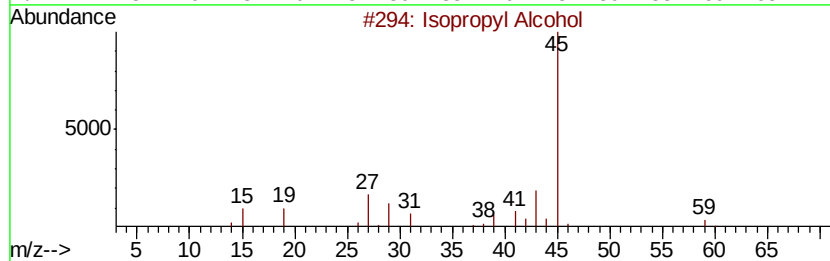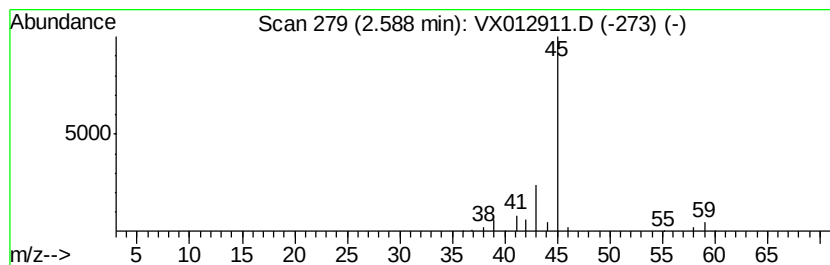

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100819\
Data File : VX012911.D
Acq On : 09 Oct 2019 00:49
Operator : JC/SP
Sample : K5190-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW10I-20191002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	5.0	ug/l	55085	1	5.65	547789	50.0