

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100819\
 Data File : VX012912.D
 Acq On : 09 Oct 2019 01:12
 Operator : JC/SP
 Sample : K5190-11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FC-MW1011-20191002

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	550626	667681	67.70%	9.606%
2	1.265	59	62	69	rBV	20695	27059	2.74%	0.389%
3	2.594	269	280	290	rBV	39503	73562	7.46%	1.058%
4	5.490	741	755	770	rBV2	108687	307775	31.21%	4.428%
5	5.655	770	782	794	rVV	200152	560654	56.85%	8.066%
6	6.057	837	848	863	rBV	127508	335547	34.02%	4.827%
7	6.849	969	978	994	rBV	310703	736809	74.71%	10.600%
8	8.709	1271	1283	1298	rBV	628075	986203	100.00%	14.188%
9	9.038	1332	1337	1343	rBV4	6888	11993	1.22%	0.173%
10	9.672	1435	1441	1445	rBV2	13672	20359	2.06%	0.293%
11	9.885	1472	1476	1482	rVB2	7335	11079	1.12%	0.159%
12	10.111	1507	1513	1528	rBV	583277	842798	85.46%	12.125%
13	10.233	1528	1533	1539	rVB4	6192	10710	1.09%	0.154%
14	10.337	1545	1550	1551	rBV2	7704	10928	1.11%	0.157%
15	10.349	1551	1552	1558	rVB2	9382	10618	1.08%	0.153%
16	10.507	1573	1578	1582	rBV3	8597	12328	1.25%	0.177%
17	10.654	1592	1602	1608	rBV7	10747	28203	2.86%	0.406%
18	10.806	1620	1627	1634	rBV5	5227	10906	1.11%	0.157%
19	11.013	1657	1661	1665	rBV2	10871	15314	1.55%	0.220%
20	11.135	1675	1681	1686	rBV	443679	587692	59.59%	8.455%
21	11.275	1700	1704	1709	rVB4	9979	14134	1.43%	0.203%
22	11.763	1780	1784	1788	rBV	11690	14119	1.43%	0.203%
23	11.916	1801	1809	1811	rBV3	12743	22023	2.23%	0.317%
24	11.940	1811	1813	1820	rVB	20375	23177	2.35%	0.333%
25	12.019	1822	1826	1830	rVV2	10952	14531	1.47%	0.209%
26	12.074	1830	1835	1847	rVB	557030	749672	76.02%	10.785%
27	12.227	1856	1860	1864	rVB	14404	17004	1.72%	0.245%
28	12.294	1864	1871	1878	rVV	33356	44537	4.52%	0.641%
29	12.367	1878	1883	1884	rVV2	21072	27362	2.77%	0.394%
30	12.385	1884	1886	1893	rVB	22073	25761	2.61%	0.371%
31	12.659	1921	1931	1934	rBV4	12562	25846	2.62%	0.372%
32	12.708	1934	1939	1943	rVB5	9405	15388	1.56%	0.221%
33	12.763	1943	1948	1953	rBV4	25222	39661	4.02%	0.571%
34	12.891	1962	1969	1974	rVB3	27292	50377	5.11%	0.725%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX100819\
 Data File : VX012912.D
 Acq On : 09 Oct 2019 01:12
 Operator : JC/SP
 Sample : K5190-11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FC-MW1011-20191002

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
 Title : SW846 8260

35	12.952	1974	1979	1981	rBV	20994	30604	3.10%	0.440%
36	13.086	1996	2001	2006	rVB2	10164	14206	1.44%	0.204%
37	13.190	2013	2018	2021	rVB	16023	18990	1.93%	0.273%
38	13.245	2024	2027	2031	rVB	8923	10696	1.08%	0.154%
39	13.342	2039	2043	2048	rVV3	10485	17154	1.74%	0.247%
40	13.452	2056	2061	2063	rBV4	8326	13801	1.40%	0.199%
41	13.470	2063	2064	2070	rVB	10437	10387	1.05%	0.149%
42	13.556	2075	2078	2081	rBV4	7715	10346	1.05%	0.149%
43	13.592	2081	2084	2087	rVB2	11223	13896	1.41%	0.200%
44	13.635	2087	2091	2094	rBV4	10826	16167	1.64%	0.233%
45	13.690	2094	2100	2102	rVV3	25828	62077	6.29%	0.893%
46	13.714	2102	2104	2109	rVV	42807	49847	5.05%	0.717%
47	13.806	2113	2119	2123	rBV	21140	30087	3.05%	0.433%
48	13.903	2131	2135	2140	rVB2	17070	23649	2.40%	0.340%
49	13.976	2140	2147	2151	rBV	38662	57685	5.85%	0.830%
50	14.025	2151	2155	2158	rVV2	12053	17330	1.76%	0.249%
51	14.123	2167	2171	2174	rBV3	9258	11844	1.20%	0.170%
52	14.159	2174	2177	2183	rVB2	11970	12852	1.30%	0.185%
53	14.427	2215	2221	2225	rBV3	16106	23268	2.36%	0.335%
54	14.470	2225	2228	2234	rVB4	7994	11378	1.15%	0.164%
55	14.537	2234	2239	2243	rBV2	15547	28409	2.88%	0.409%
56	14.726	2266	2270	2274	rVB2	26253	33772	3.42%	0.486%
57	14.775	2274	2278	2282	rVB3	9214	13589	1.38%	0.195%
58	14.842	2283	2289	2293	rBV2	19579	30949	3.14%	0.445%
59	14.970	2307	2310	2315	rVB4	8611	13813	1.40%	0.199%
60	15.238	2347	2354	2362	rVV5	10765	22317	2.26%	0.321%


Sum of corrected areas: 6950923

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100819\
Data File : VX012912.D
Acq On : 09 Oct 2019 01:12
Operator : JC/SP
Sample : K5190-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW1011-20191002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

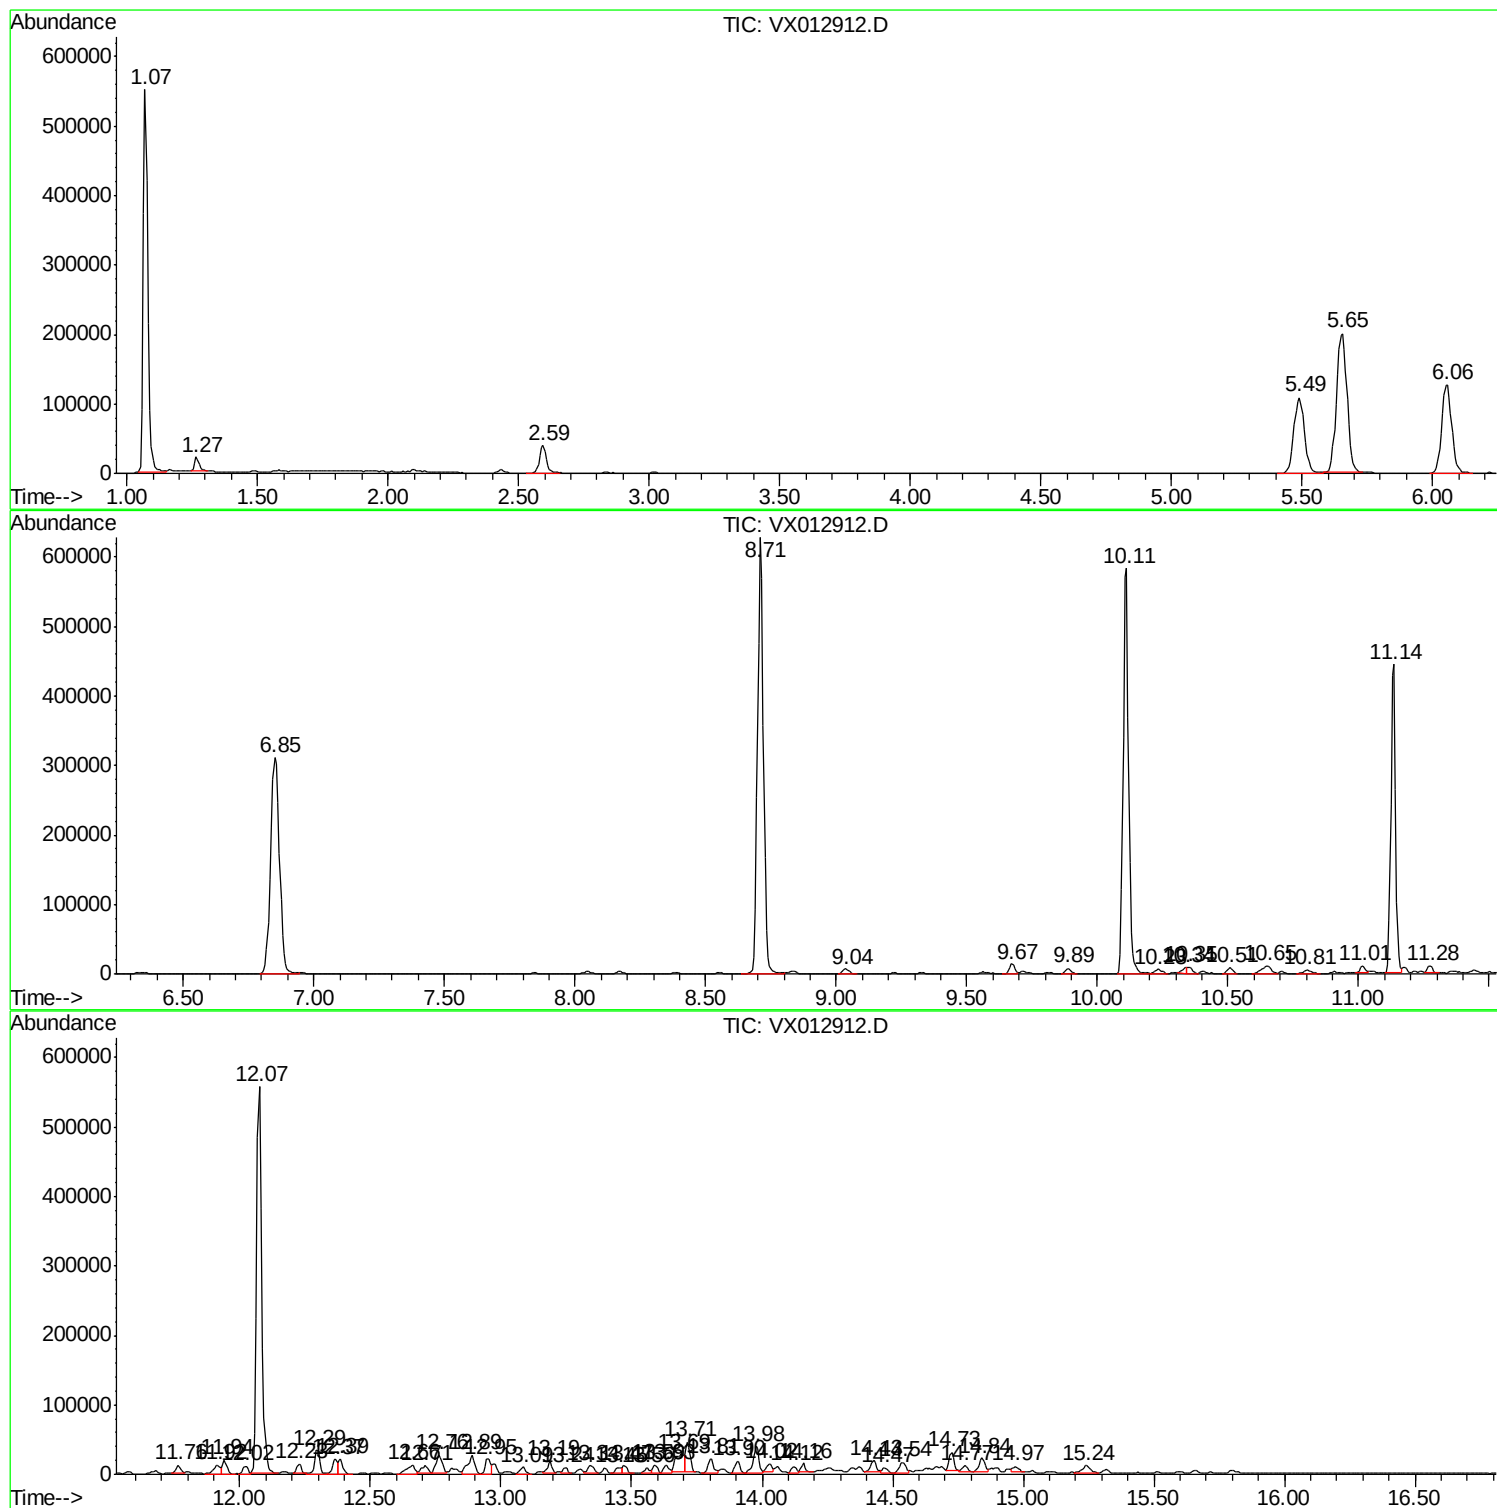

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX100819\
Data File : VX012912.D
Acq On : 09 Oct 2019 01:12
Operator : JC/SP
Sample : K5190-11
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW1011-20191002










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	6.56 ug/l	73562	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		Formamide	45	CH3NO	000075-12-7	5
4		Ethylamine	45	C2H7N	000075-04-7	5
5		2-Butanol	74	C4H10O	000078-92-2	4

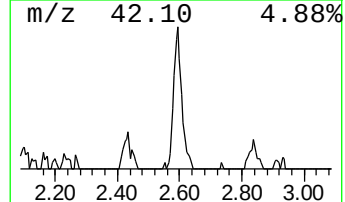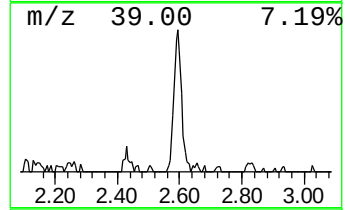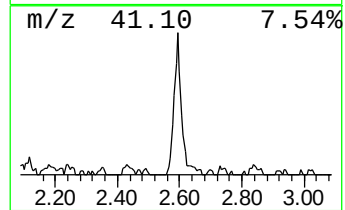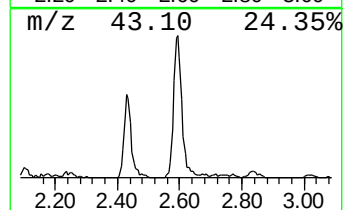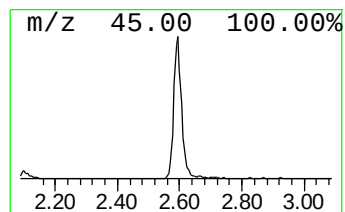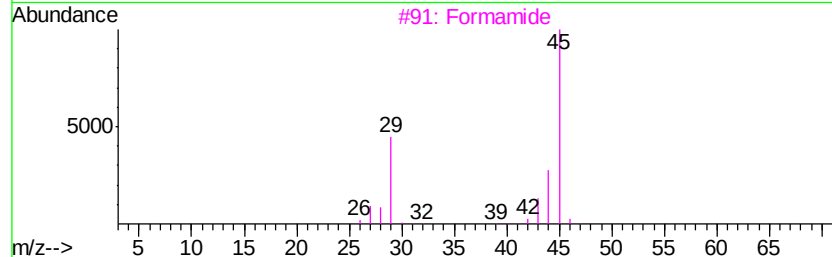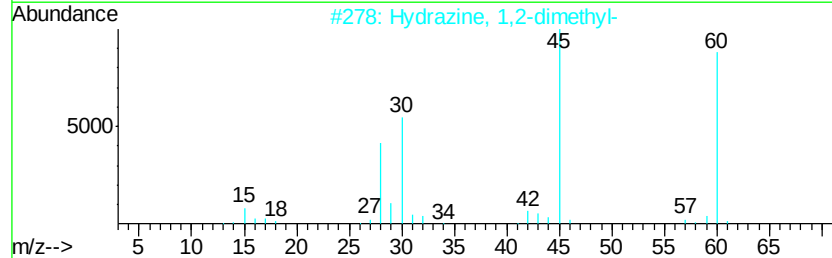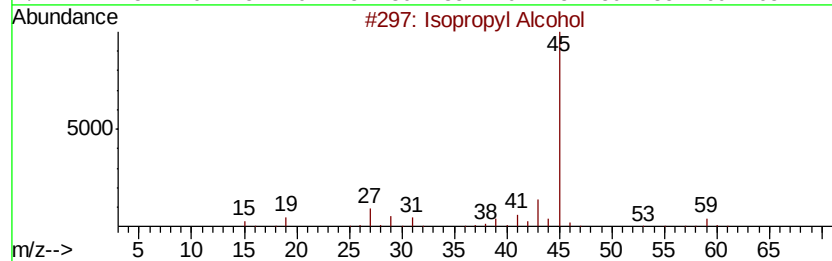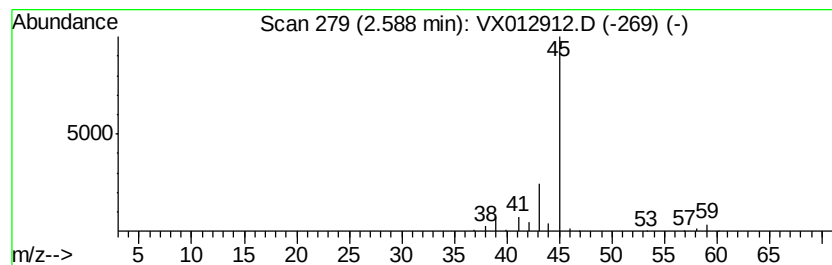

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX100819\
Data File : VX012912.D
Acq On : 09 Oct 2019 01:12
Operator : JC/SP
Sample : K5190-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FC-MW1011-20191002

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	6.6	ug/l	73562	1	5.65	560654	50.0