


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX100819\
Data File : VX012903.D
Acq On : 08 Oct 2019 20:56
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X100819W.M
Title : SW846 8260
Last Update : Wed Oct 09 01:51:23 2019

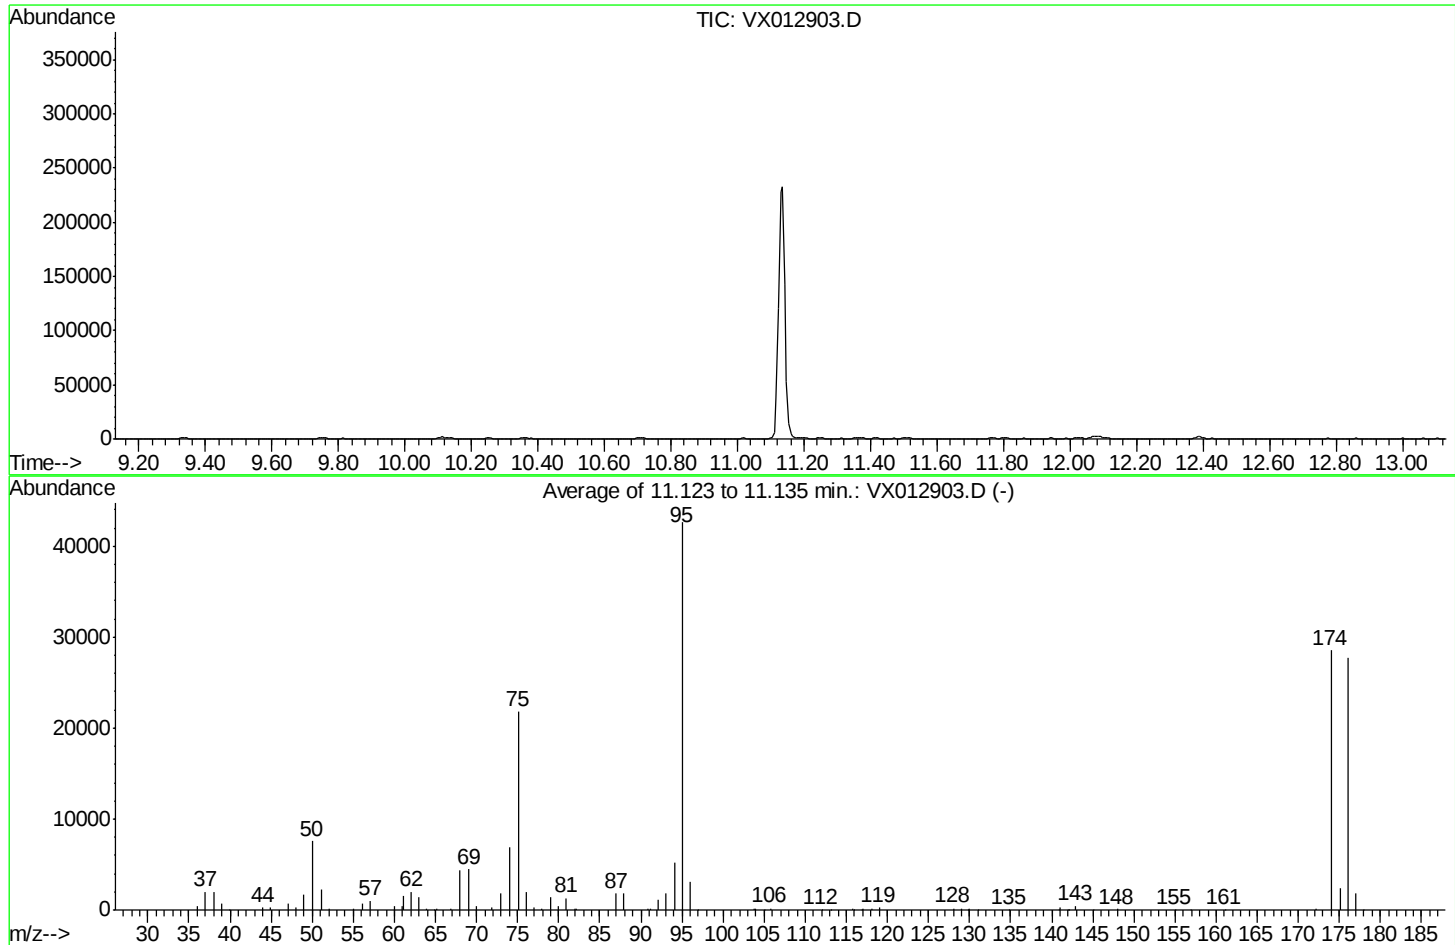

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7548	PASS
75	95	30	60	51.0	21750	PASS
95	95	100	100	100.0	42616	PASS
96	95	5	9	7.3	3132	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.9	28509	PASS
175	174	5	9	8.3	2363	PASS
176	174	95	101	97.3	27729	PASS
177	176	5	9	6.5	1812	PASS